


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA F\Data\BF121417\
Data File : BF101423.D
Acq On : 15 Dec 2017 5:10
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Dec 14 15:42:32 2017

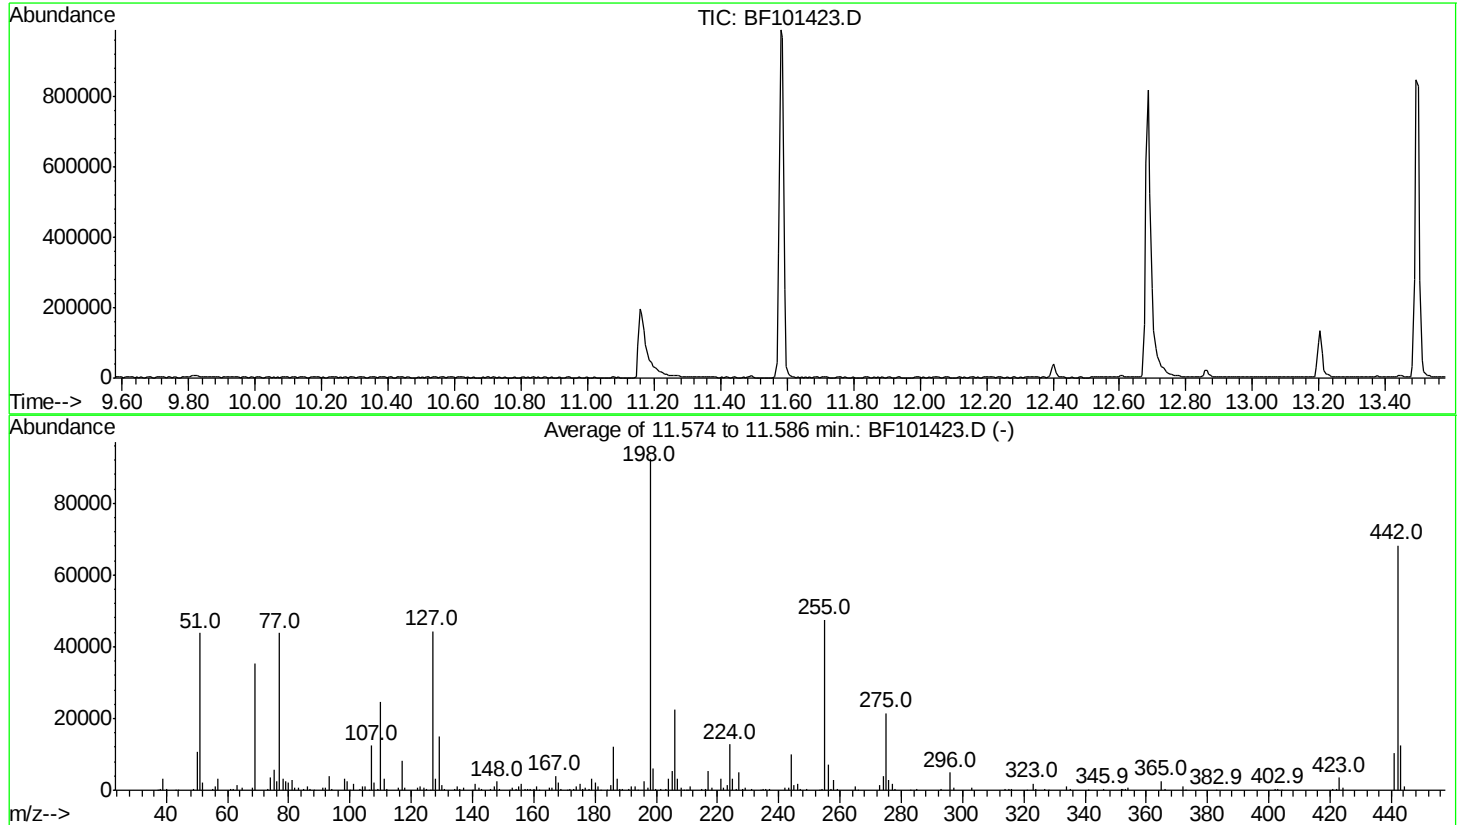

AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.4	43768	PASS
68	69	0.00	2	1.6	574	PASS
69	198	0.00	100	38.4	35440	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.9	44296	PASS
197	198	0.00	2	0.9	808	PASS
198	198	100	100	100.0	92400	PASS
199	198	5	9	6.5	5994	PASS
275	198	10	60	23.3	21528	PASS
365	198	1	100	2.7	2522	PASS
441	443	0.01	100	81.8	10352	PASS
442	198	50	100	73.9	68242	PASS
443	442	15	24	18.5	12658	PASS