
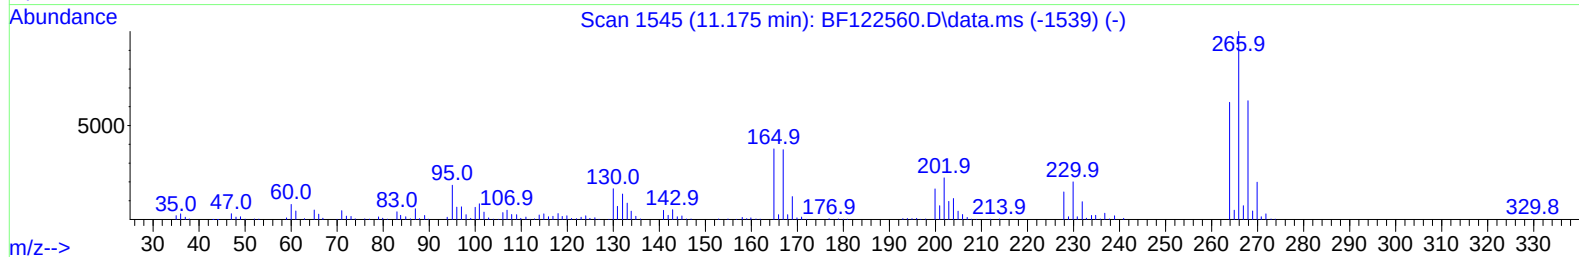
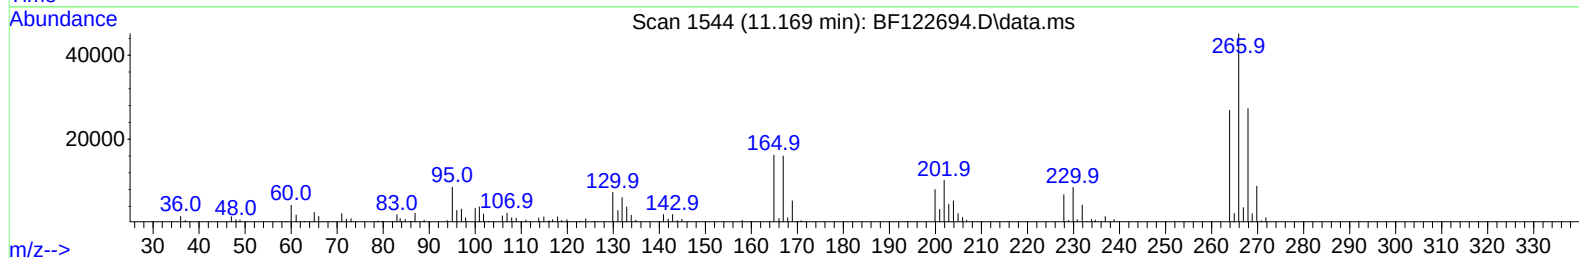


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121420\
Data File : BF122694.D
Acq On : 14 Dec 2020 8:38
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 15 08:01:54 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 07 12:08:49 2020
Response via : Initial Calibration

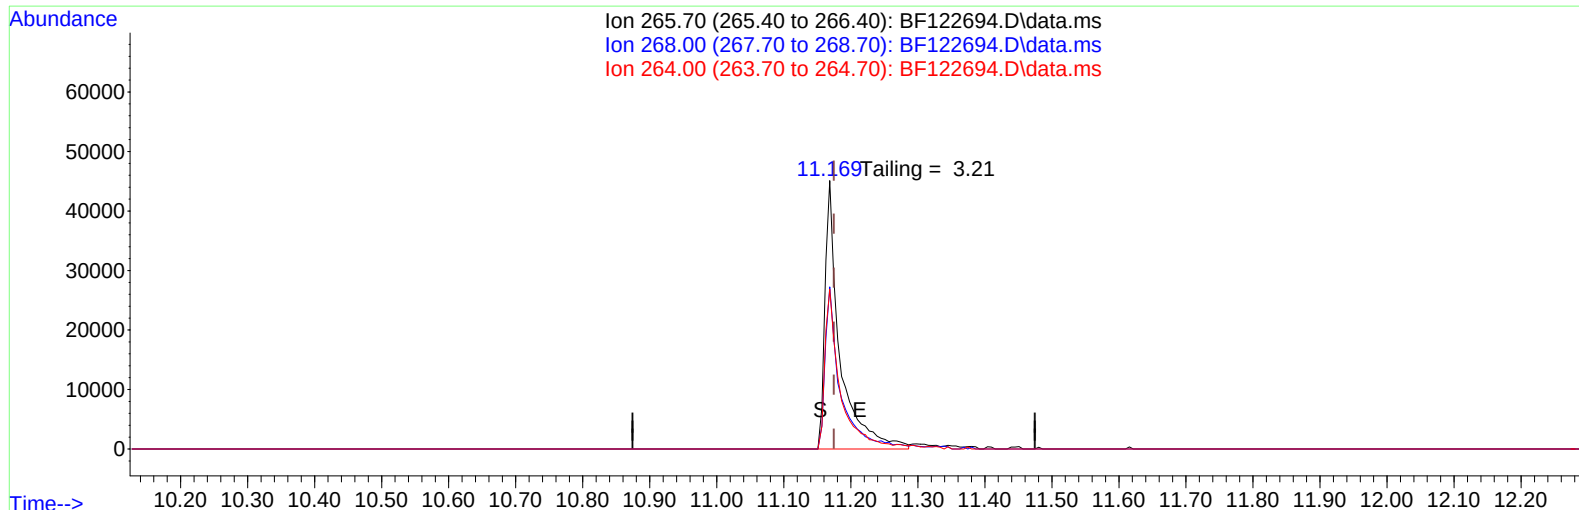

TIC: BF122694.D\data.ms

(70) Pentachlorophenol (C)




11.169min (-0.006) 31106.15 ng

response 70361

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	60.43
264.00	62.30	59.51
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121420\
Data File : BF122694.D
Acq On : 14 Dec 2020 8:38
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 15 08:01:54 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 07 12:08:49 2020
Response via : Initial Calibration

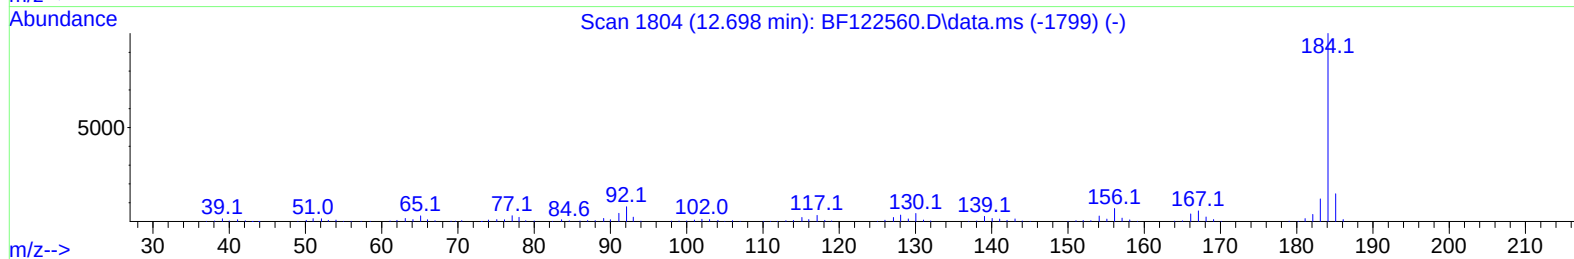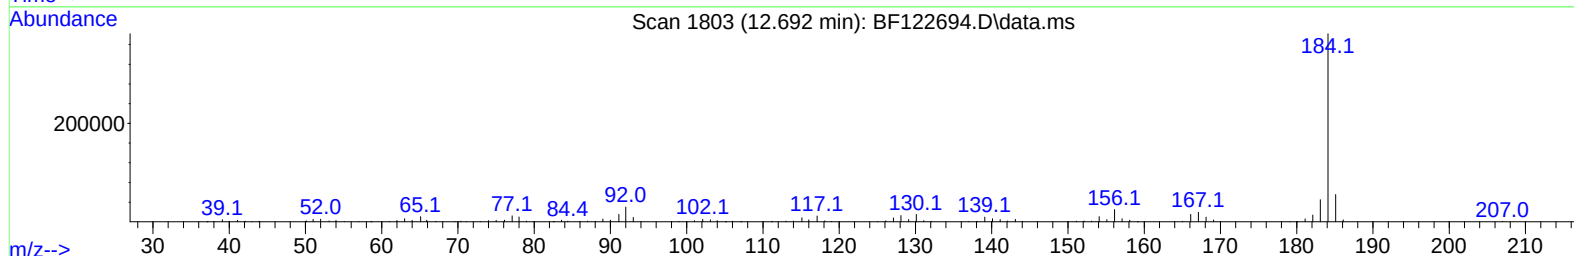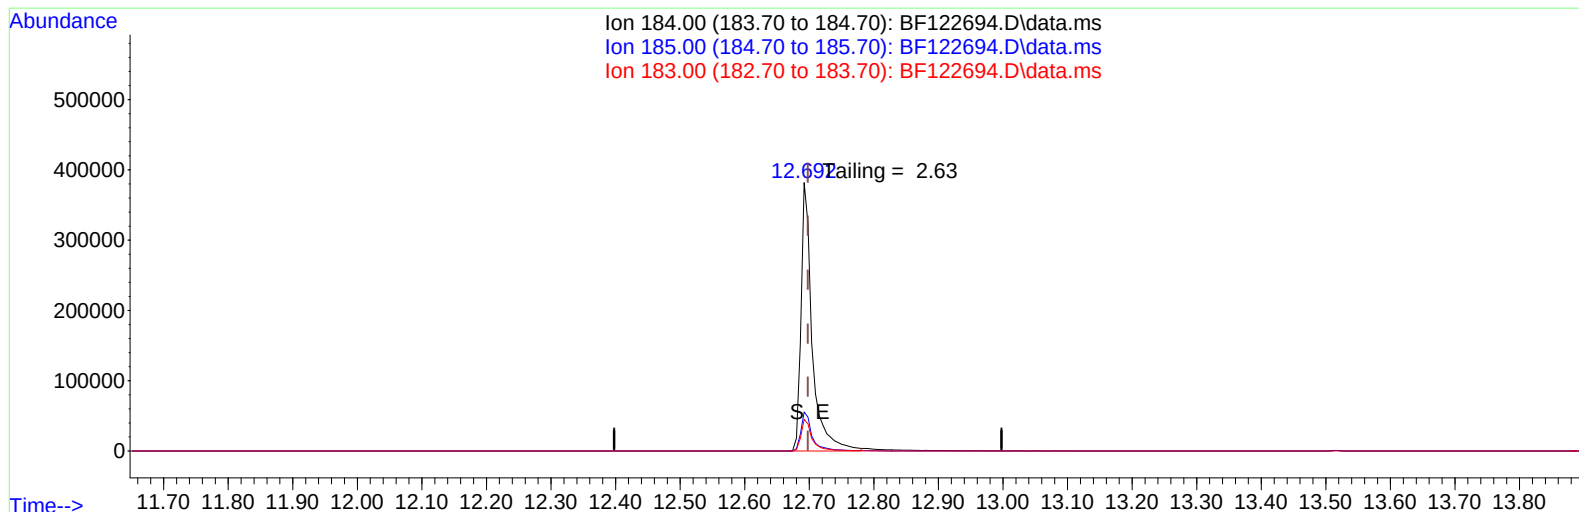

TIC: BF122694.D\data.ms

(77) Benzidine

12.692min (-0.006) 0.00 ng

response 471860

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.55
183.00	12.10	11.82
0.00	0.00	0.00