

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121420\
 Data File : BF122713.D
 Acq On : 14 Dec 2020 18:58
 Operator : JU/CG
 Sample : L5047-01 2X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OK-03-121120

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF122713.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.445	567	571	594	rBV	994148	1037985	66.95%	6.847%
2	6.463	740	744	763	rBV	1104091	1222640	78.86%	8.065%
3	6.833	804	807	814	rBV	1127938	937490	60.47%	6.184%
4	7.392	899	902	914	rBV	609541	635862	41.01%	4.195%
5	8.122	1022	1026	1032	rBV	1321316	1218636	78.60%	8.039%
6	9.192	1204	1208	1219	rBV	1751225	1550392	100.00%	10.227%
7	9.274	1219	1222	1225	rVV4	17730	18591	1.20%	0.123%
8	9.592	1272	1276	1280	rBV2	69395	90827	5.86%	0.599%
9	9.874	1320	1324	1328	rBV	1738443	1432620	92.40%	9.451%
10	9.904	1328	1329	1338	rVB	50174	51037	3.29%	0.337%
11	10.080	1356	1359	1363	rVB2	16737	20491	1.32%	0.135%
12	10.421	1414	1417	1424	rBV	33919	38600	2.49%	0.255%
13	10.527	1430	1435	1437	rBV5	17677	20421	1.32%	0.135%
14	10.663	1454	1458	1469	rBV	592120	627255	40.46%	4.138%
15	10.792	1475	1480	1483	rBV	33449	45415	2.93%	0.300%
16	10.863	1487	1492	1496	rBV7	11145	19516	1.26%	0.129%
17	11.221	1549	1553	1555	rBV4	20695	23608	1.52%	0.156%
18	11.257	1556	1559	1564	rVB	40889	45622	2.94%	0.301%
19	11.357	1573	1576	1579	rBV	1355676	1348304	86.97%	8.894%
20	11.380	1579	1580	1584	rVV	299511	244054	15.74%	1.610%
21	11.433	1587	1589	1594	rVB	39585	40292	2.60%	0.266%
22	11.598	1613	1617	1623	rBV	32101	49525	3.19%	0.327%
23	11.863	1659	1662	1664	rBV	16930	18561	1.20%	0.122%
24	11.892	1664	1667	1673	rVV3	42418	50392	3.25%	0.332%
25	11.974	1678	1681	1683	rVV	33967	29344	1.89%	0.194%
26	12.157	1710	1712	1715	rBV2	18104	18807	1.21%	0.124%
27	12.339	1740	1743	1745	rBV3	16987	19737	1.27%	0.130%
28	12.410	1752	1755	1757	rBV2	26707	26385	1.70%	0.174%
29	12.439	1757	1760	1762	rBV4	28270	36520	2.36%	0.241%
30	12.574	1780	1783	1787	rBV	202675	181266	11.69%	1.196%
31	12.674	1798	1800	1804	rBV5	17415	19355	1.25%	0.128%
32	12.727	1806	1809	1812	rBV5	16156	22679	1.46%	0.150%
33	12.804	1817	1822	1829	rBV	154325	230377	14.86%	1.520%
34	12.945	1842	1846	1849	rBV	1526558	1408170	90.83%	9.289%
35	13.127	1875	1877	1880	rBV	33333	31633	2.04%	0.209%
36	13.998	2021	2025	2029	rBV	1112266	1159163	74.77%	7.647%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121420\
Data File : BF122713.D
Acq On : 14 Dec 2020 18:58
Operator : JU/CG
Sample : L5047-01 2X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-03-121120

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37 15.468 2270 2275 2283 rVB 884949 1187537 76.60% 7.834%




Sum of corrected areas: 15159109

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121420\
Data File : BF122713.D
Acq On : 14 Dec 2020 18:58
Operator : JU/CG
Sample : L5047-01 2X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-03-121120

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

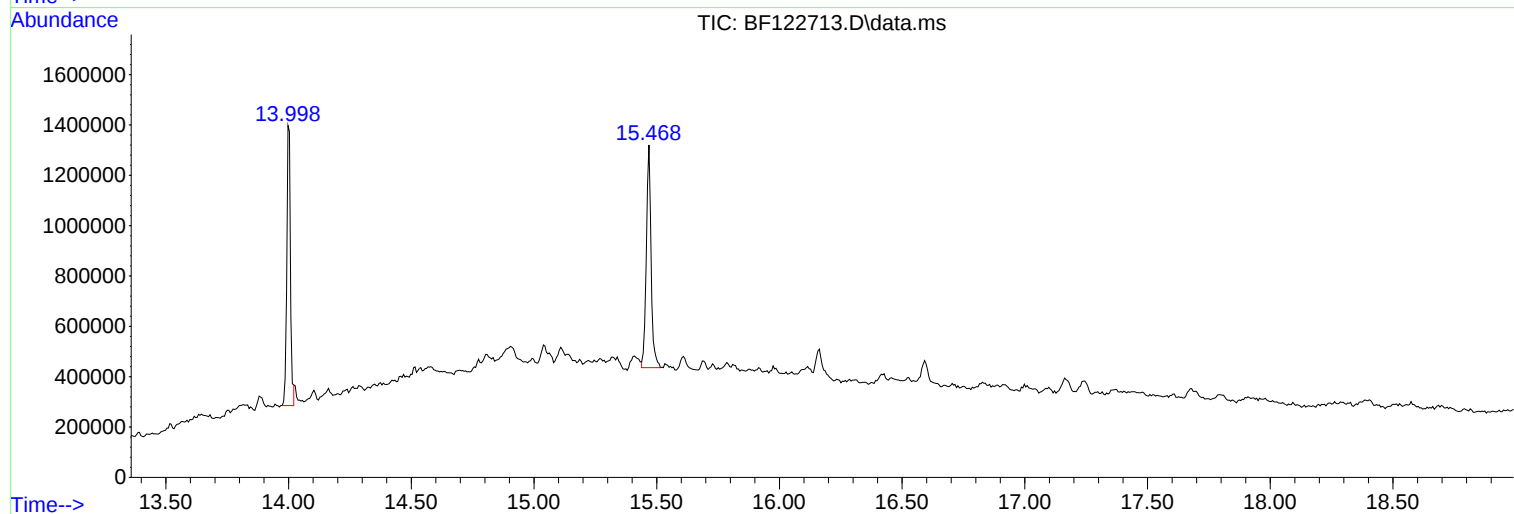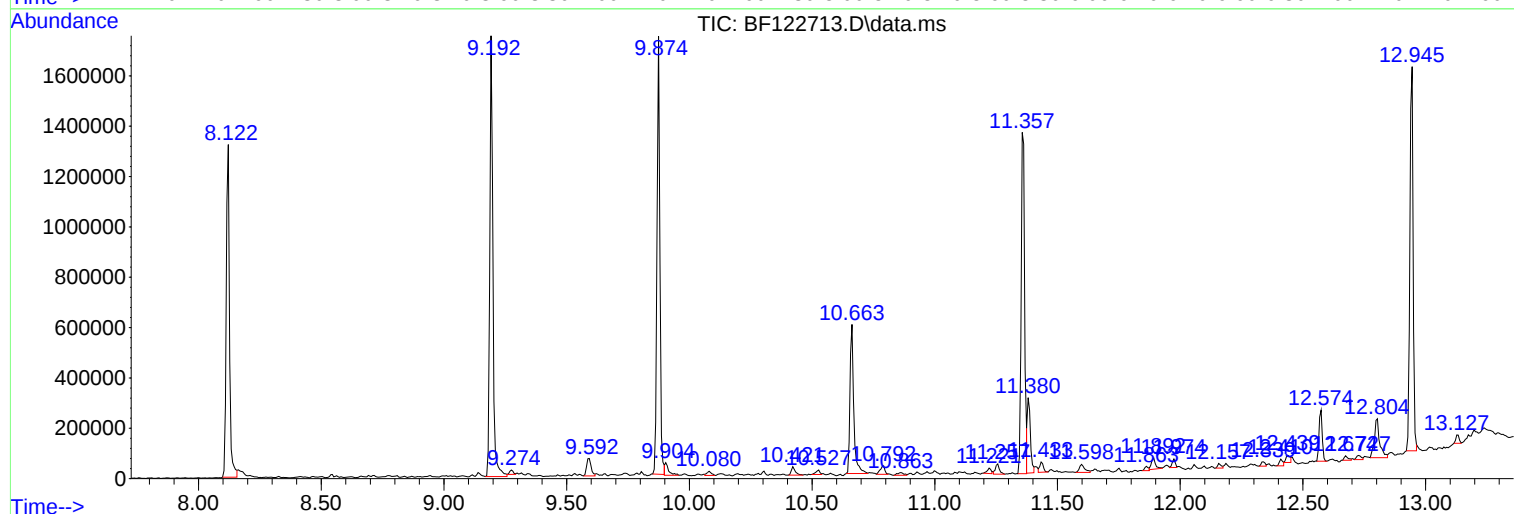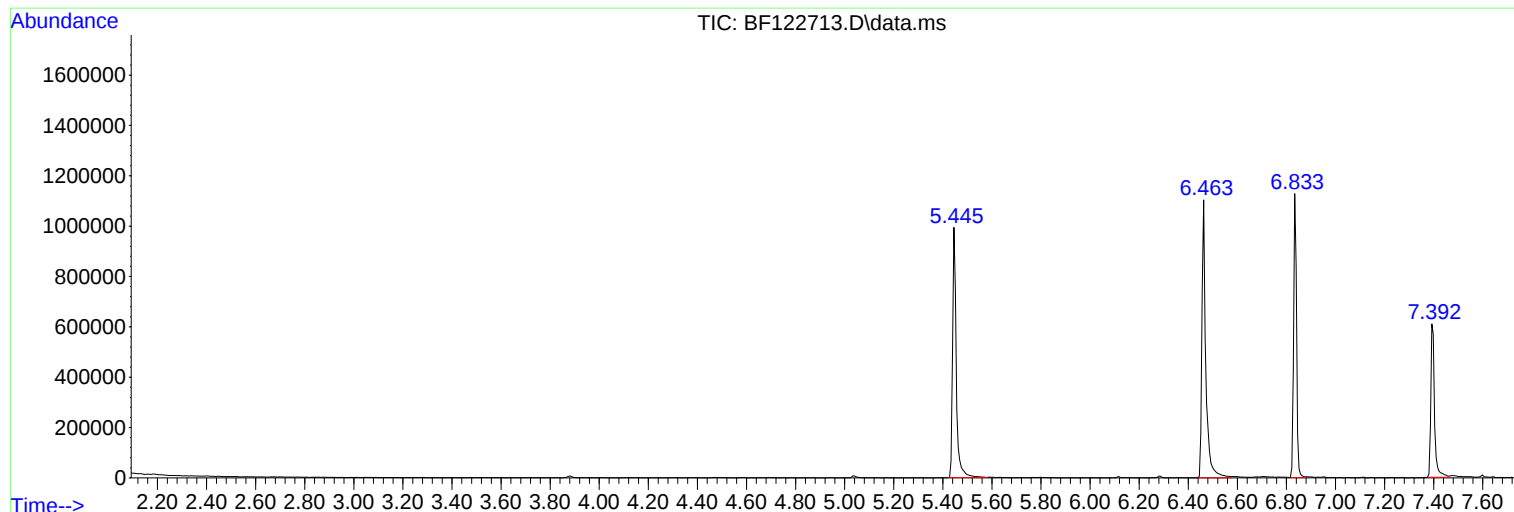

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121420\
Data File : BF122713.D
Acq On : 14 Dec 2020 18:58
Operator : JU/CG
Sample : L5047-01 2X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-03-121120

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121420\
Data File : BF122713.D
Acq On : 14 Dec 2020 18:58
Operator : JU/CG
Sample : L5047-01 2X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-03-121120

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------