
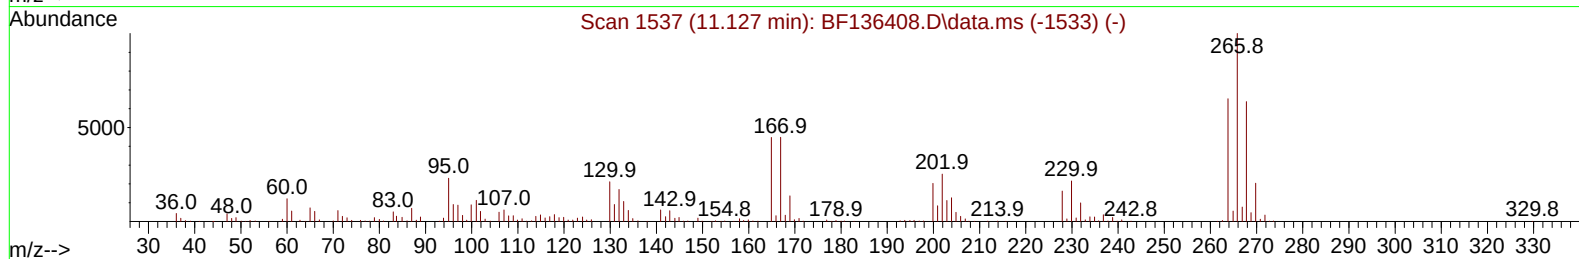
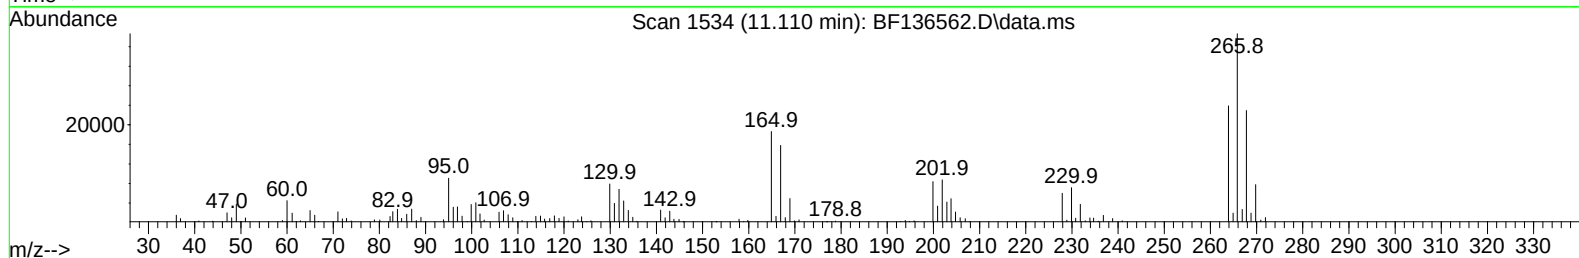


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121423\
Data File : BF136562.D
Acq On : 14 Dec 2023 11:17
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 14 13:01:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 06 09:40:27 2023
Response via : Initial Calibration

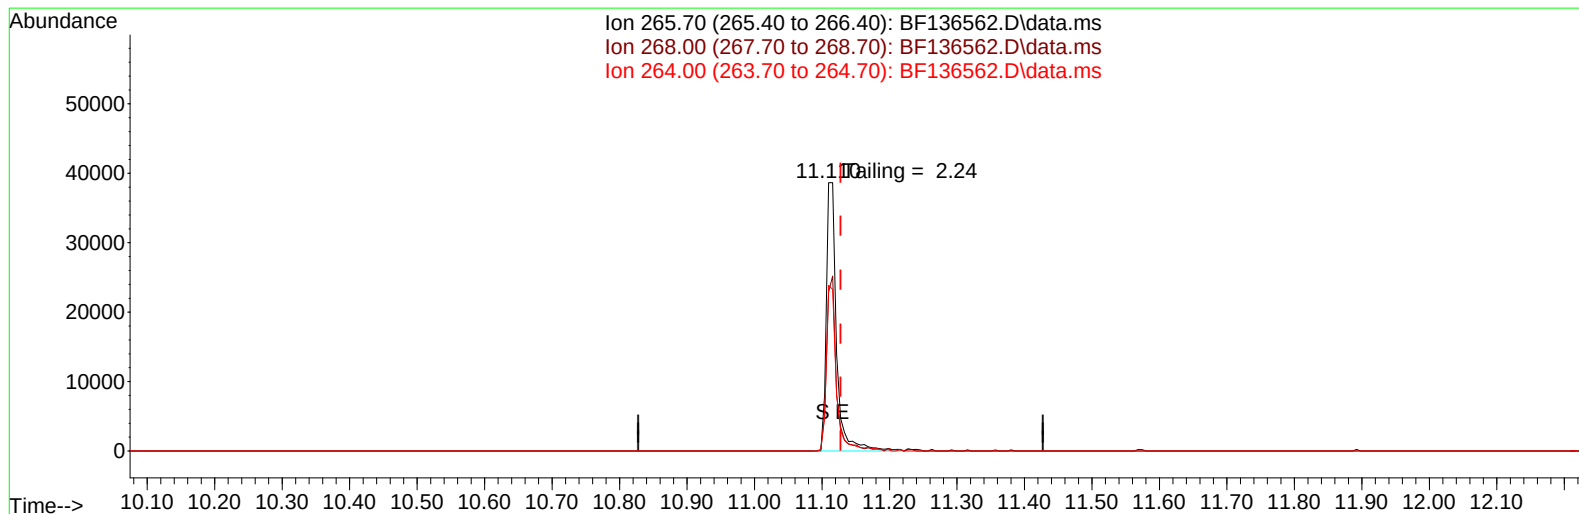

TIC: BF136562.D\data.ms

(70) Pentachlorophenol (C)




11.110min (-0.018) 14880.04 ng

response 40739

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	59.29
264.00	65.30	61.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121423\
Data File : BF136562.D
Acq On : 14 Dec 2023 11:17
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 14 13:01:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 06 09:40:27 2023
Response via : Initial Calibration

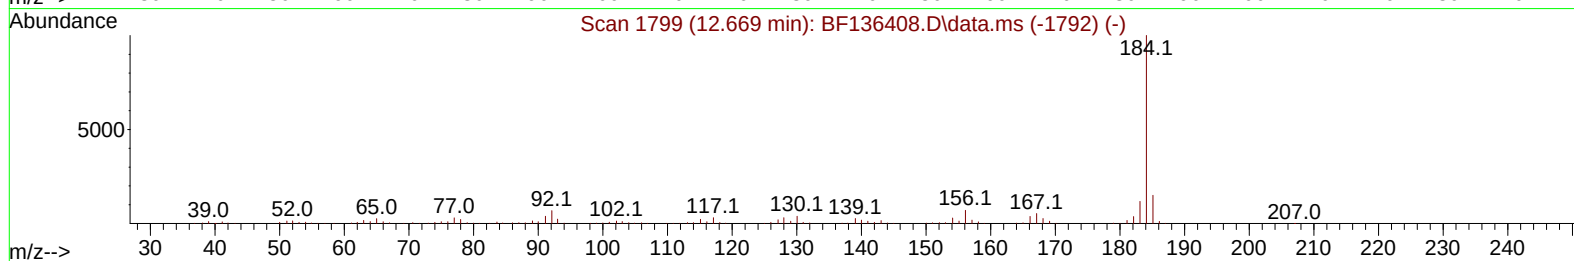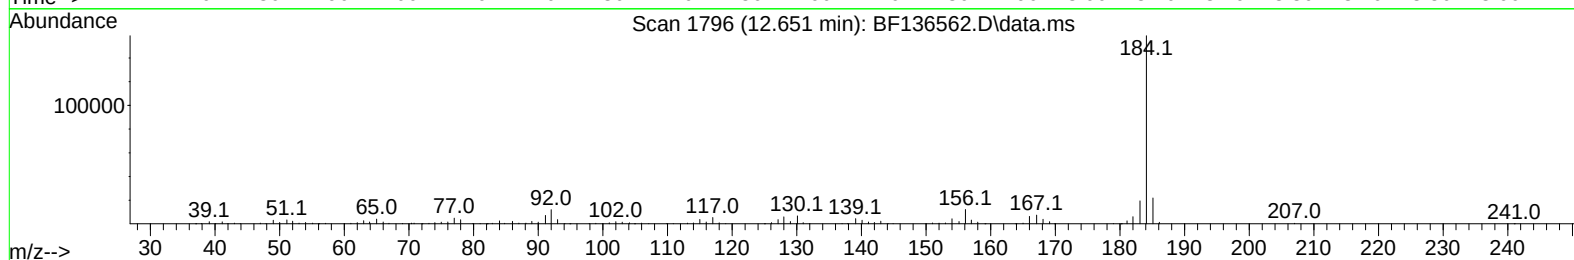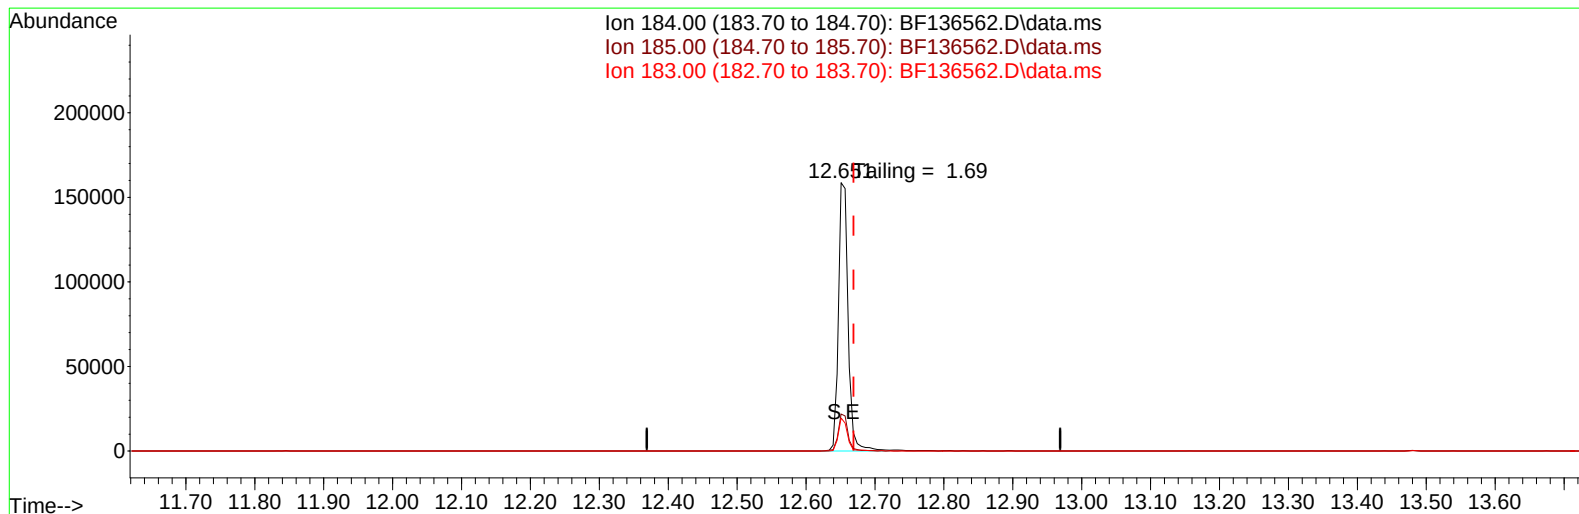

TIC: BF136562.D\data.ms

(77) Benzidine

12.651min (-0.018) 217.03 ng

response 154901

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	13.81
183.00	11.70	12.31
0.00	0.00	0.00