
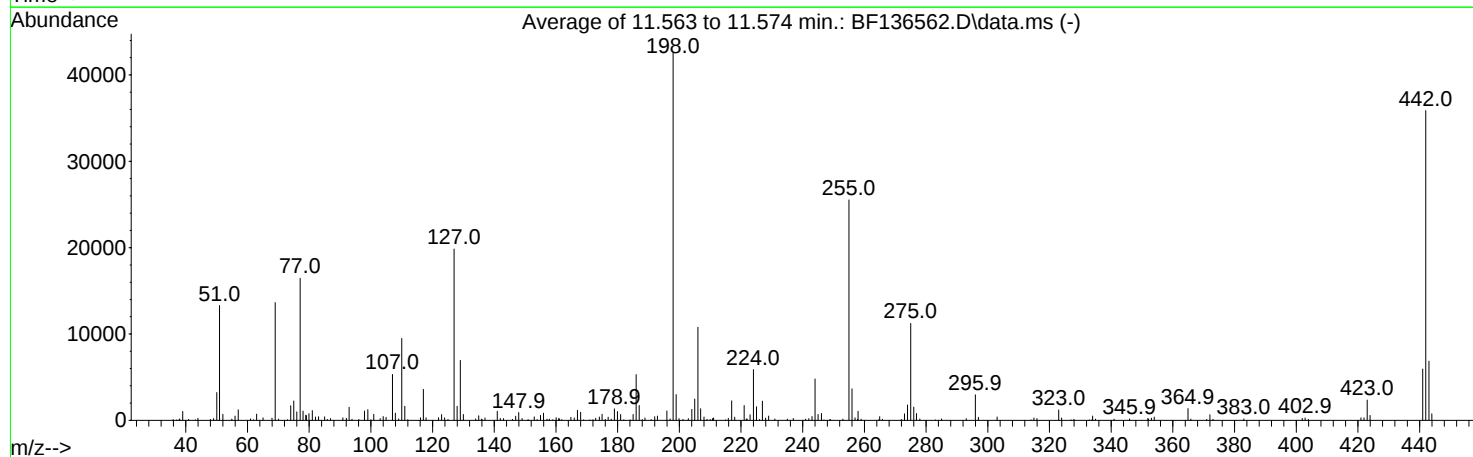


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121423\
Data File : BF136562.D
Acq On : 14 Dec 2023 11:17
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Dec 15 00:33:23 2023

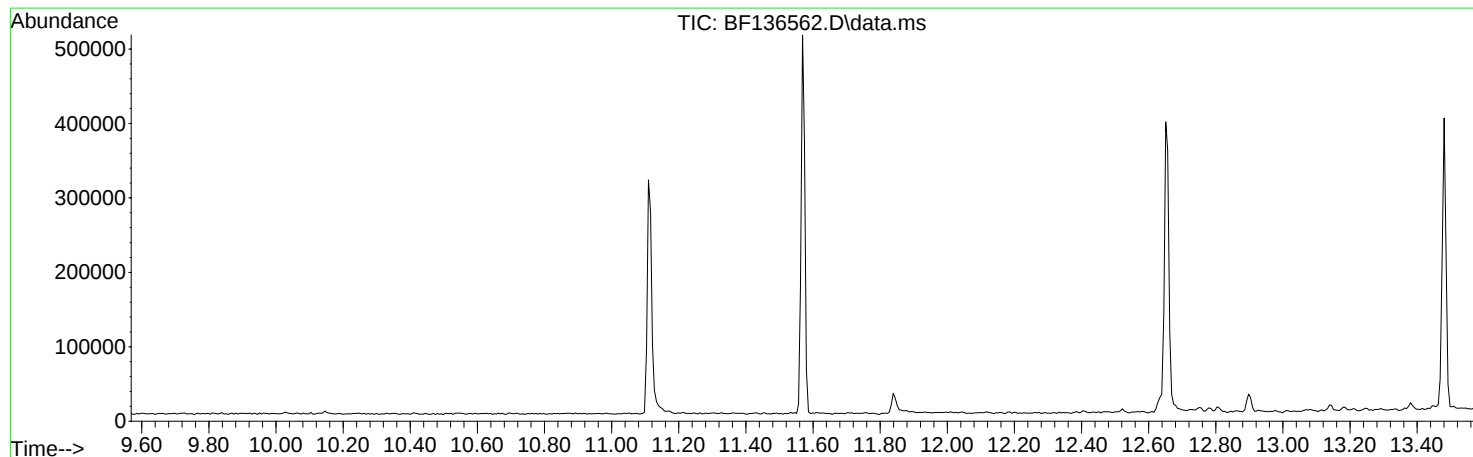




AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1607

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	31.2	13307	PASS
68	69	0.00	2	1.9	265	PASS
69	198	0.00	100	32.0	13645	PASS
70	69	0.00	2	1.1	149	PASS
127	198	10	80	46.6	19842	PASS
197	198	0.00	2	0.4	166	PASS
198	198	100	100	100.0	42603	PASS
199	198	5	9	7.0	2977	PASS
275	198	10	60	26.4	11233	PASS
365	198	1	100	3.2	1366	PASS
441	198	0.01	100	14.0	5950	PASS
442	442	50	100	100.0	35868	PASS
443	442	15	24	19.1	6852	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121423\
Data File : BF136562.D
Acq On : 14 Dec 2023 11:17
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 14 13:01:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 06 09:40:27 2023
Response via : Initial Calibration

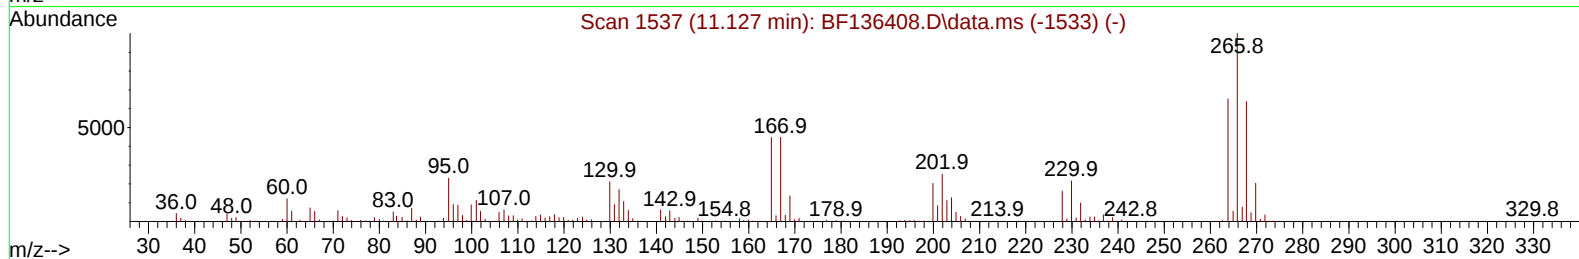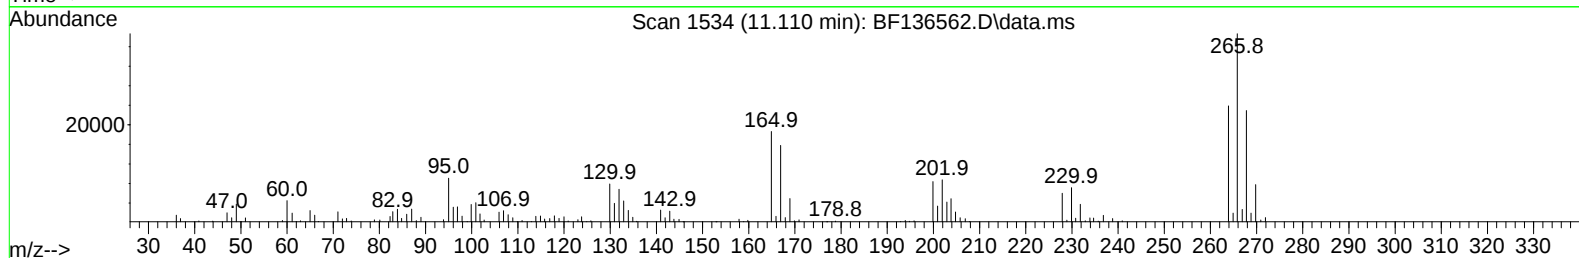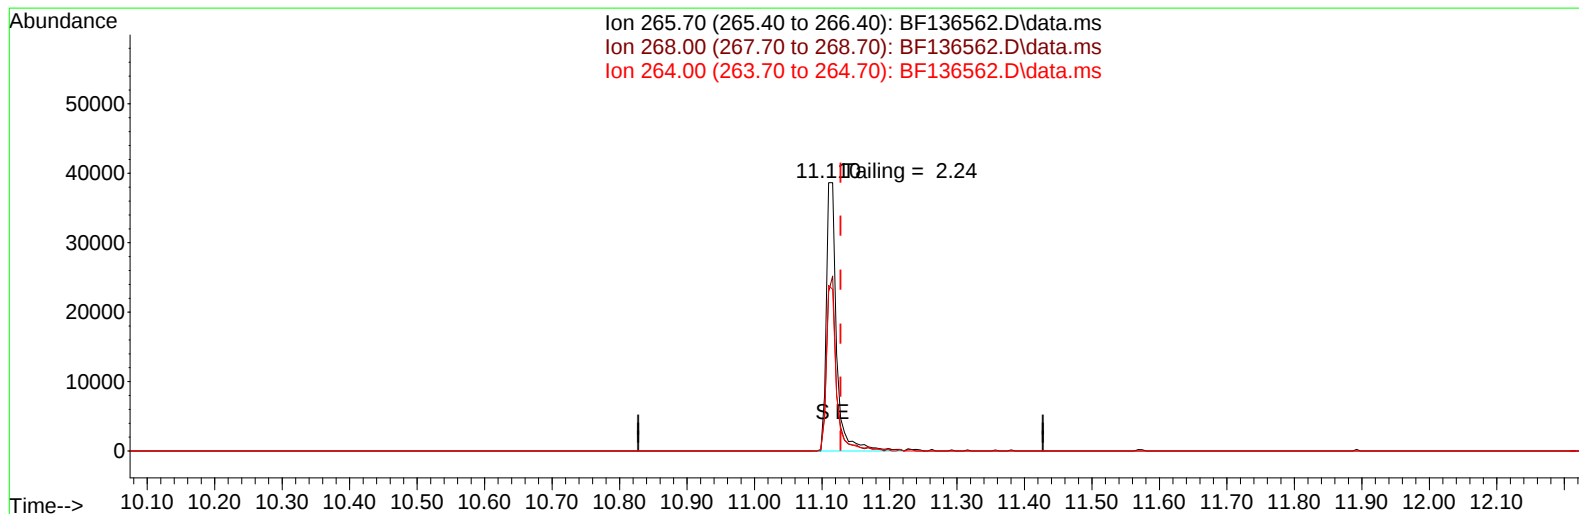

TIC: BF136562.D\data.ms

(70) Pentachlorophenol (C)

11.110min (-0.018) 14880.04 ng




response 40739

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	59.29
264.00	65.30	61.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121423\
Data File : BF136562.D
Acq On : 14 Dec 2023 11:17
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 14 13:01:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 06 09:40:27 2023
Response via : Initial Calibration

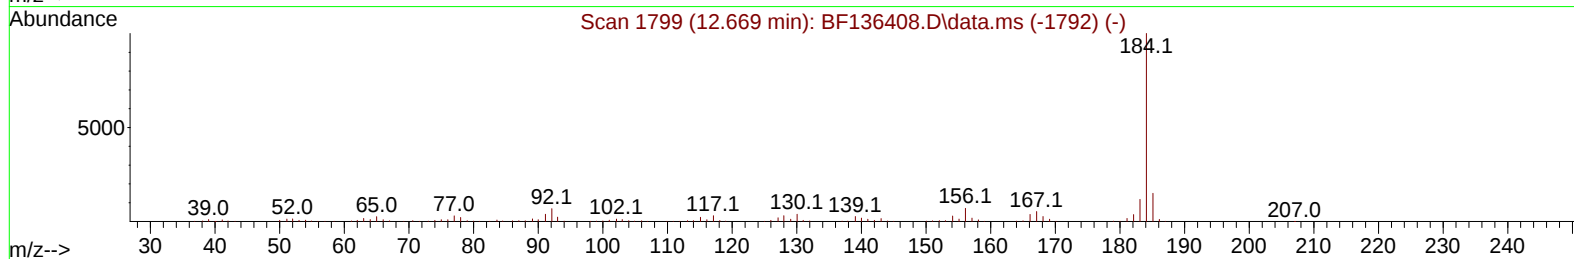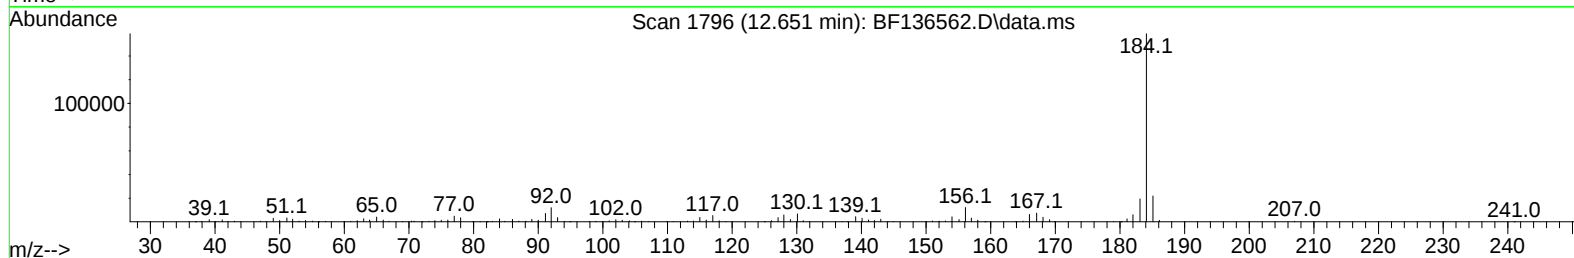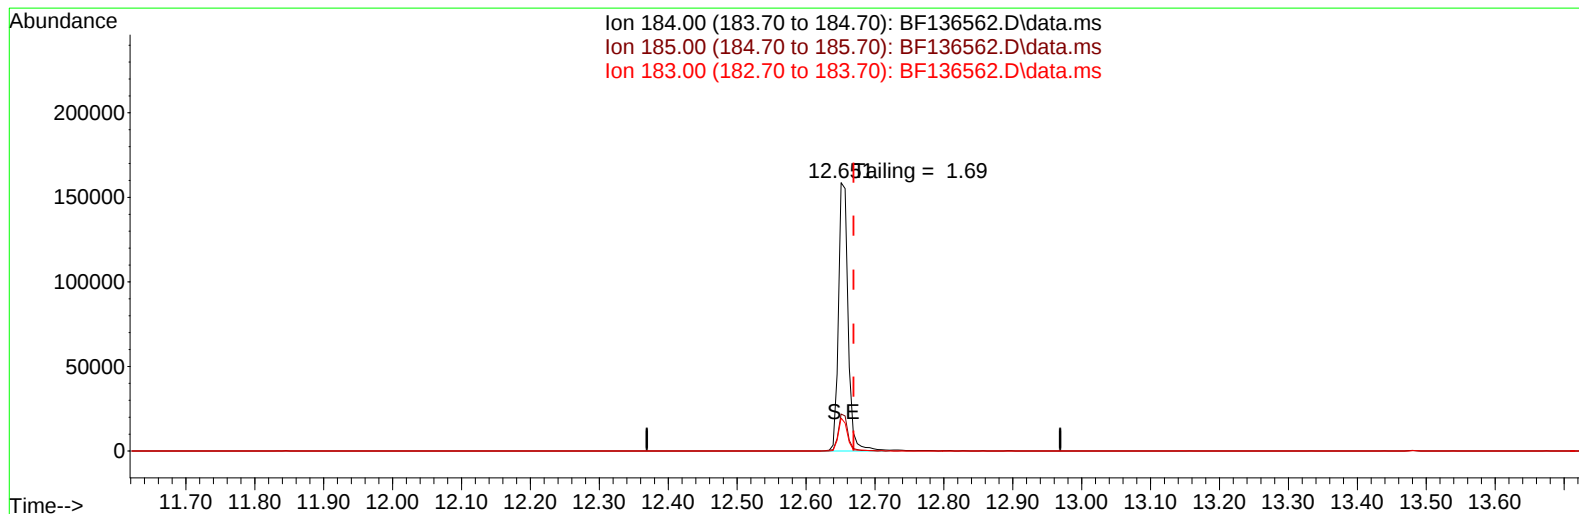

TIC: BF136562.D\data.ms

(77) Benzidine

12.651min (-0.018) 217.03 ng

response 154901

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	13.81
183.00	11.70	12.31
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/14/2023	BNA_F	<u>BF136562.D</u>
Compound Name	Response	Retention Time
DDT	61367	13.48
DDD	1547	13.18
DDE	67	12.898
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1614	62981	2.56

Instrument :
BNA_F
ClientSampleId :
DFTPP