

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF121515\
 Data File : BF083841.D
 Acq On : 16 Dec 2015 4:10
 Operator : UM/IZ
 Sample : G4739-09DL 2X
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 K206-18-19DL

Quant Time: Dec 16 07:34:45 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121315.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 14 01:30:12 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.90	152	91206	20.00	ng	-0.02
21) Naphthalene-d8	8.19	136	347673	20.00	ng	-0.02
38) Acenaphthene-d10	9.94	164	147255	20.00	ng	-0.02
63) Phenanthrene-d10	11.43	188	239610	20.00	ng	-0.02
75) Chrysene-d12	14.05	240	192046	20.00	ng	-0.02
86) Perylene-d12	15.49	264	147175	20.00	ng	-0.01

System Monitoring Compounds						
5) 2-Fluorophenol	5.50	112	340933	60.30	ng	-0.02
7) Phenol-d6	6.53	99	489075	68.31	ng	-0.01
23) Nitrobenzene-d5	7.46	82	257648	41.46	ng	-0.02
41) 2,4,6-Tribromophenol	10.73	330	86957	57.95	ng	-0.02
44) 2-Fluorobiphenyl	9.26	172	490167	42.54	ng	-0.02
78) Terphenyl-d14	13.00	244	336154	37.65	ng	-0.02


Target Compounds				Qvalue		
9) Benzaldehyde	6.67	77	8537	2.22	ng	95
19) n-Nitroso-di-n-propylamine	7.46	70	35326	8.06	ng	# 71
25) Isophorone	7.46	82	222362	18.24	ng	# 69
48) Acenaphthylene	9.80	152	99830	6.16	ng	99
49) Dimethylphthalate	9.65	163	73398	6.39	ng	99
51) Acenaphthene	9.97	154	30780	3.14	ng	99
54) Dibenzofuran	10.14	168	26103	2.01	ng	# 91
57) Fluorene	10.49	166	58016	5.67	ng	96
66) 4-Bromophenyl-phenylether	10.73	248	5779	2.16	ng	# 1
70) Phenanthrene	11.45	178	467217	36.71	ng	99
71) Anthracene	11.49	178	204495	15.47	ng	99
74) Fluoranthene	12.64	202	706799	53.74	ng	97
77) Pyrene	12.87	202	784219	51.67	ng	98
80) Benzo(a)anthracene	14.04	228	327972	30.03	ng	# 90
82) Chrysene	14.04	228	327972	30.79	ng	94
85) Indeno(1,2,3-cd)pyrene	16.92	276	71751	6.86	ng	# 100
87) Benzo(b)fluoranthene	15.08	252	280777	29.90	ng	# 97
88) Benzo(k)fluoranthene	15.08	252	280777	33.00	ng	98
89) Benzo(a)pyrene	15.44	252	179004	21.36	ng	99
91) Benzo(g,h,i)perylene	17.36	276	74408	8.69	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF121515\
Data File : BF083841.D
Acq On : 16 Dec 2015 4:10
Operator : UM/IZ
Sample : G4739-09DL 2X
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
K206-18-19DL

Quant Time: Dec 16 07:34:45 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 14 01:30:12 2015
Response via : Initial Calibration

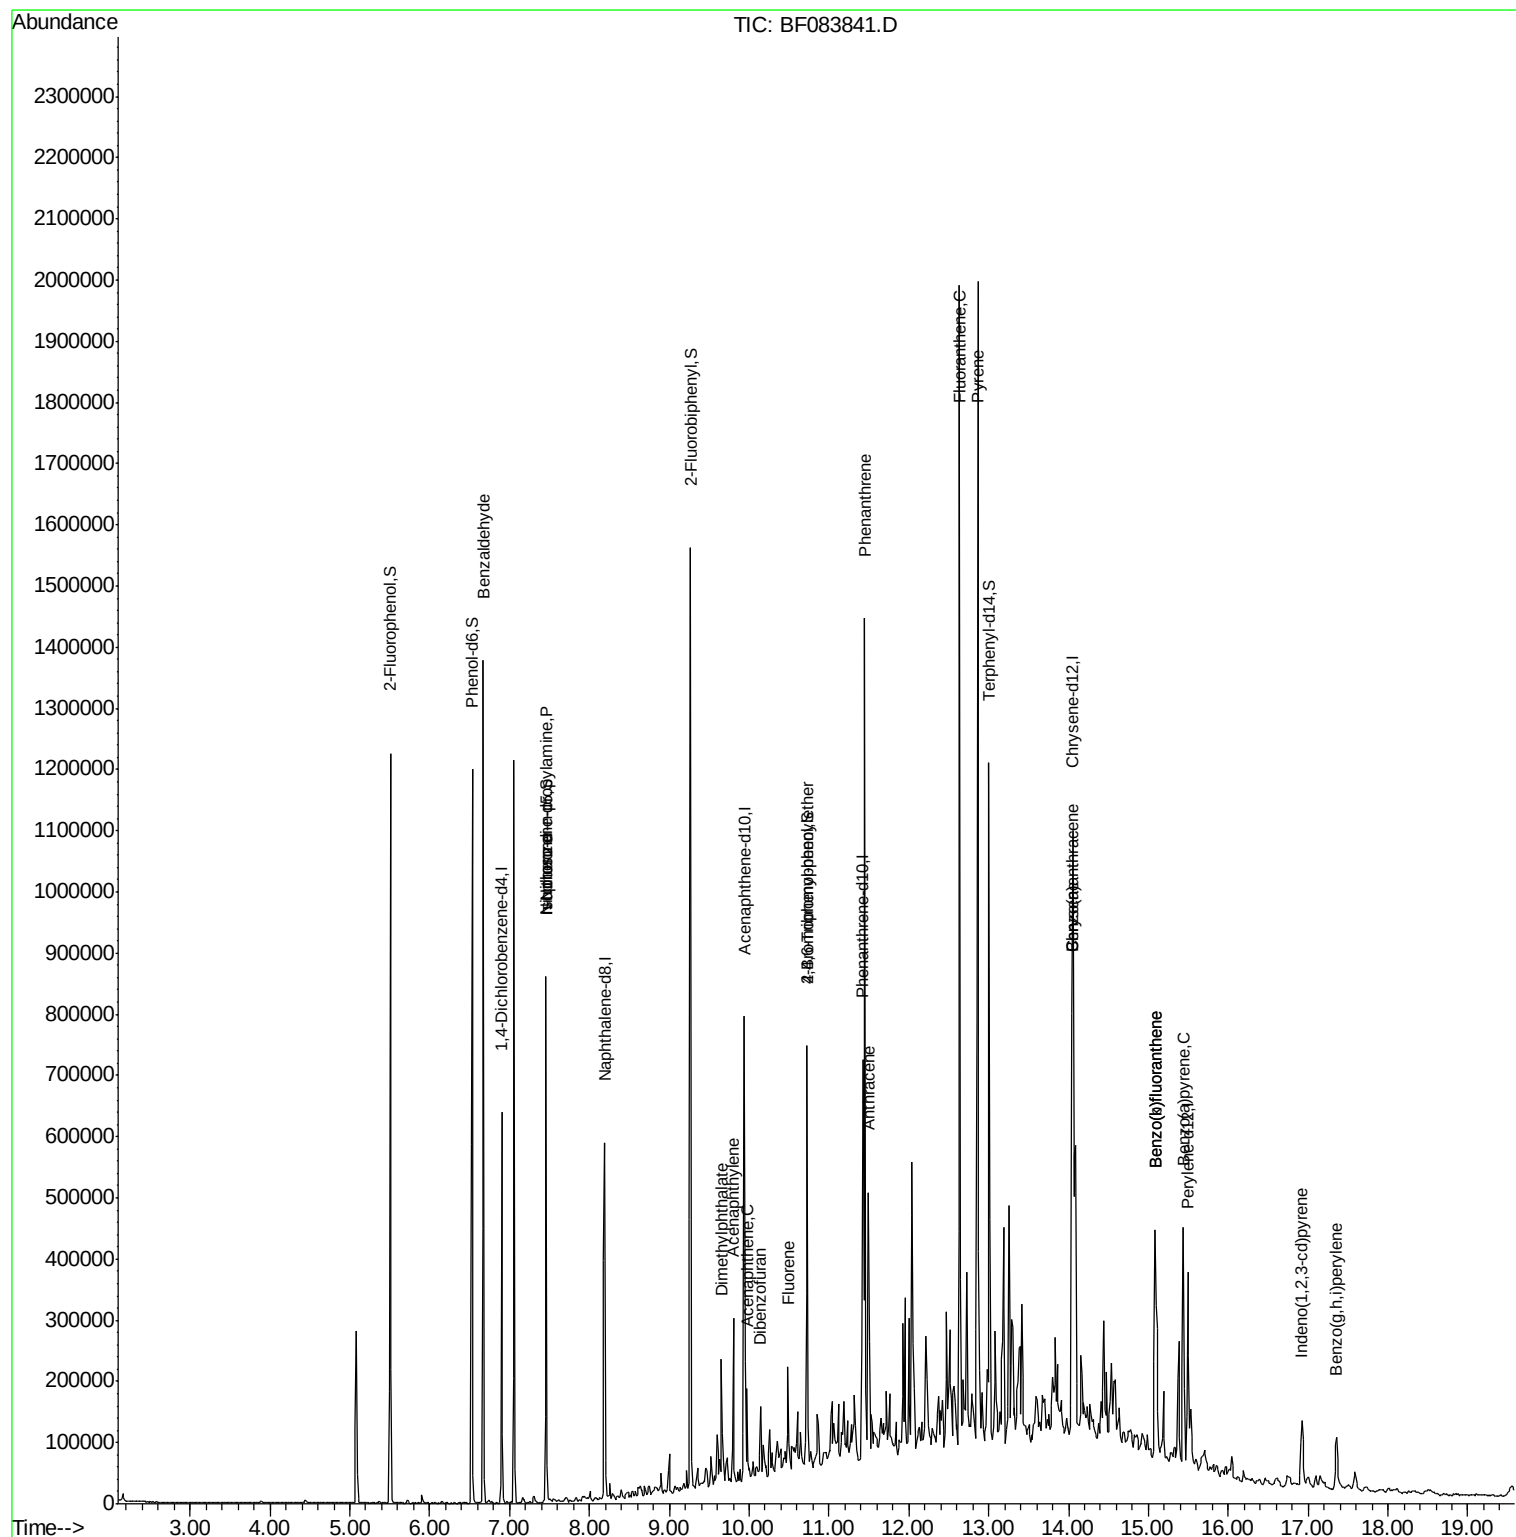



#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.90 min Scan# 421

Delta R.T. -0.02 min

Lab File: BF083841.D

Acq: 16 Dec 2015 4:10

Instrument :

BNA_F

ClientSampleId :

K206-18-19DL


Tgt Ion:152 Resp: 91206

Ion Ratio Lower Upper

152 100

150 156.1 126.5 189.7




115 68.2 52.3 78.5



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

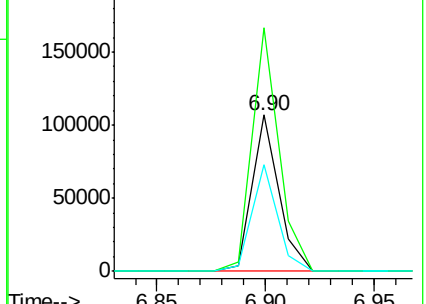

#5

2-Fluorophenol

Concen: 60.30 ng

RT: 5.50 min Scan# 299

Delta R.T. -0.02 min

Lab File: BF083841.D

Acq: 16 Dec 2015 4:10


Tgt Ion:112 Resp: 340933

Ion Ratio Lower Upper

112 100

64 57.0 50.5 75.7



63 29.9 25.8 38.6




Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

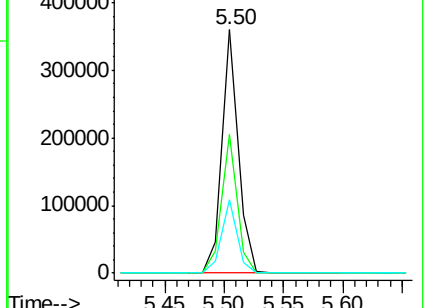



#7

Phenol-d6

Concen: 68.31 ng

RT: 6.53 min Scan# 389

Delta R.T. -0.01 min

Lab File: BF083841.D

Acq: 16 Dec 2015 4:10

Instrument :

BNA_F

ClientSampleId :

K206-18-19DL


Tgt Ion: 99 Resp: 489075

Ion Ratio Lower Upper

99 100

42 13.0 17.3 25.9#




71 32.6 26.6 40.0

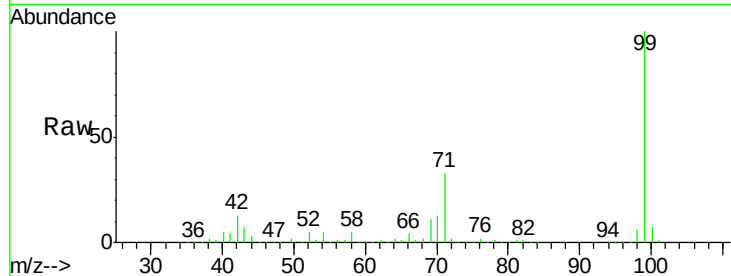

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

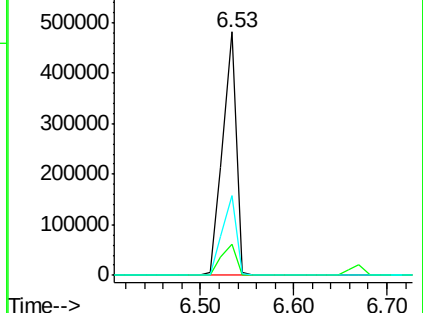

#9

Benzaldehyde

Concen: 2.22 ng

RT: 6.67 min Scan# 401

Delta R.T. 0.21 min

Lab File: BF083841.D

Acq: 16 Dec 2015 4:10


Tgt Ion: 77 Resp: 8537

Ion Ratio Lower Upper

77 100

105 85.7 71.8 111.8



106 83.4 66.8 106.8




Abundance Ion 77.00 (76.70 to 77.70): BF0

Ion 105.00 (104.70 to 105.70): E

Ion 106.00 (105.70 to 106.70): E



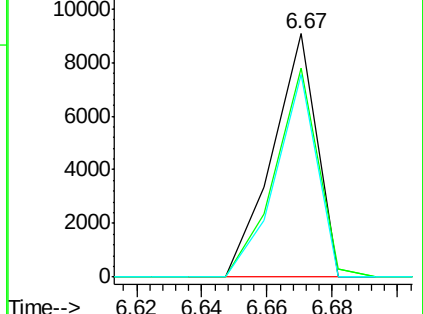





#19
n-Nitroso-di-n-propylamine
Concen: 8.06 ng
RT: 7.46 min Scan# 470
Delta R.T. 0.11 min
Lab File: BF083841.D
Acq: 16 Dec 2015 4:10




Instrument :
BNA_F
ClientSampleId :
K206-18-19DL


Tgt Ion: 70 Resp: 35326
Ion Ratio Lower Upper
70 100
42 40.6 49.2 73.8#
101 0.0 7.1 10.7#
130 2.2 15.4 23.0#

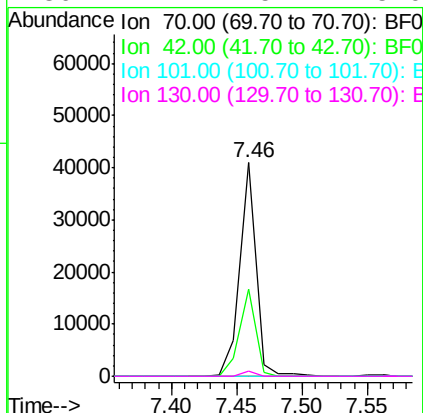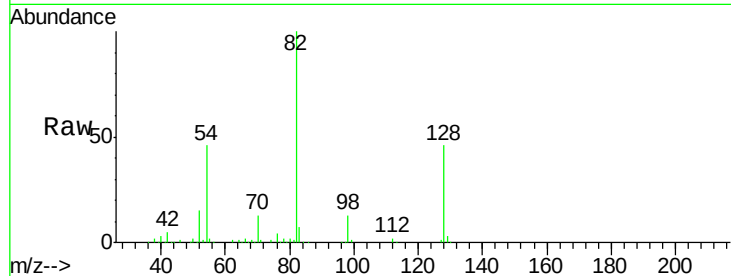

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.19 min Scan# 534
Delta R.T. -0.02 min
Lab File: BF083841.D
Acq: 16 Dec 2015 4:10

Tgt Ion: 136 Resp: 347673
Ion Ratio Lower Upper
136 100
137 10.3 8.7 13.1
54 4.7 7.8 11.6#
68 4.2 5.7 8.5#

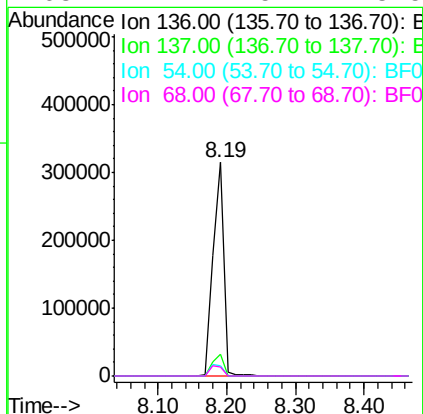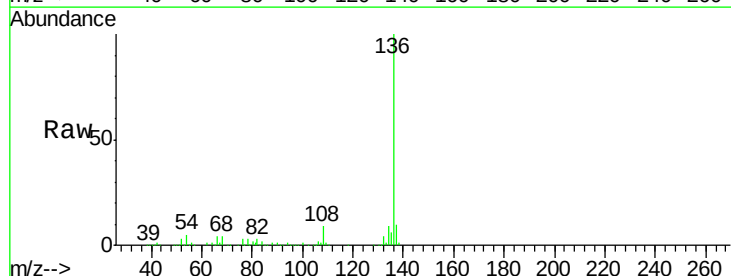







#23
 Nitrobenzene-d5
 Concen: 41.46 ng
 RT: 7.46 min Scan# 470
 Delta R.T. -0.02 min
 Lab File: BF083841.D
 Acq: 16 Dec 2015 4:10

Instrument :
 BNA_F
 ClientSampleId :
 K206-18-19DL

Tgt Ion	Ratio	Lower	Upper
82	100		
128	46.0	30.7	46.1
54	45.9	42.5	63.7

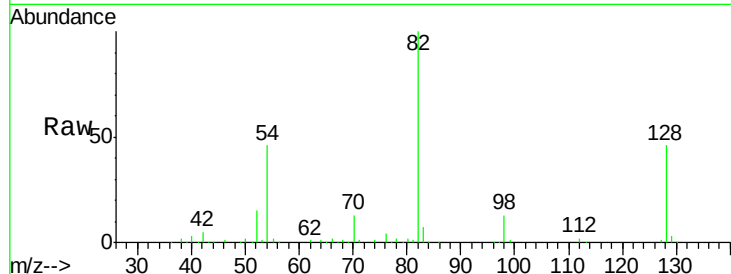


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): BF0
 Ion 54.00 (53.70 to 54.70): BF0

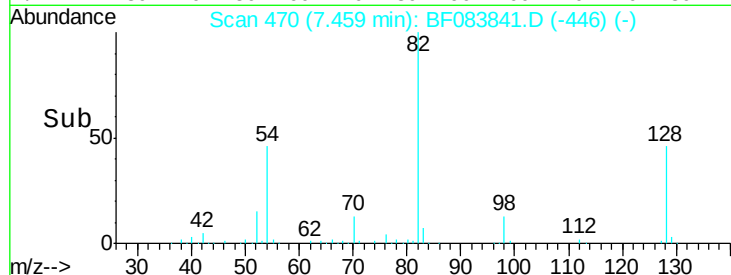
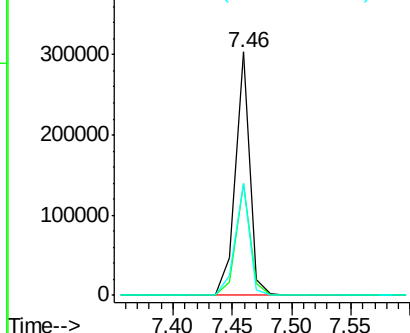



#25
 Isophorone
 Concen: 18.24 ng
 RT: 7.46 min Scan# 470
 Delta R.T. -0.29 min
 Lab File: BF083841.D
 Acq: 16 Dec 2015 4:10

Tgt Ion	Ratio	Lower	Upper
82	100		
95	0.0	5.0	7.4#
138	0.0	12.1	18.1#

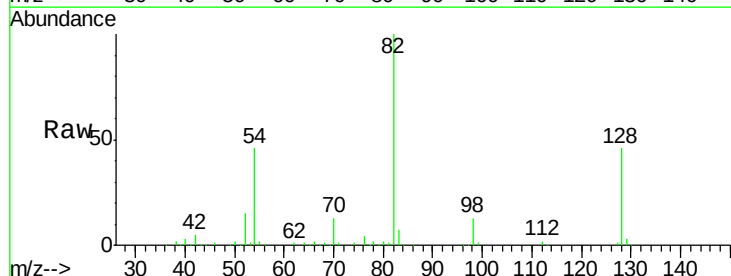

Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 95.00 (94.70 to 95.70): BF0
 Ion 138.00 (137.70 to 138.70): BF0

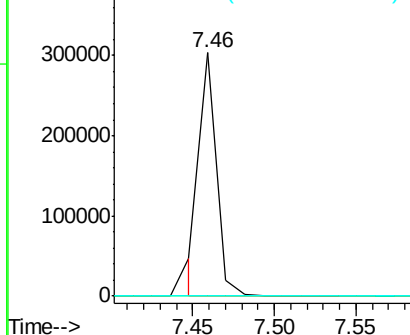







#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.94 min Scan# 687
Delta R.T. -0.02 min
Lab File: BF083841.D
Acq: 16 Dec 2015 4:10

Instrument :
BNA_F
ClientSampleId :
K206-18-19DL

Tgt Ion:164 Resp: 147255
Ion Ratio Lower Upper
164 100
162 104.8 78.8 118.2
160 46.2 33.4 50.2




Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E


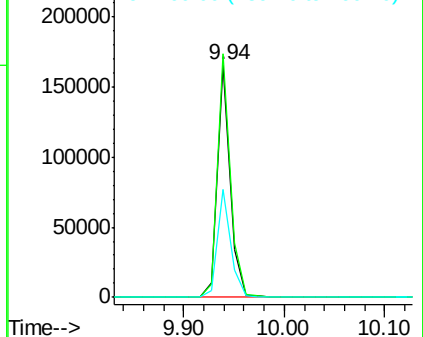



#41
2,4,6-Tribromophenol
Concen: 57.95 ng
RT: 10.73 min Scan# 756
Delta R.T. -0.02 min
Lab File: BF083841.D
Acq: 16 Dec 2015 4:10

Tgt Ion:330 Resp: 86957
Ion Ratio Lower Upper
330 100
332 96.6 0.0 0.0#
141 37.0 0.0 0.0#



Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

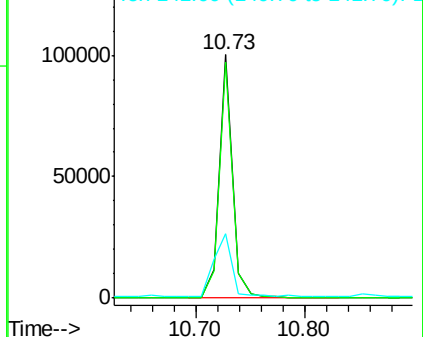







#44
 2-Fluorobiphenyl
 Concen: 42.54 ng
 RT: 9.26 min Scan# 628
 Delta R.T. -0.02 min
 Lab File: BF083841.D
 Acq: 16 Dec 2015 4:10

Instrument :
 BNA_F
 ClientSampleId :
 K206-18-19DL

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.7	28.6	42.8
170	23.6	19.4	29.0




Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E


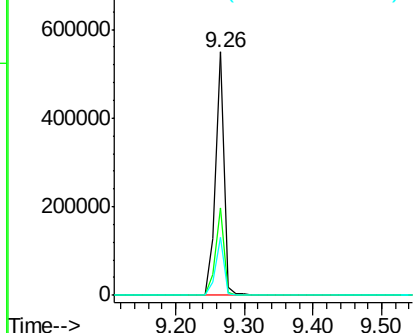



#48
 Acenaphthylene
 Concen: 6.16 ng
 RT: 9.80 min Scan# 675
 Delta R.T. -0.02 min
 Lab File: BF083841.D
 Acq: 16 Dec 2015 4:10

Tgt Ion	Ratio	Lower	Upper
152	100		
151	20.1	16.3	24.5
153	14.4	10.8	16.2



Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 151.00 (150.70 to 151.70): E
 Ion 153.00 (152.70 to 153.70): E

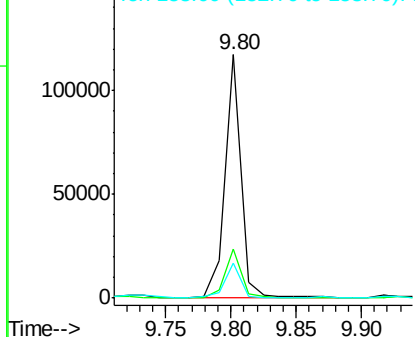



#49

Dimethylphthalate

Concen: 6.39 ng

RT: 9.65 min Scan# 662

Delta R.T. -0.03 min

Lab File: BF083841.D

Acq: 16 Dec 2015 4:10

Instrument :

BNA_F

ClientSampleId :

K206-18-19DL


Tgt Ion:163 Resp: 73398

Ion Ratio Lower Upper

163 100

194 3.7 2.8 4.2




164 10.4 8.6 13.0



Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

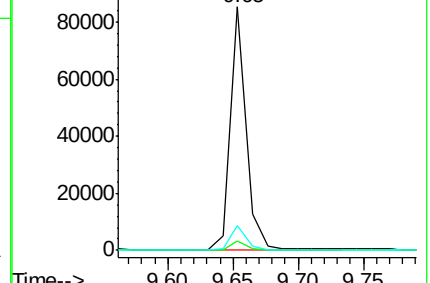

#51

Acenaphthene

Concen: 3.14 ng

RT: 9.97 min Scan# 690

Delta R.T. -0.02 min

Lab File: BF083841.D

Acq: 16 Dec 2015 4:10


Tgt Ion:154 Resp: 30780

Ion Ratio Lower Upper

154 100

153 113.4 91.4 137.0



152 54.6 43.4 65.2




Abundance Ion 154.00 (153.70 to 154.70): E

Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E




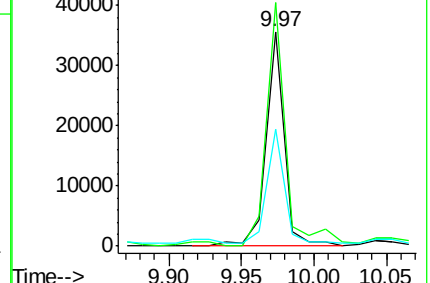


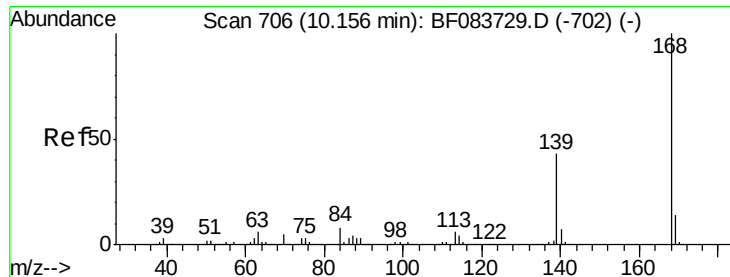

#54
Dibenzenofuran
Concen: 2.01 ng
RT: 10.14 min Scan# 705
Delta R.T. -0.02 min
Lab File: BF083841.D
Acq: 16 Dec 2015 4:10




Instrument :
BNA_F
ClientSampleId :
K206-18-19DL


Tgt Ion:168 Resp: 26103
Ion Ratio Lower Upper
168 100
139 38.2 28.0 42.0
169 20.8 10.8 16.2#

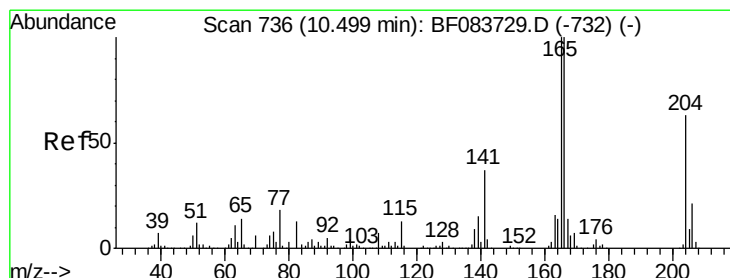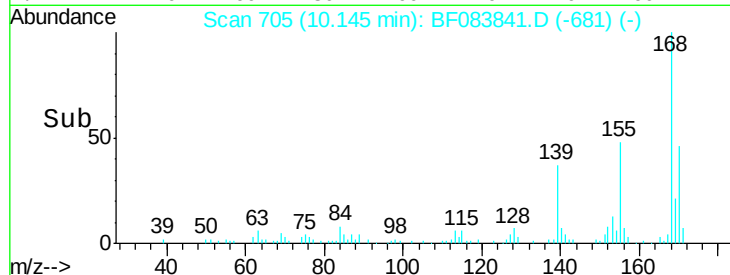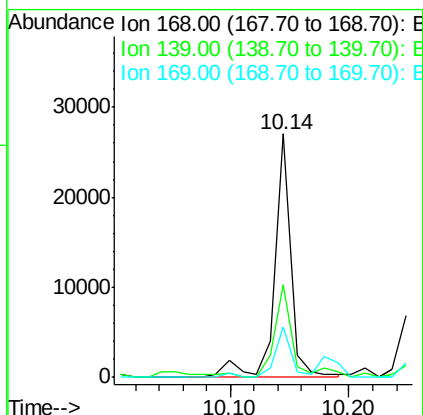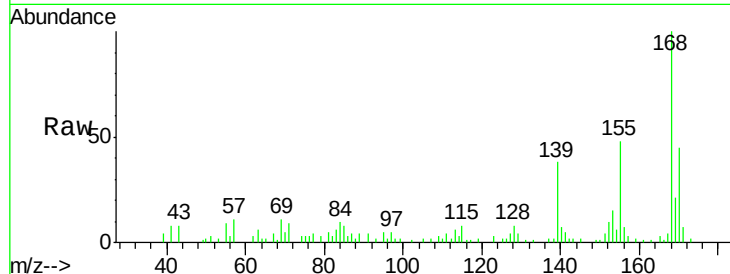

#57
Fluorene
Concen: 5.67 ng
RT: 10.49 min Scan# 735
Delta R.T. -0.02 min
Lab File: BF083841.D
Acq: 16 Dec 2015 4:10

Tgt Ion:166 Resp: 58016
Ion Ratio Lower Upper
166 100
165 103.6 80.0 120.0
167 14.9 10.6 16.0

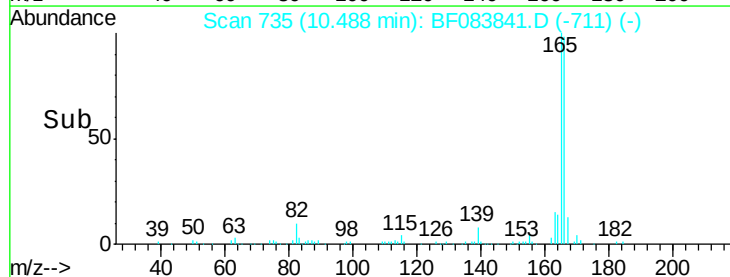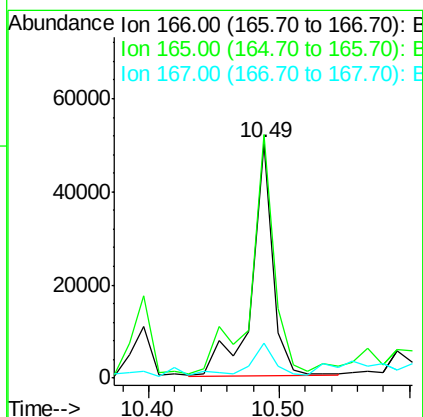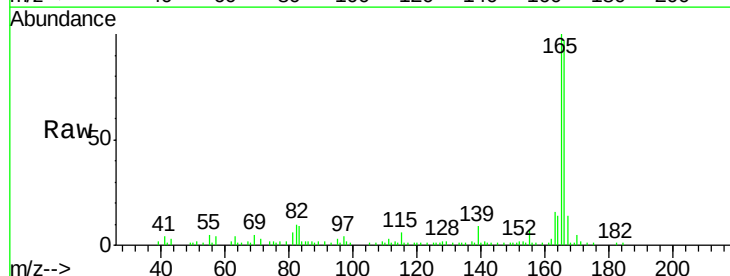



#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.43 min Scan# 817

Delta R.T. -0.02 min

Lab File: BF083841.D

Acq: 16 Dec 2015 4:10

Instrument :

BNA_F

ClientSampleId :

K206-18-19DL


Tgt Ion:188 Resp: 239610

Ion Ratio Lower Upper

188 100

94 9.2 9.4 14.2#




80 9.3 10.6 16.0#



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

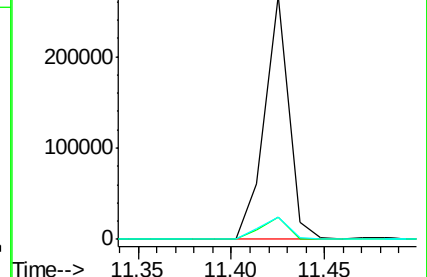

#66

4-Bromophenyl-phenylether

Concen: 2.16 ng

RT: 10.73 min Scan# 756

Delta R.T. -0.26 min

Lab File: BF083841.D

Acq: 16 Dec 2015 4:10


Tgt Ion:248 Resp: 5779

Ion Ratio Lower Upper

248 100

250 202.9 79.2 118.8#



141 419.1 58.2 87.4#




Abundance Ion 248.00 (247.70 to 248.70): E

Ion 250.00 (249.70 to 250.70): E

Ion 141.00 (140.70 to 141.70): E

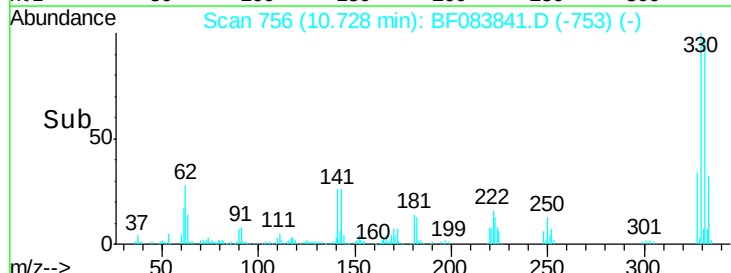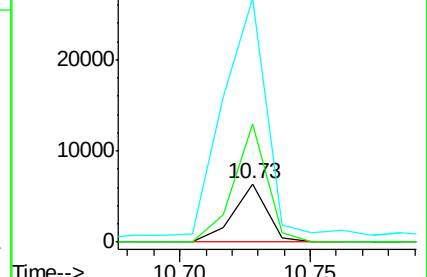



#70

Phenanthrene

Concen: 36.71 ng

RT: 11.45 min Scan# 819

Delta R.T. -0.02 min

Lab File: BF083841.D

Acq: 16 Dec 2015 4:10

Instrument :

BNA_F

ClientSampleId :

K206-18-19DL


Tgt Ion:178 Resp: 467217

Ion Ratio Lower Upper

178 100

176 19.7 15.7 23.5


179 15.7 12.2 18.4





Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

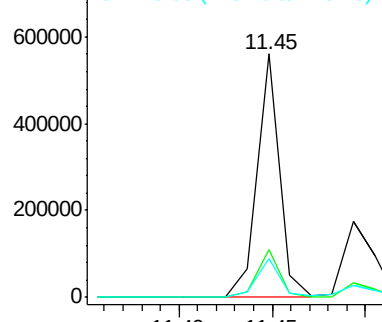

Time-->



#71

Anthracene

Concen: 15.47 ng

RT: 11.49 min Scan# 823

Delta R.T. -0.02 min

Lab File: BF083841.D

Acq: 16 Dec 2015 4:10


Tgt Ion:178 Resp: 204495

Ion Ratio Lower Upper

178 100

176 18.3 15.2 22.8


179 16.1 12.6 18.8




Abundance Ion 178.00 (177.70 to 178.70): E


Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

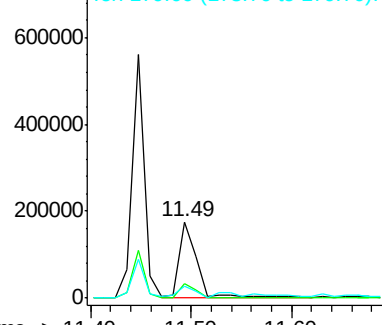

Time-->





#74

Fluoranthene

Concen: 53.74 ng

RT: 12.64 min Scan# 923

Delta R.T. -0.01 min

Lab File: BF083841.D

Acq: 16 Dec 2015 4:10

Instrument :

BNA_F

ClientSampleId :

K206-18-19DL


Tgt Ion: 202 Resp: 706799

Ion Ratio Lower Upper

202 100

101 13.5 0.0 31.5




203 18.3 0.0 37.6



Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

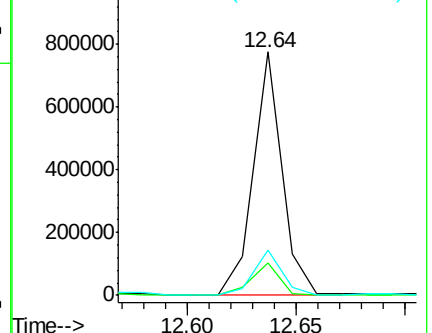

#75

Chrysene-d12

Concen: 20.00 ng

RT: 14.05 min Scan# 1047

Delta R.T. -0.02 min

Lab File: BF083841.D

Acq: 16 Dec 2015 4:10


Tgt Ion: 240 Resp: 192046

Ion Ratio Lower Upper

240 100

120 16.6 8.1 12.1#



236 25.4 20.8 31.2




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E




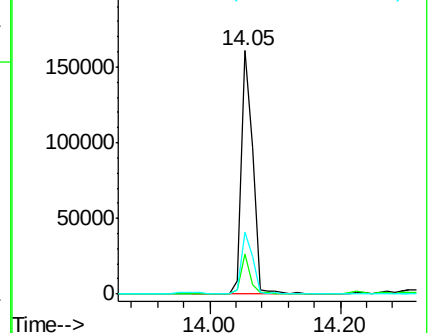




#77
 Pyrene
 Concen: 51.67 ng
 RT: 12.87 min Scan# 943
 Delta R.T. -0.01 min
 Lab File: BF083841.D
 Acq: 16 Dec 2015 4:10




Instrument :
 BNA_F
 ClientSampleID :
 K206-18-19DL


Tgt Ion: 202 Resp: 784219
 Ion Ratio Lower Upper
 202 100
 200 21.9 16.7 25.1
 203 18.5 14.3 21.5

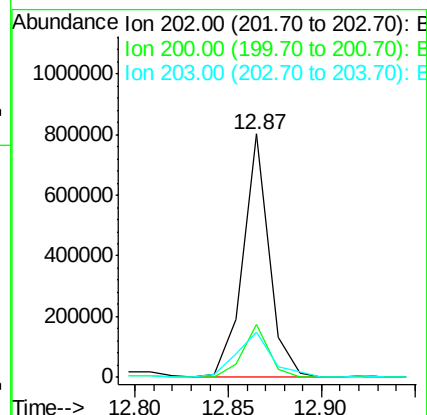

#78
 Terphenyl-d14
 Concen: 37.65 ng
 RT: 13.00 min Scan# 955
 Delta R.T. -0.02 min
 Lab File: BF083841.D
 Acq: 16 Dec 2015 4:10

Tgt Ion: 244 Resp: 336154
 Ion Ratio Lower Upper
 244 100
 212 7.4 6.1 9.1
 122 15.2 11.0 16.6

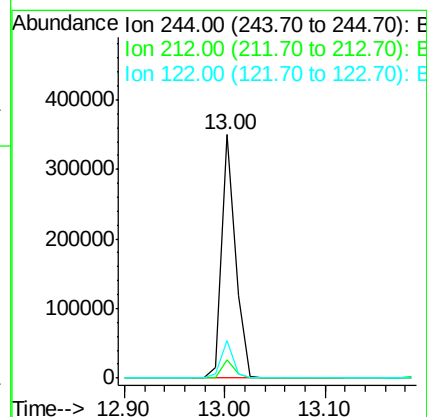



#80

Benzo(a)anthracene

Concen: 30.03 ng

RT: 14.04 min Scan# 1046

Delta R.T. -0.02 min

Lab File: BF083841.D

Acq: 16 Dec 2015 4:10

Instrument :

BNA_F

ClientSampleId :

K206-18-19DL


Tgt Ion:228 Resp: 327972

Ion Ratio Lower Upper

228 100

226 35.3 22.3 33.5#




229 21.2 15.7 23.5



Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

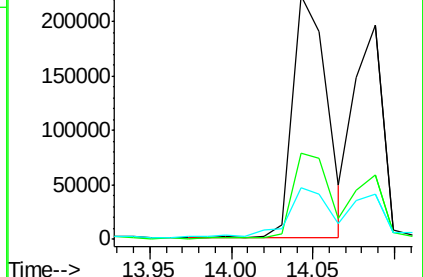

#82

Chrysene

Concen: 30.79 ng

RT: 14.04 min Scan# 1046

Delta R.T. -0.06 min

Lab File: BF083841.D

Acq: 16 Dec 2015 4:10


Tgt Ion:228 Resp: 327972

Ion Ratio Lower Upper

228 100

226 35.3 24.7 37.1



229 21.2 16.3 24.5




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E



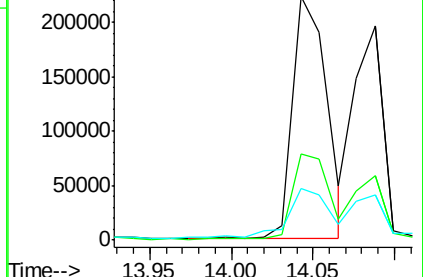





#85
 Indeno(1,2,3-cd)pyrene
 Concen: 6.86 ng
 RT: 16.92 min Scan# 1298
 Delta R.T. -0.02 min
 Lab File: BF083841.D
 Acq: 16 Dec 2015 4:10




Instrument :
 BNA_F
 ClientSampleId :
 K206-18-19DL


Tgt Ion: 276 Resp: 71751
 Ion Ratio Lower Upper
 276 100
 138 25.0 0.0 0.0#
 277 27.3 0.0 0.0#

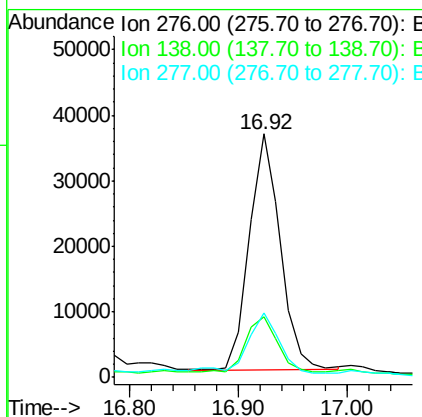

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.49 min Scan# 1173
 Delta R.T. -0.01 min
 Lab File: BF083841.D
 Acq: 16 Dec 2015 4:10

Tgt Ion: 264 Resp: 147175
 Ion Ratio Lower Upper
 264 100
 260 24.3 19.4 29.0
 265 23.0 17.8 26.6

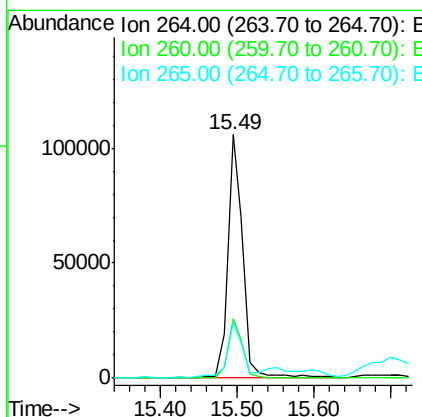

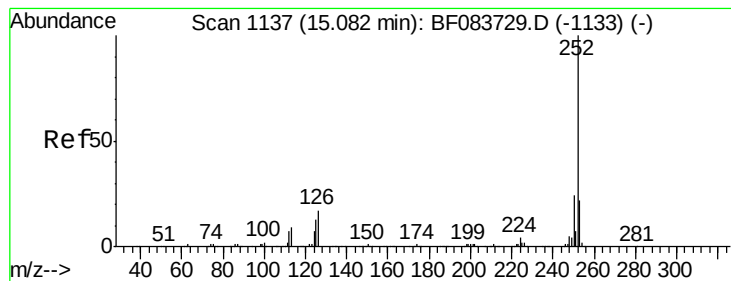

#87

Benzo(b)fluoranthene

Concen: 29.90 ng

RT: 15.08 min Scan# 1137

Delta R.T. -0.01 min

Lab File: BF083841.D

Acq: 16 Dec 2015 4:10





Instrument :

BNA_F

ClientSampleId :

K206-18-19DL

Tgt Ion:	252	Resp:	280777
Ion Ratio		Lower	Upper
252	100		
253	22.5	18.2	27.4
125	13.0	8.2	12.4#

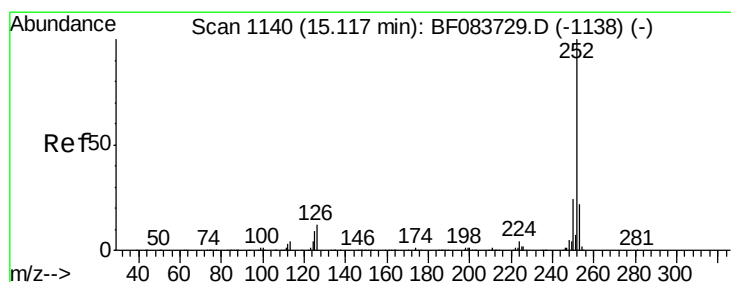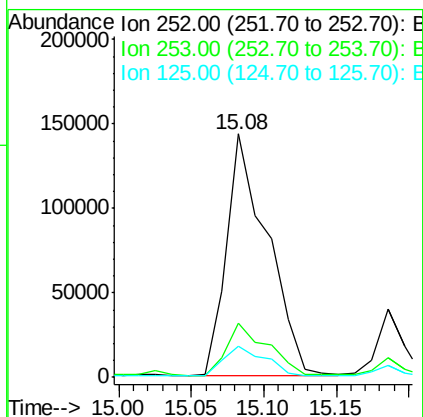

#88

Benzo(k)fluoranthene

Concen: 33.00 ng




RT: 15.08 min Scan# 1137


Delta R.T. -0.05 min

Lab File: BF083841.D

Acq: 16 Dec 2015 4:10

Tgt Ion:	252	Resp:	280777
Ion Ratio		Lower	Upper
252	100		
253	22.5	18.6	27.8
125	13.0	11.5	17.3

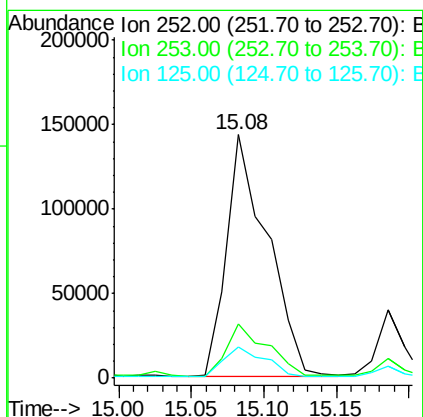



#89

Benzo(a)pyrene

Concen: 21.36 ng

RT: 15.44 min Scan# 1168

Delta R.T. -0.01 min

Lab File: BF083841.D

Acq: 16 Dec 2015 4:10

Instrument :

BNA_F

ClientSampleId :

K206-18-19DL


Tgt Ion: 252 Resp: 179004

Ion Ratio Lower Upper

252 100

253 22.6 17.5 26.3




125 13.6 11.0 16.6



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

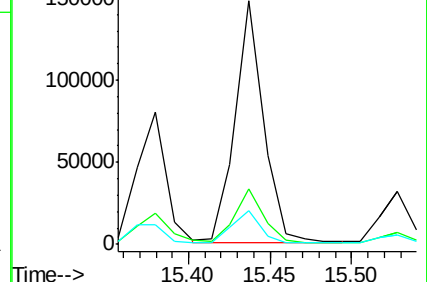

#91

Benzo(g,h,i)perylene

Concen: 8.69 ng

RT: 17.36 min Scan# 1336

Delta R.T. -0.02 min

Lab File: BF083841.D

Acq: 16 Dec 2015 4:10


Tgt Ion: 276 Resp: 74408

Ion Ratio Lower Upper

276 100

277 23.8 19.2 28.8

138 24.3 19.5 29.3



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 277.00 (276.70 to 277.70): E

Ion 138.00 (137.70 to 138.70): E

