
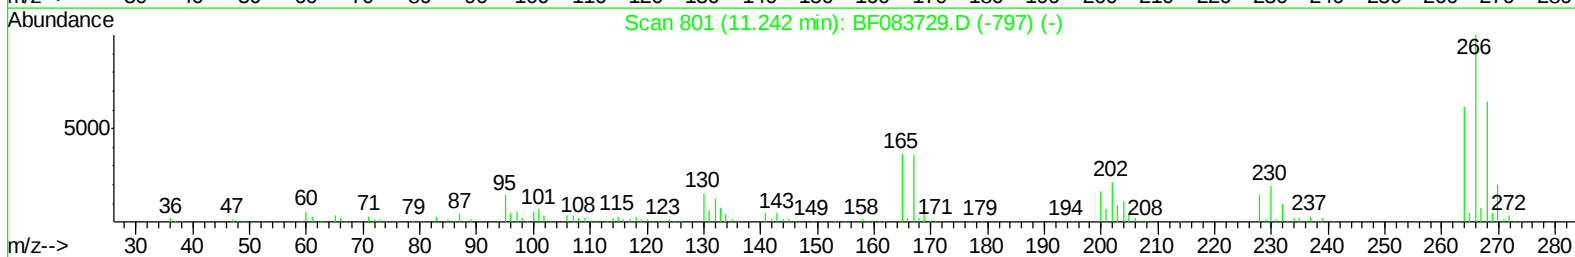
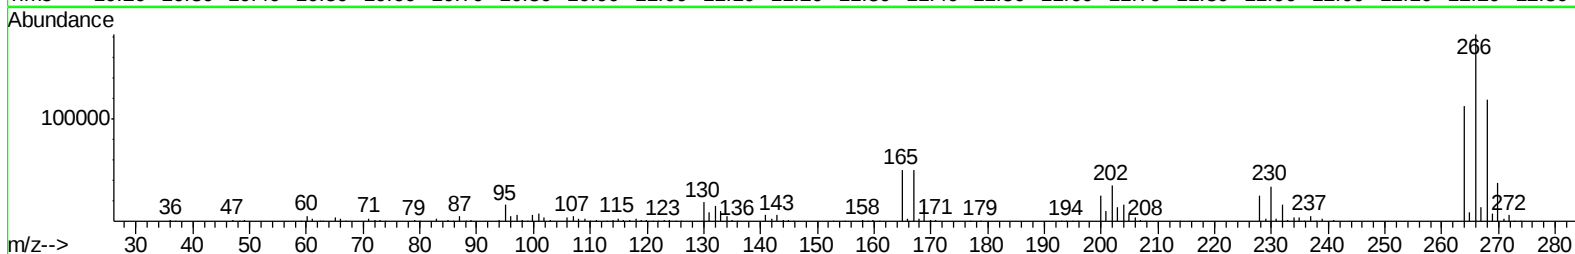


Data Path : Z:\HPCHEM1\BNA_F\Data\BF121515\
Data File : BF083801.D
Acq On : 15 Dec 2015 6:50
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 15 07:56:03 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 14 01:30:12 2015
Response via : Initial Calibration

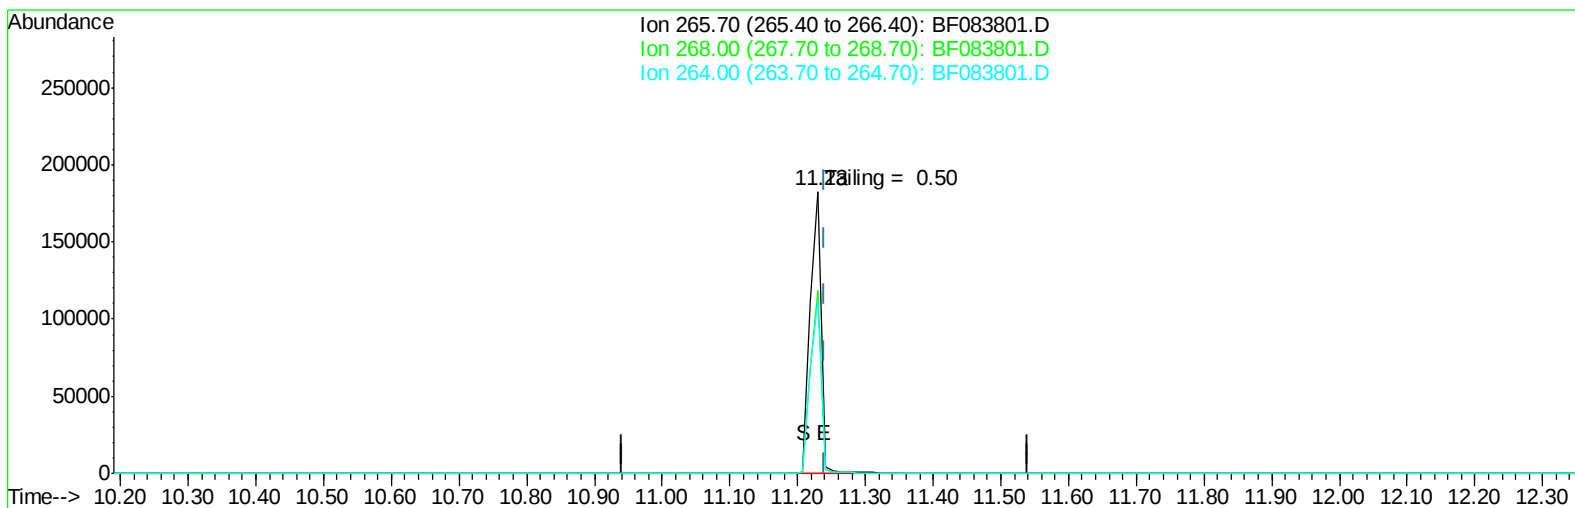

TIC: BF083801.D

(69) Pentachlorophenol (C)




11.230min (-0.011) 46297.38ng

response 208831

Ion	Exp%	Act%
265.70	100	100
268.00	62.70	65.00
264.00	64.30	61.48
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF121515\
Data File : BF083801.D
Acq On : 15 Dec 2015 6:50
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 15 07:56:03 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 14 01:30:12 2015
Response via : Initial Calibration

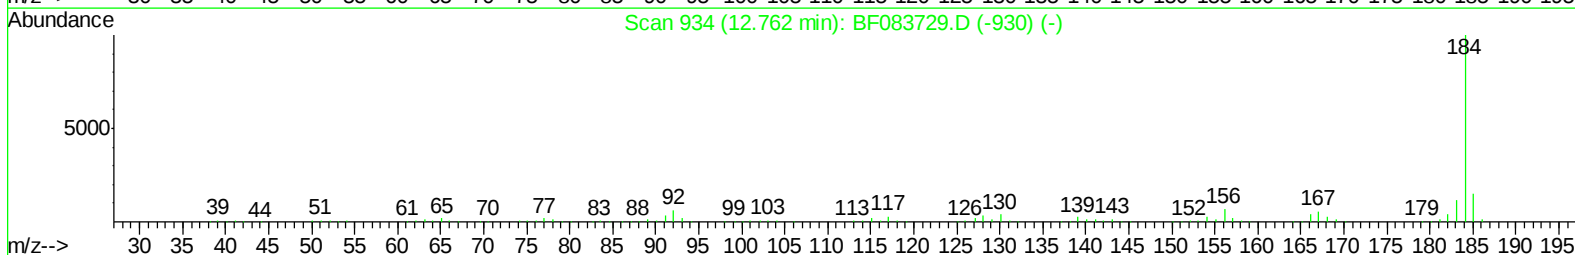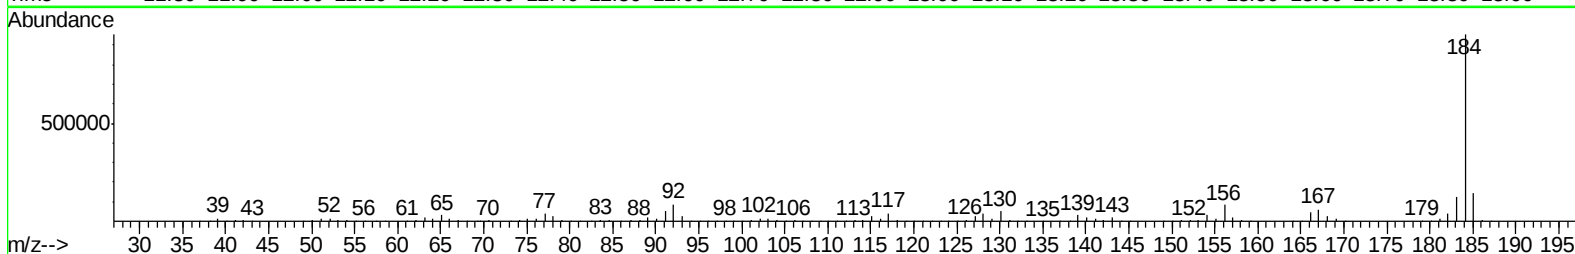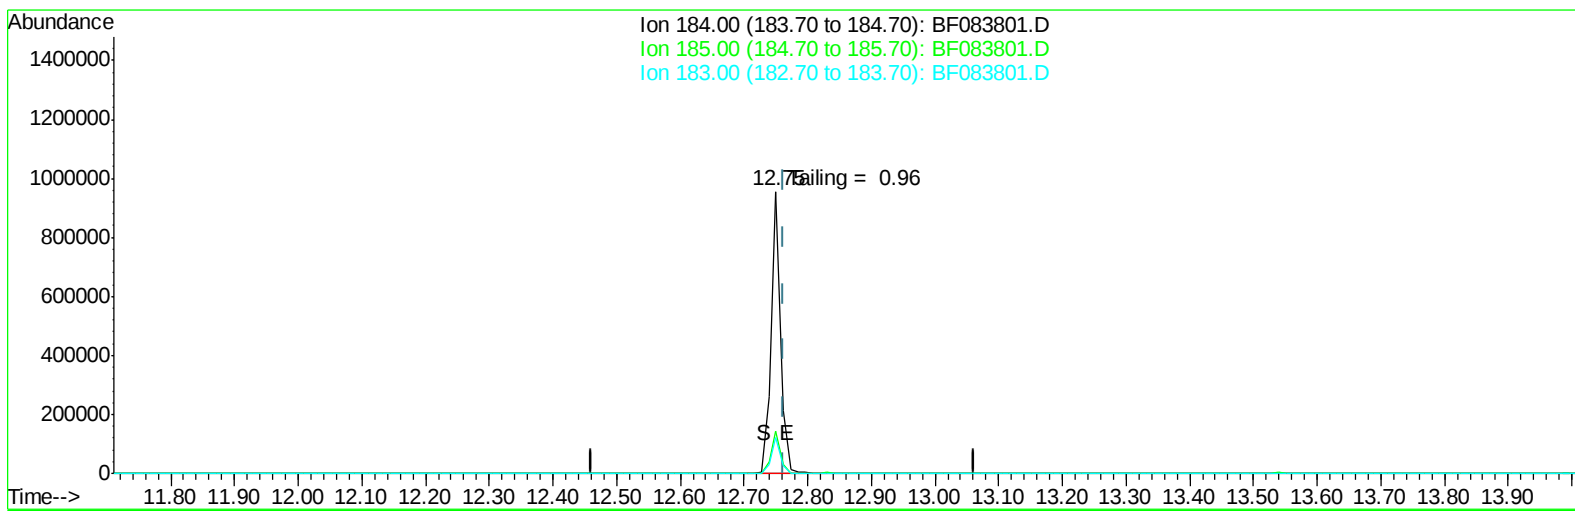

TIC: BF083801.D

(76) Benzidine

12.751min (-0.012) 0.00ng

response 1008043

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	15.07
183.00	11.20	12.77
0.00	0.00	0.00