
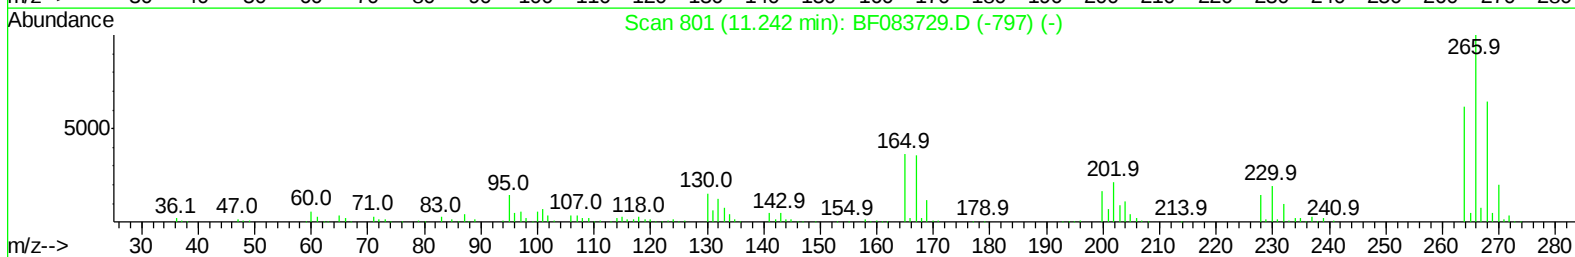
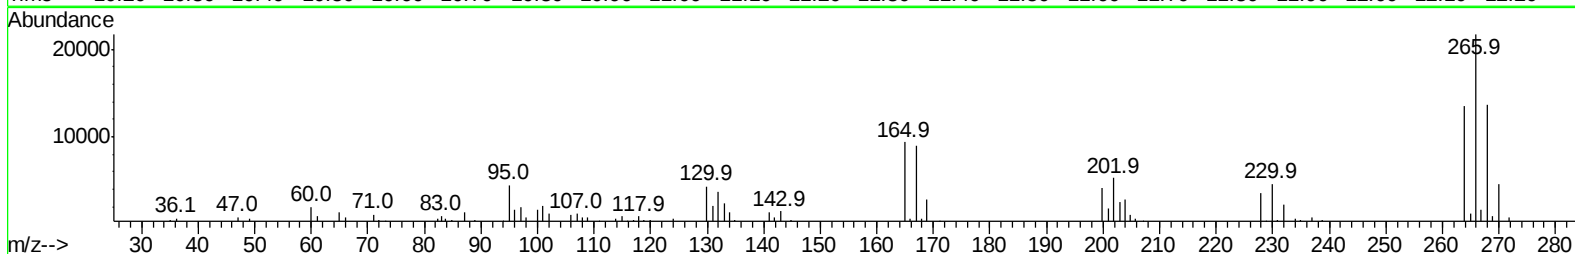


Data Path : Z:\HPCHEM1\BNA F\Data\BF121515\
Data File : BF083827.D
Acq On : 15 Dec 2015 21:39
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 16 08:09:02 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 14 01:30:12 2015
Response via : Initial Calibration

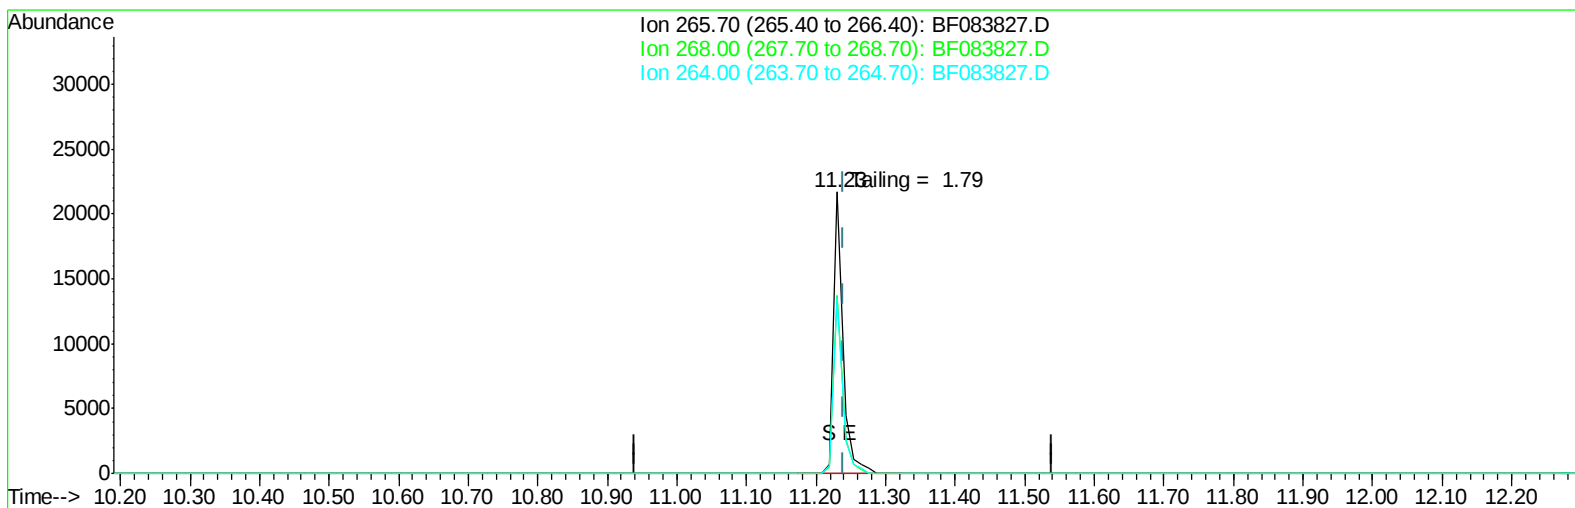

TIC: BF083827.D

(69) Pentachlorophenol (C)




11.231min (-0.010) 0.00ng

response 19827

Ion	Exp%	Act%
265.70	100	100
268.00	62.70	63.02
264.00	64.30	62.33
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF121515\
Data File : BF083827.D
Acq On : 15 Dec 2015 21:39
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 16 08:09:02 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 14 01:30:12 2015
Response via : Initial Calibration

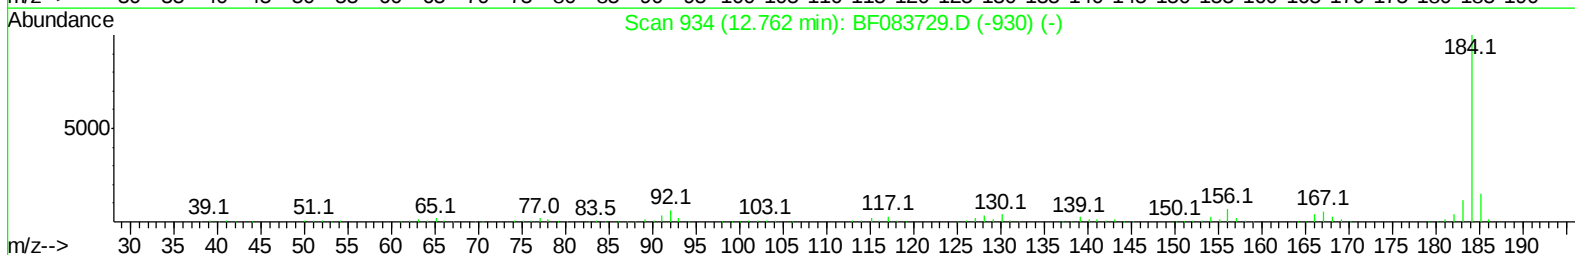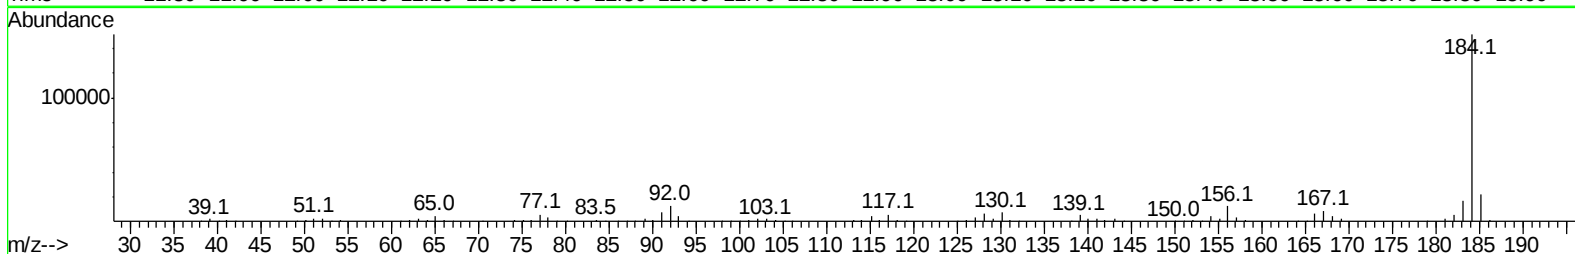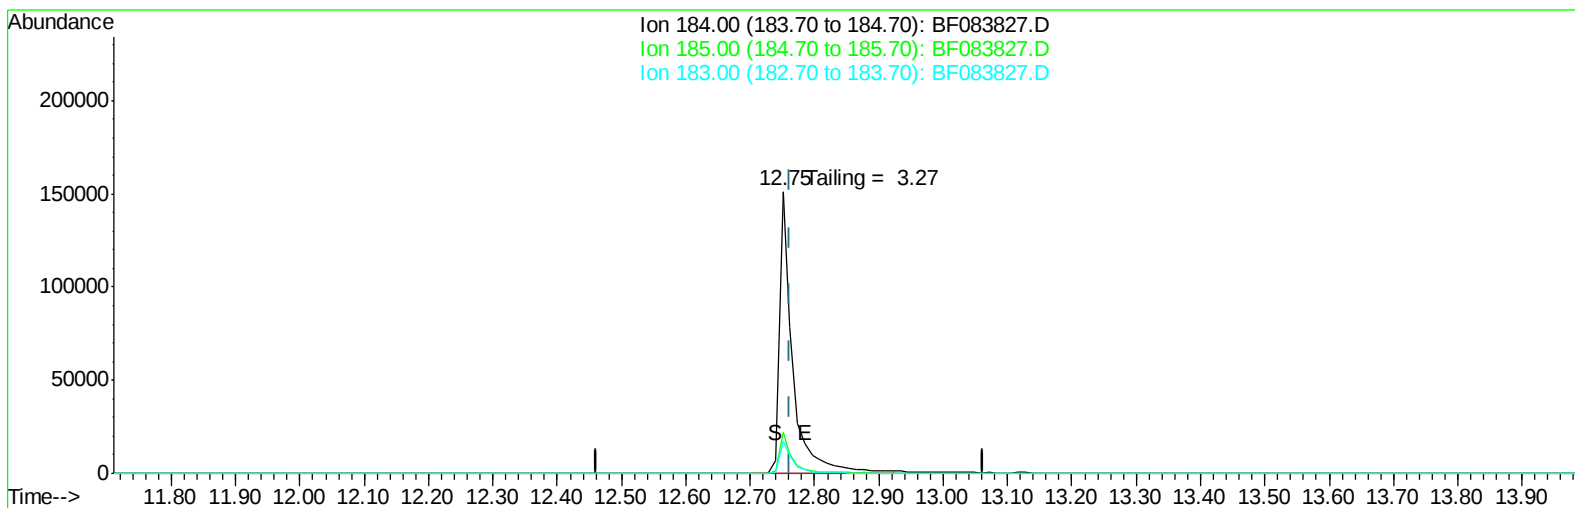

TIC: BF083827.D

(76) Benzidine

12.751min (-0.011) 28504.78ng

response 223234

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	14.57
183.00	11.20	11.47
0.00	0.00	0.00