


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF121515\
 Data File : BF083801.D
 Acq On : 15 Dec 2015 6:50
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 14 01:30:12 2015

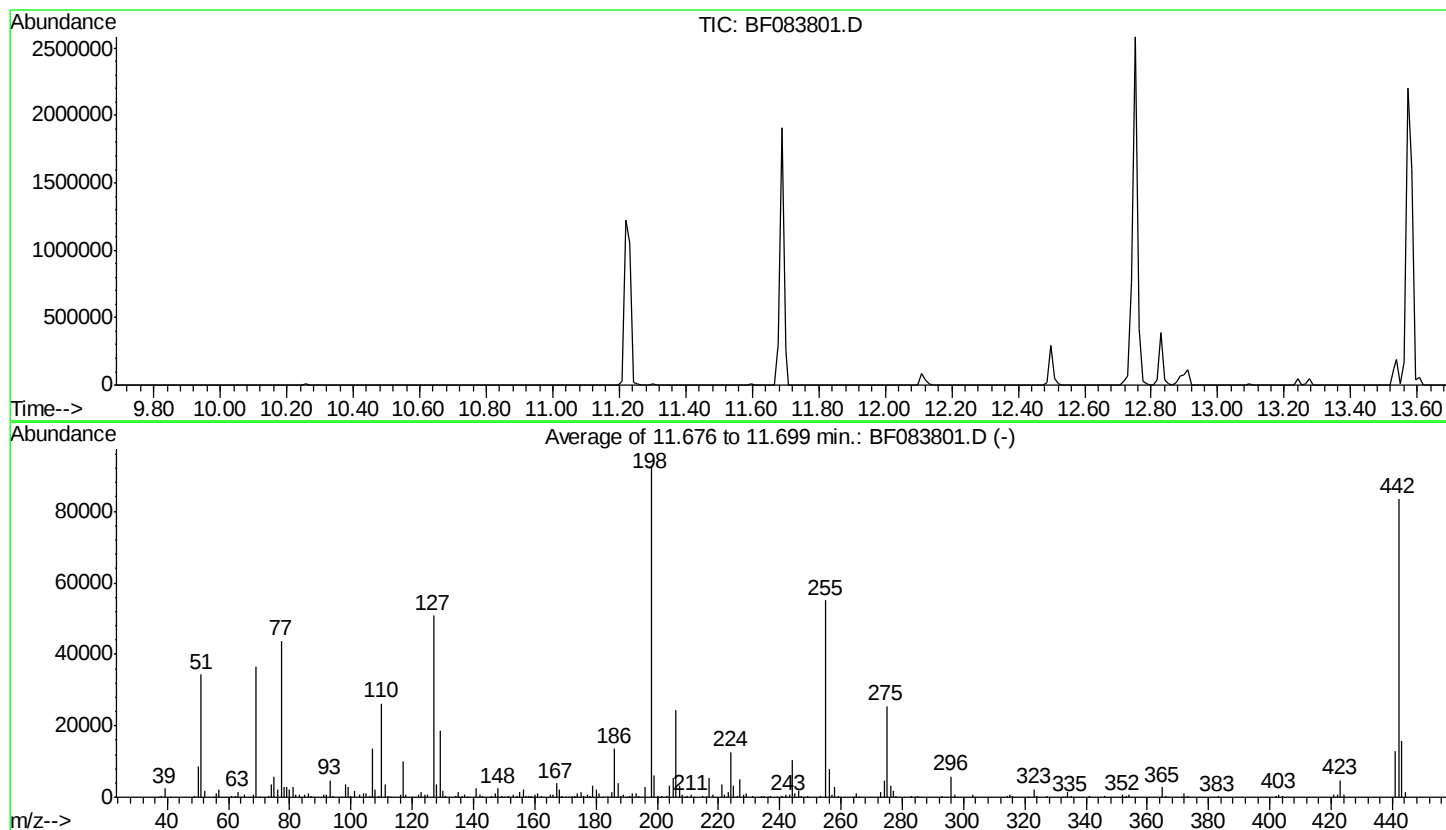

AutoFind: Scans 839, 840, 841; Background Corrected with Scan 836

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.0	34355	PASS
68	69	0.00	2	2.0	728	PASS
69	198	0.00	100	39.5	36683	PASS
70	69	0.00	2	0.3	117	PASS
127	198	10	80	54.7	50705	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	92780	PASS
199	198	5	9	6.5	5991	PASS
275	198	10	60	27.5	25522	PASS
365	198	1	100	3.1	2847	PASS
441	442	0.01	24	15.3	12760	PASS
442	198	50	100	90.0	83538	PASS
443	442	15	24	19.0	15831	PASS