


Data Path : V:\HPCHEM1\BNA_F\DATA\BF121515\
 Data File : BF083827.D
 Acq On : 15 Dec 2015 21:39
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 14 01:30:12 2015

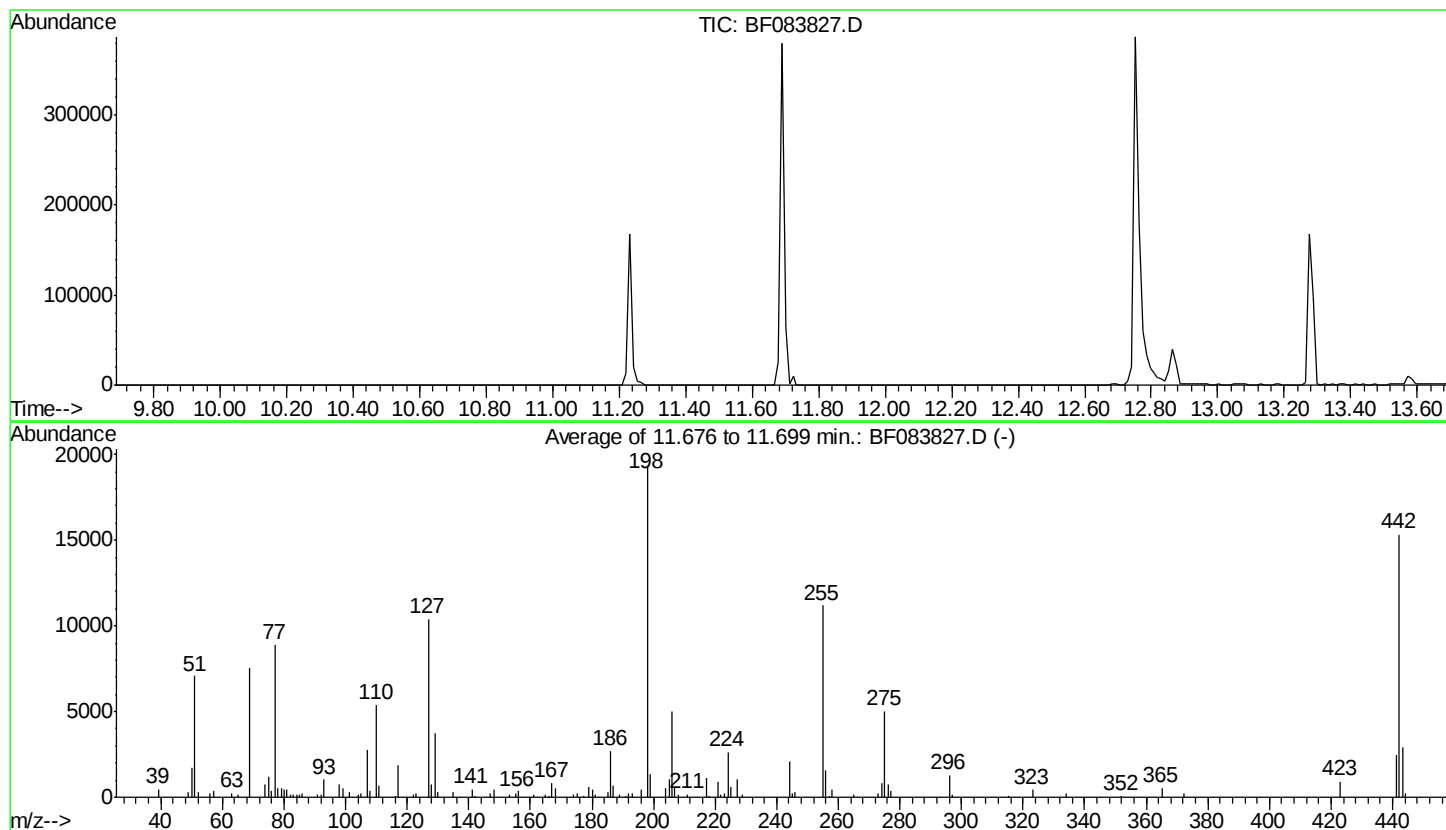

AutoFind: Scans 839, 840, 841; Background Corrected with Scan 836

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.6	7089	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	39.0	7551	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.8	10406	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	19351	PASS
199	198	5	9	6.8	1312	PASS
275	198	10	60	26.0	5037	PASS
365	198	1	100	2.7	531	PASS
441	442	0.01	24	16.3	2495	PASS
442	198	50	100	79.2	15322	PASS
443	442	15	24	18.8	2887	PASS