

Data Path : Z:\HPCHEM1\BNA F\DATA\BF121516\
 Data File : BF091642.D
 Acq On : 15 Dec 2016 21:37
 Operator : UM/SJ
 Sample : H6029-02
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 IDW-WATER-02

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF120916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.944	248	250	253	rBV	1028387	1452135	17.28%	2.418%
2	5.379	286	288	291	rBV	3123280	4084178	48.61%	6.800%
3	6.419	377	379	382	rBV	3004345	2632253	31.33%	4.383%
4	6.556	388	391	393	rBV	6693427	6873649	81.82%	11.444%
5	6.784	409	411	413	rBV	2046443	1807053	21.51%	3.009%
6	6.944	422	425	427	rVB	6491760	6619636	78.79%	11.021%
7	7.356	457	461	463	rBV	4334948	5715898	68.04%	9.517%
8	8.065	521	523	526	rBV	2047508	2377815	28.30%	3.959%
9	9.150	615	618	620	rBV	8618023	8401340	100.00%	13.988%
10	9.539	650	652	655	rBV	127977	134867	1.61%	0.225%
11	9.825	674	677	679	rVB	2965034	2666952	31.74%	4.440%
12	10.259	712	715	717	rVB3	90704	163743	1.95%	0.273%
13	10.613	743	746	748	rBV	4476338	4871279	57.98%	8.110%
14	10.739	755	757	761	rVB2	50617	85031	1.01%	0.142%
15	11.173	793	795	799	rBV3	94810	141736	1.69%	0.236%
16	11.299	804	806	809	rBV	2100581	2023251	24.08%	3.369%
17	11.871	855	856	859	rVB2	245444	241746	2.88%	0.402%
18	12.888	942	945	948	rBV	5218608	6426001	76.49%	10.699%
19	13.791	1022	1024	1028	rBV3	68049	86991	1.04%	0.145%
20	13.928	1034	1036	1039	rBV	1267439	1631789	19.42%	2.717%
21	15.345	1157	1160	1162	rBV	1269330	1625366	19.35%	2.706%


Sum of corrected areas: 60062709

Data Path : Z:\HPCHEM1\BNA F\DATA\BF121516\
Data File : BF091642.D
Acq On : 15 Dec 2016 21:37
Operator : UM/SJ
Sample : H6029-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
IDW-WATER-02

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF120916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

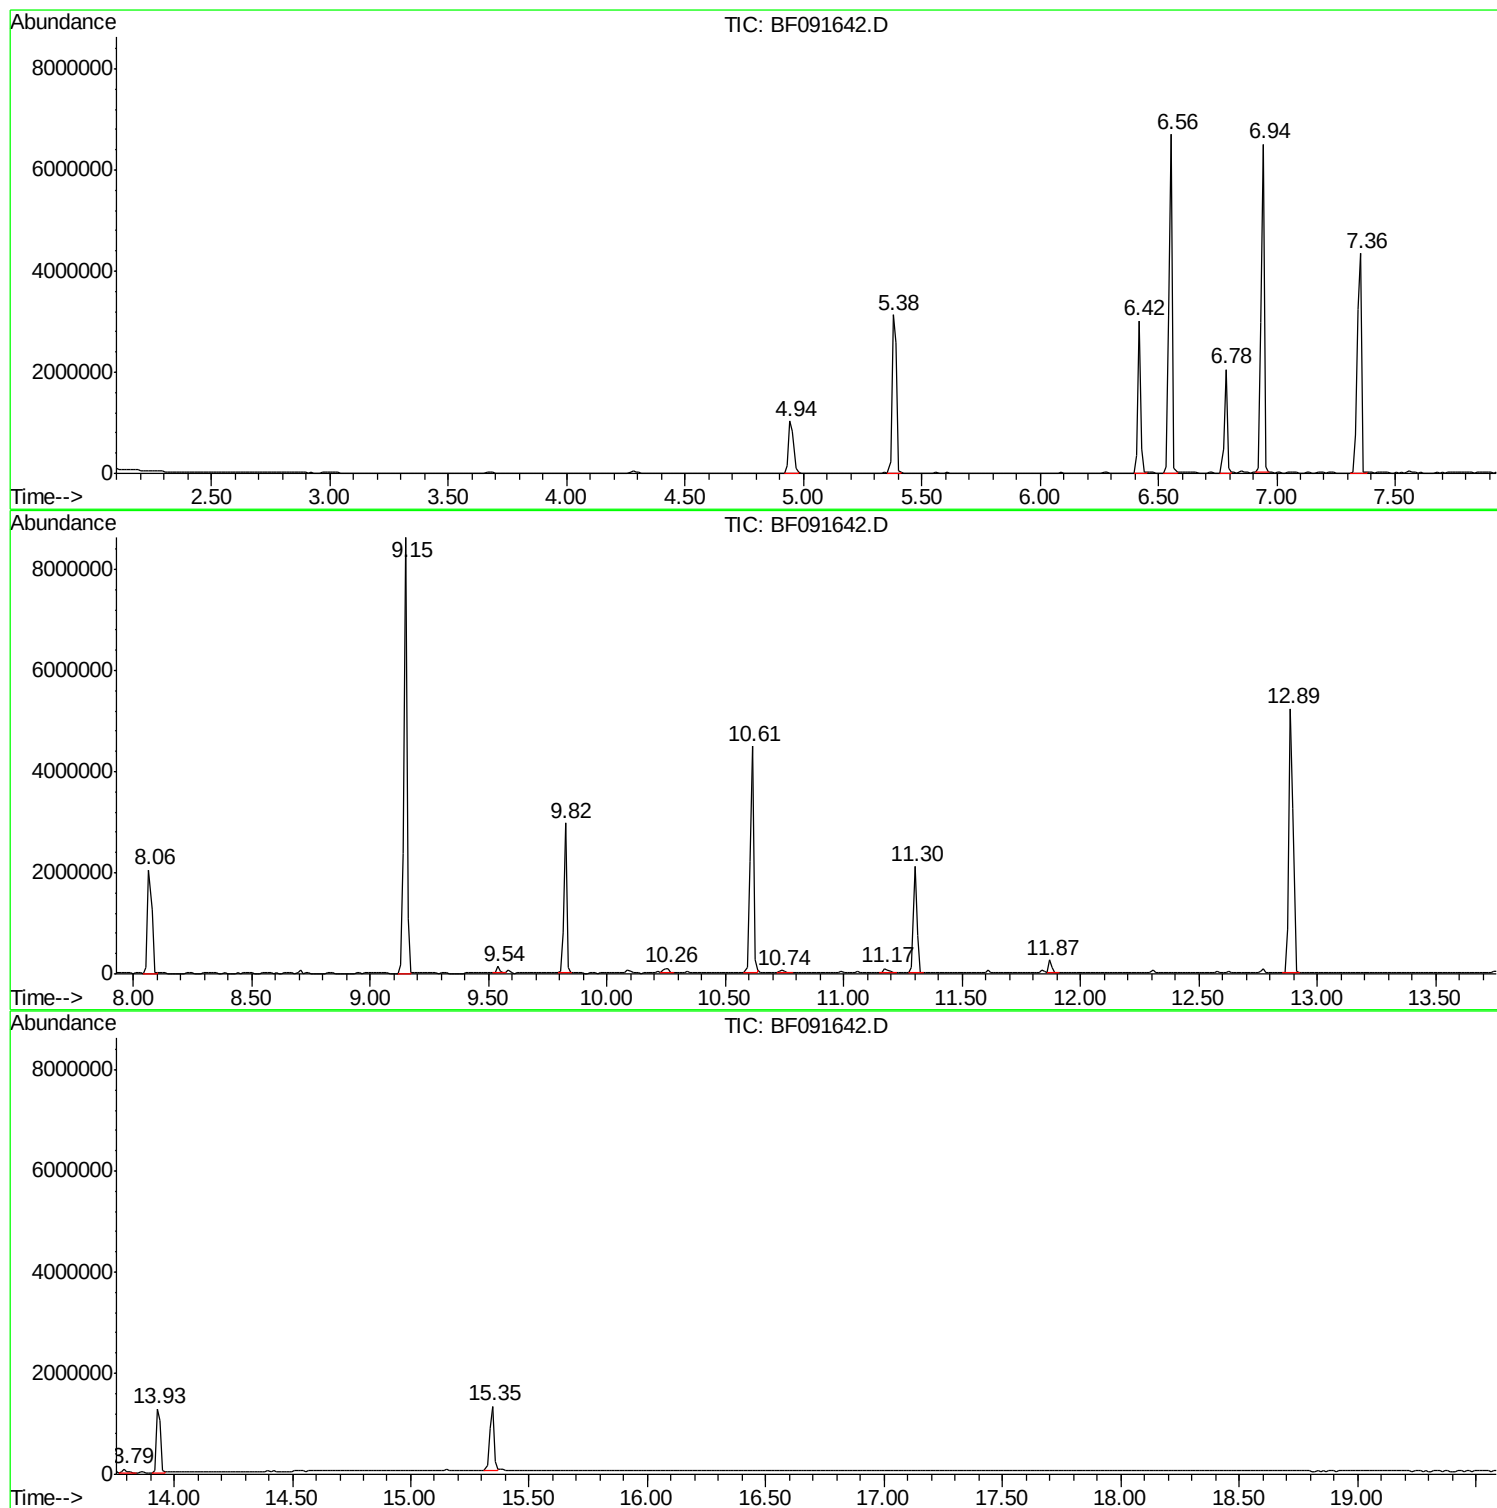

Data Path : Z:\HPCHEM1\BNA F\DATA\BF121516\
Data File : BF091642.D
Acq On : 15 Dec 2016 21:37
Operator : UM/SJ
Sample : H6029-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
IDW-WATER-02










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF120916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.94	16.07 ng	1452140	1,4-Dichlorobenzene-d4	6.78

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	64
2		Acetic acid, cyano-, 1,1-dimethyl...	141	C7H11NO2	001116-98-9	25
3		2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	9
4		Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9
5		Butane, 1-ethoxy-	102	C6H14O	000628-81-9	9

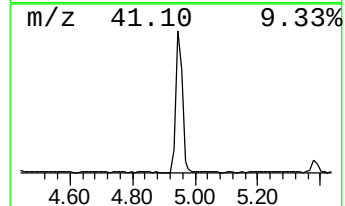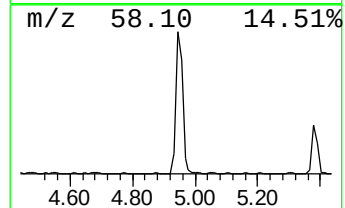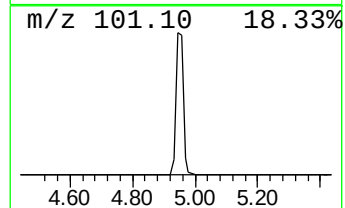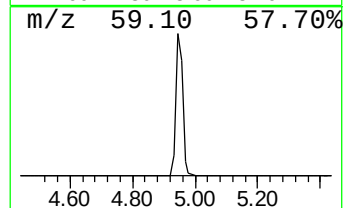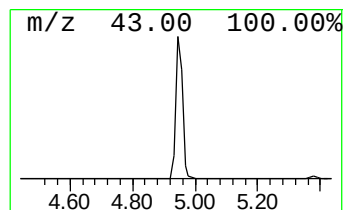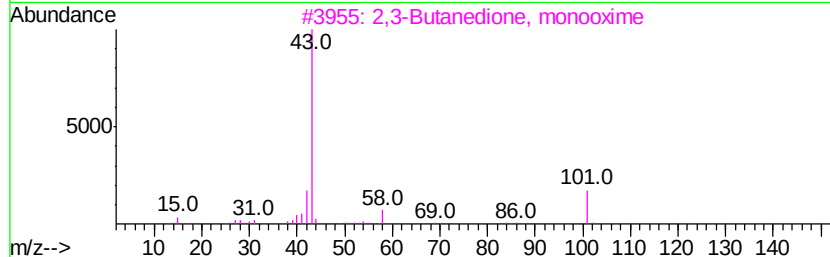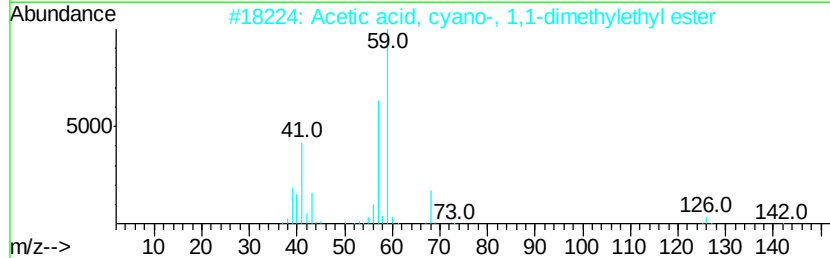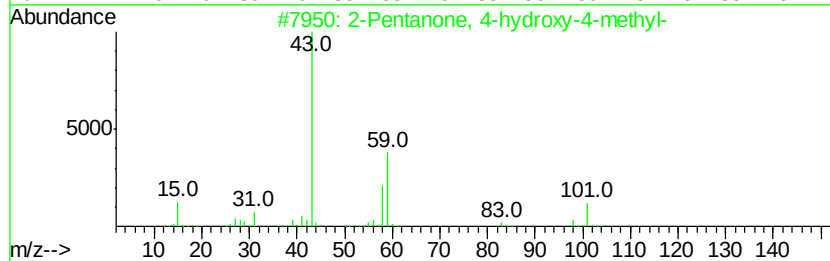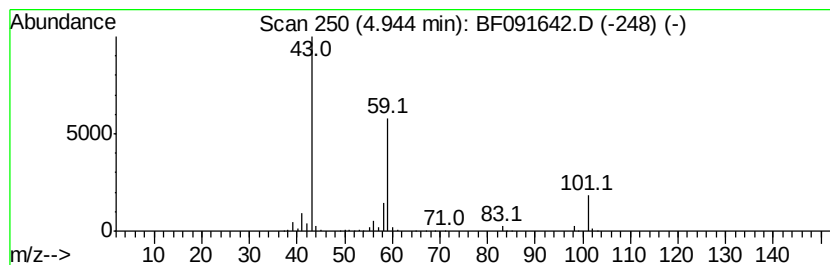

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF121516\
Data File : BF091642.D
Acq On : 15 Dec 2016 21:37
Operator : UM/SJ
Sample : H6029-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
IDW-WATER-02










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF120916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.56 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.56	76.08 ng	6873650	1,4-Dichlorobenzene-d4	6.78

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10
3		Benzene, 1,3,5-trifluoro-	132	C6H3F3	000372-38-3	9
4		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
5		Benzene, 1-ethenyl-3,5-dimethyl-	132	C10H12	005379-20-4	9

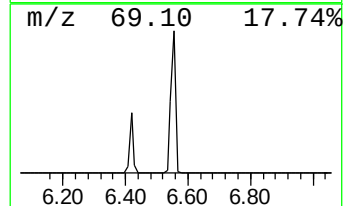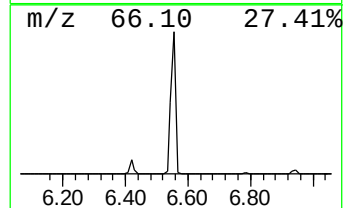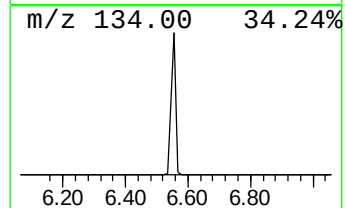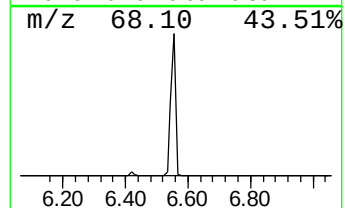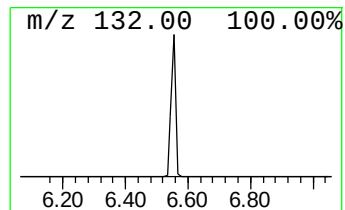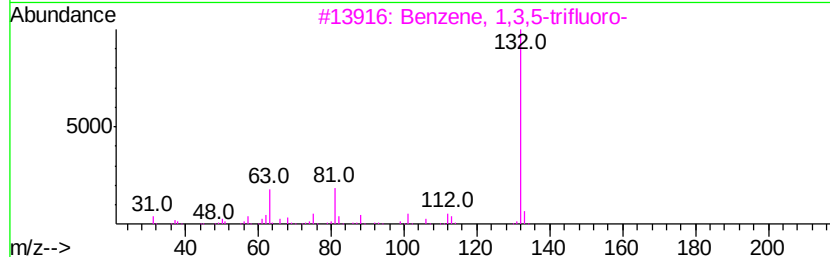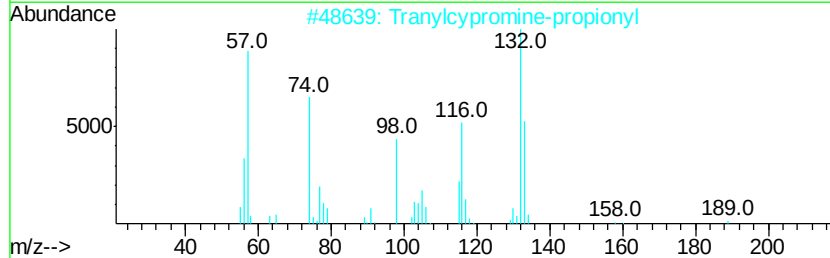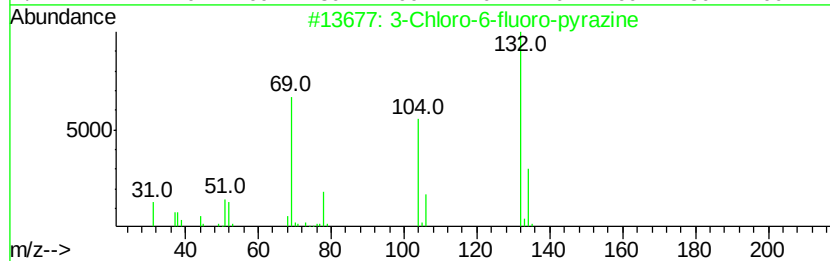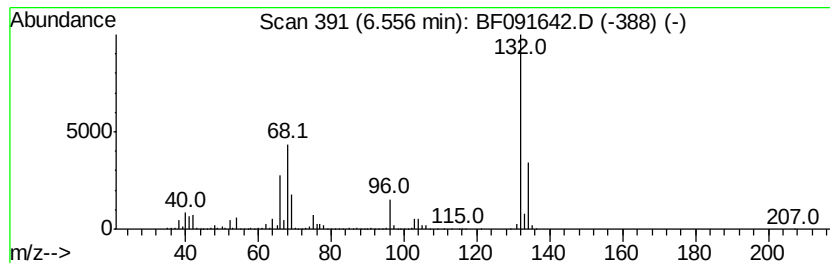

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF121516\
Data File : BF091642.D
Acq On : 15 Dec 2016 21:37
Operator : UM/SJ
Sample : H6029-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
IDW-WATER-02

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF120916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	4.94	16.1	ng	1452140	1	6.78	1807050	20.0
unknown6.56	6.56	76.1	ng	6873650	1	6.78	1807050	20.0