


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF121516\
 Data File : BF091652.D
 Acq On : 16 Dec 2016 3:39
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF120916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 16 00:35:41 2016

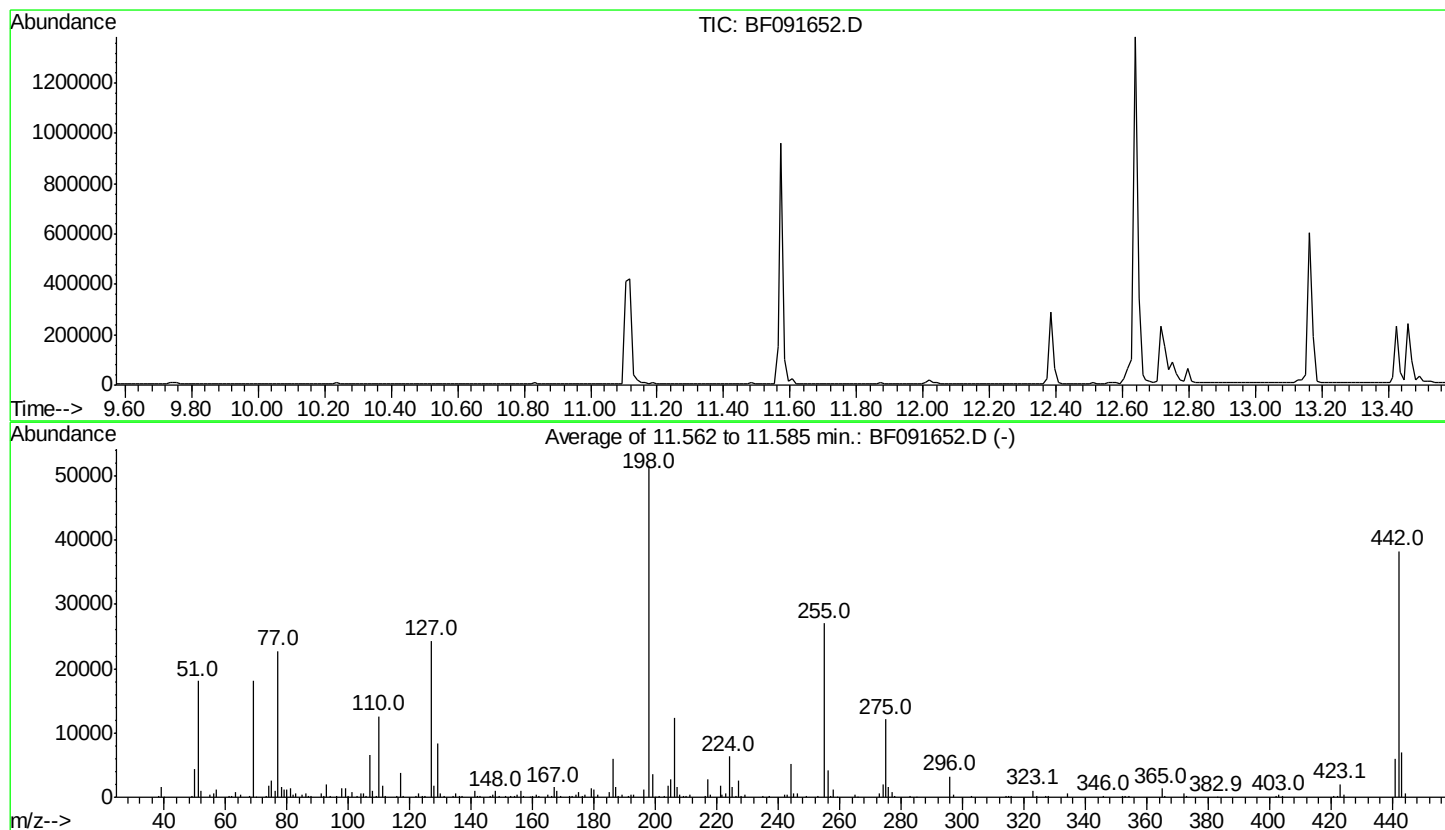

AutoFind: Scans 829, 830, 831; Background Corrected with Scan 826

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.0	18079	PASS
68	69	0.00	2	1.1	205	PASS
69	198	0.00	100	35.3	18187	PASS
70	69	0.00	2	0.6	104	PASS
127	198	10	80	47.2	24356	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	51588	PASS
199	198	5	9	6.8	3528	PASS
275	198	10	60	23.5	12100	PASS
365	198	1	100	2.6	1367	PASS
441	442	0.01	24	15.6	5988	PASS
442	198	50	100	74.2	38299	PASS
443	442	15	24	18.4	7054	PASS