

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF121517\
 Data File : BF101469.D
 Acq On : 16 Dec 2017 3:56
 Operator : SJ/JU
 Sample : I6882-06
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Dec 16 04:58:02 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 15 17:36:17 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.81	152	156372	20.00	ng	0.00
21) Naphthalene-d8	8.10	136	605311	20.00	ng	0.00
38) Acenaphthene-d10	9.85	164	246066	20.00	ng	0.00
63) Phenanthrene-d10	11.35	188	393403	20.00	ng	0.00
75) Chrysene-d12	13.99	240	287305	20.00	ng	0.00
86) Perylene-d12	15.47	264	249792	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.43	112	356454	33.96	ng	0.00
7) Phenol-d6	6.45	99	260797	19.96	ng	0.00
23) Nitrobenzene-d5	7.39	82	938240	86.28	ng	0.00
41) 2,4,6-Tribromophenol	10.65	330	176690	74.52	ng	0.00
44) 2-Fluorobiphenyl	9.17	172	1494216	94.20	ng	0.00
78) Terphenyl-d14	12.93	244	1053370	88.39	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	7.39	70	123833	14.433	ng	# 83
25) Isophorone	7.39	82	938232	43.011	ng	# 64
50) 2,6-Dinitrotoluene	9.85	165	30890	7.679	ng	# 26
56) 2,4-Dinitrotoluene	9.85	165	30890	6.816	ng	# 23
66) 4-Bromophenyl-phenylether	10.65	248	10986	2.485	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA F\DATA\BF121517\
Data File : BF101469.D
Acq On : 16 Dec 2017 3:56
Operator : SJ/JU
Sample : I6882-06
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Dec 16 04:58:02 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 15 17:36:17 2017
Response via : Initial Calibration

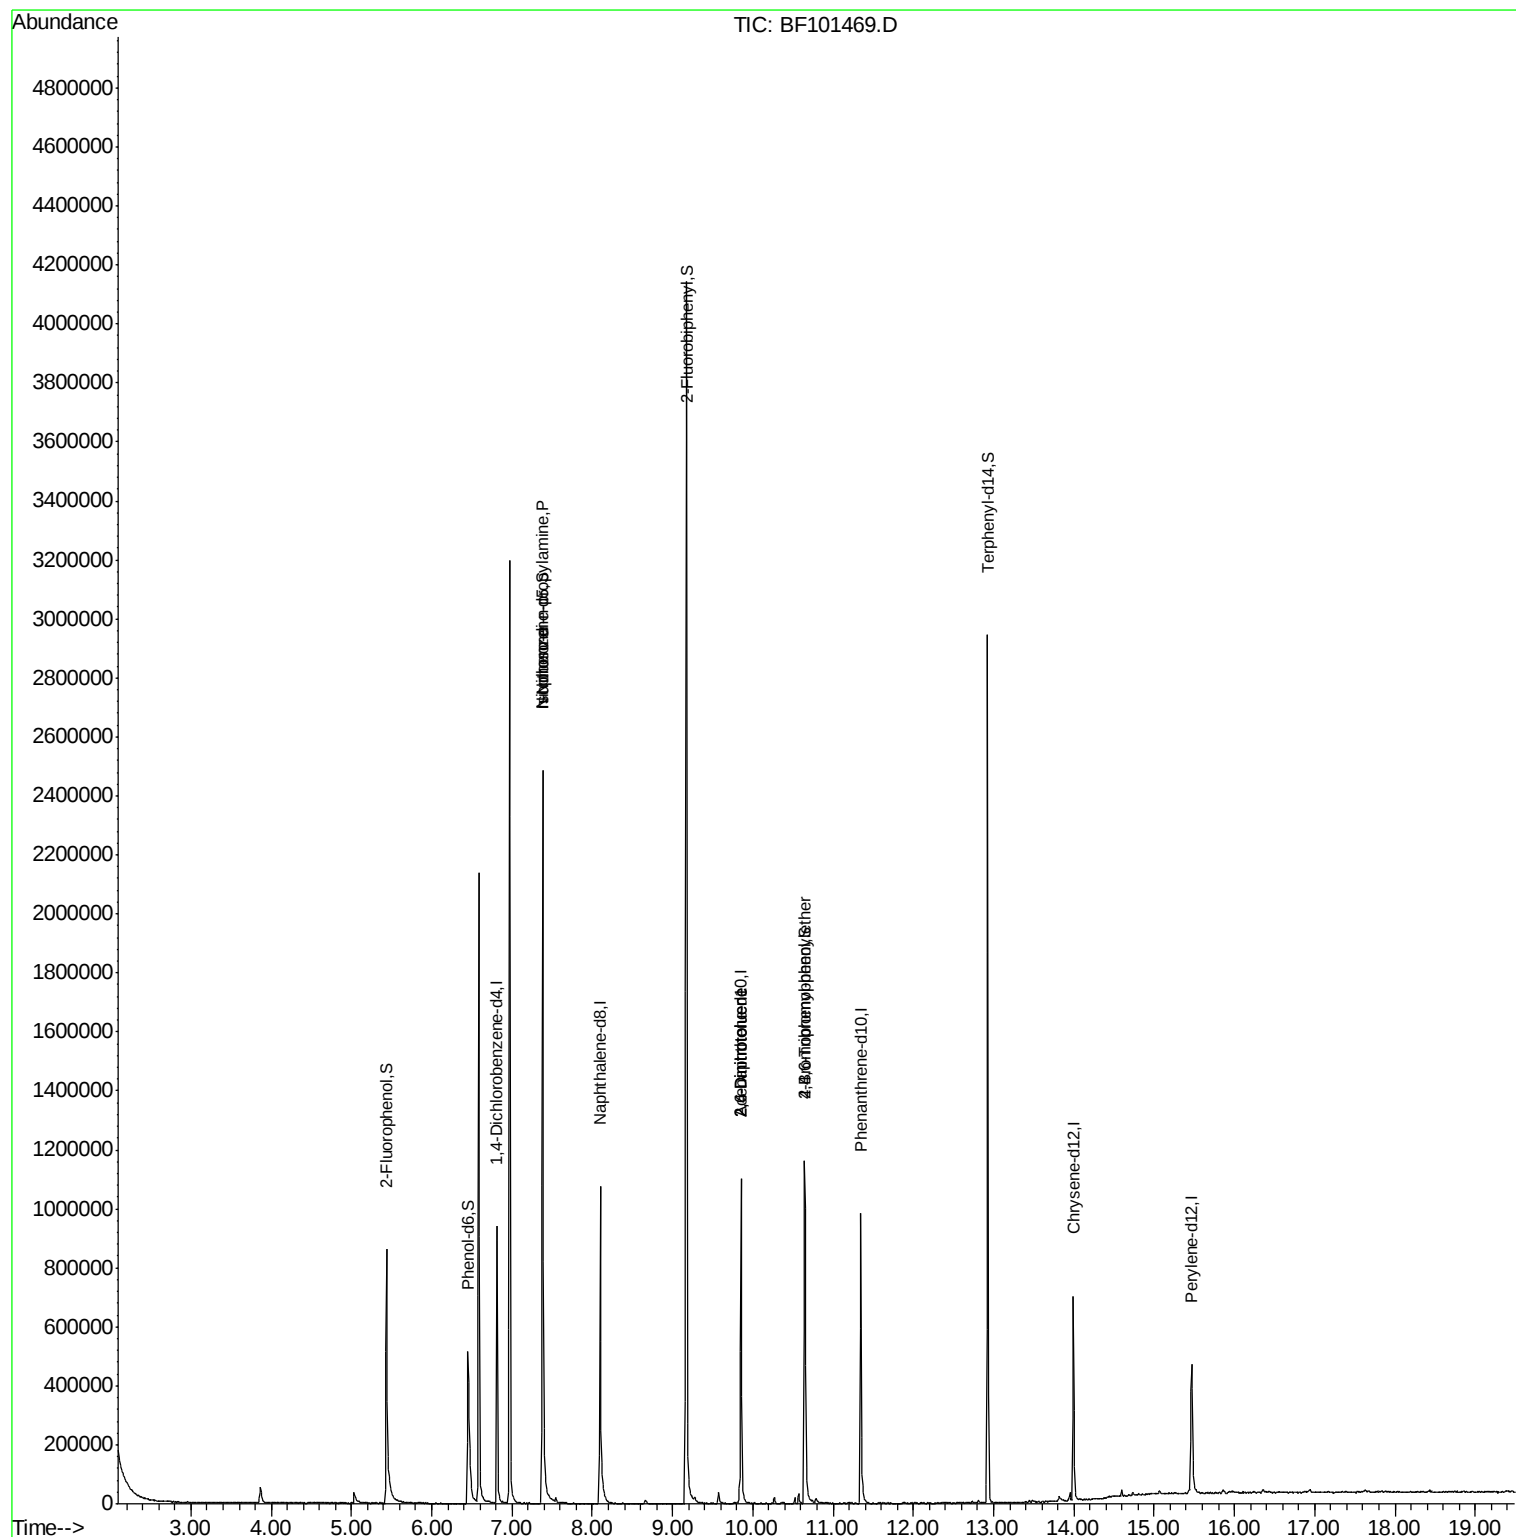




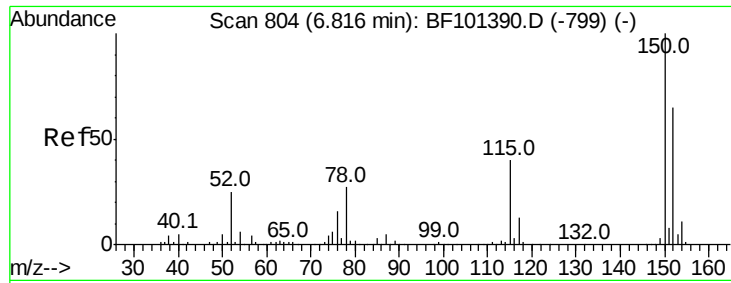


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.81 min Scan# 803
Delta R.T. -0.01 min
Lab File: BF101469.D
Acq: 16 Dec 2017 3:56

Instrument :
BNA_F
ClientSampleId :




Tot Ion:152 Resp: 156372
Ion Ratio Lower Upper
152 100
150 154.8 124.6 186.8
115 62.0 50.1 75.1

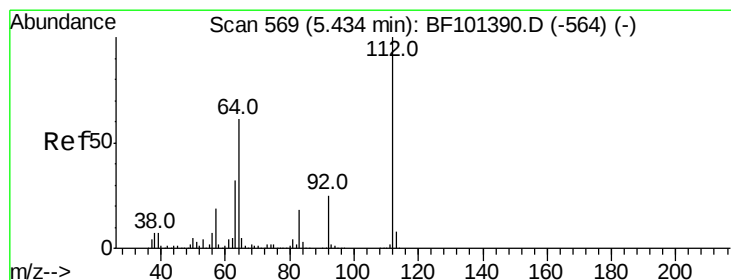
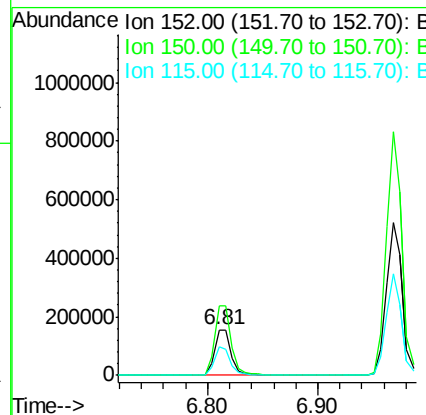
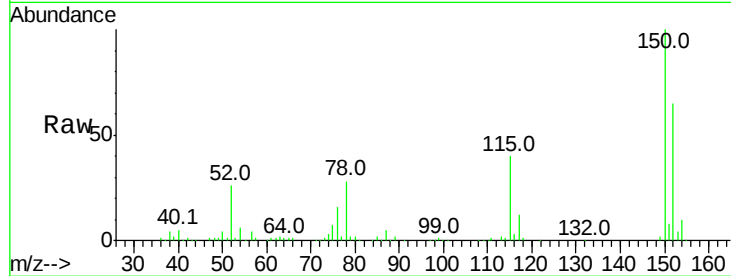


#5

2-Fluorophenol
Concen: 33.955 ng
RT: 5.43 min Scan# 569
Delta R.T. 0.01 min
Lab File: BF101469.D
Acq: 16 Dec 2017 3:56

Tgt Ion:112 Resp: 356454
Ion Ratio Lower Upper
112 100
64 61.0 47.9 71.9
63 30.6 23.7 35.5

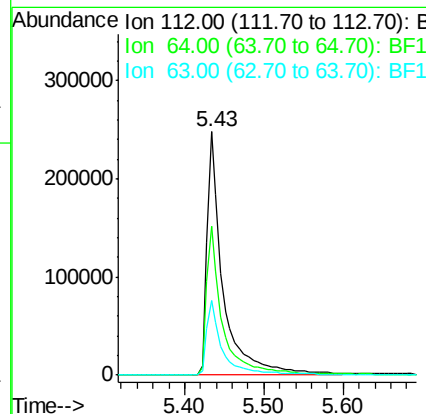

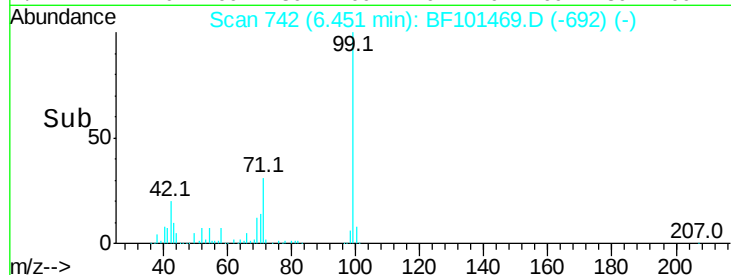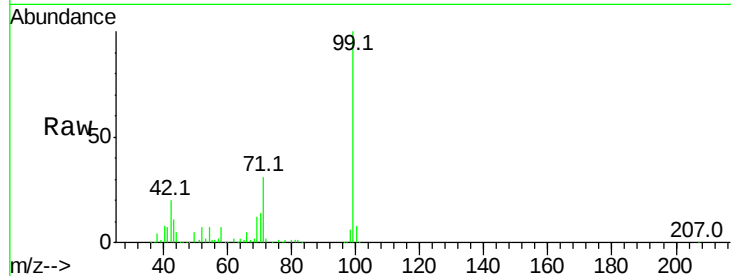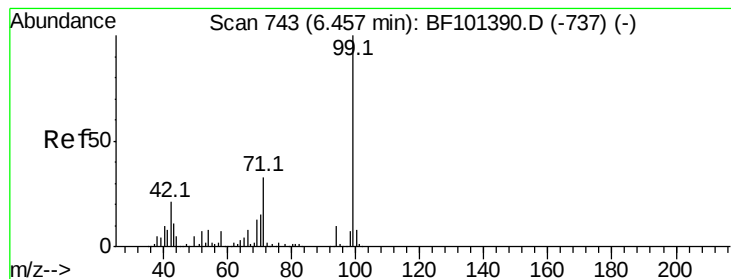

#7

Phenol-d6

Concen: 19.962 ng

RT: 6.45 min Scan# 742

Delta R.T. -0.01 min

Lab File: BF101469.D

Acq: 16 Dec 2017 3:56

Instrument :

BNA_F

ClientSampleId :





Tot Ion: 99 Resp: 260797

Ion Ratio Lower Upper

99 100

42 19.9 14.5 21.7

71 31.3 25.4 38.0

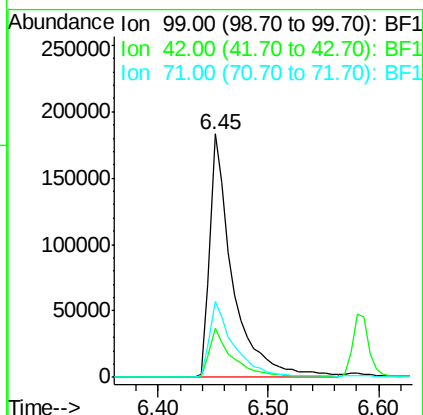

#19

n-Nitroso-di-n-propylamine

Concen: 14.433 ng

RT: 7.39 min Scan# 901

Delta R.T. 0.15 min

Lab File: BF101469.D

Acq: 16 Dec 2017 3:56

Tgt Ion: 70 Resp: 123833


Ion Ratio Lower Upper


70 100

42 53.3 47.5 71.3

101 0.0 7.4 11.2#

130 2.0 16.6 25.0#

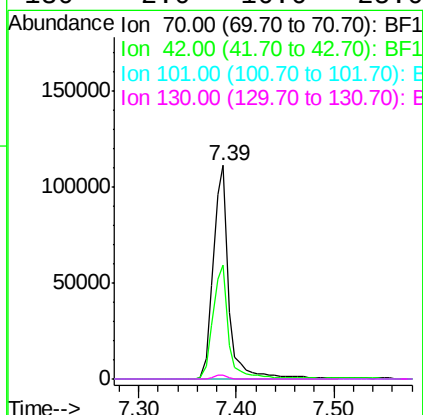


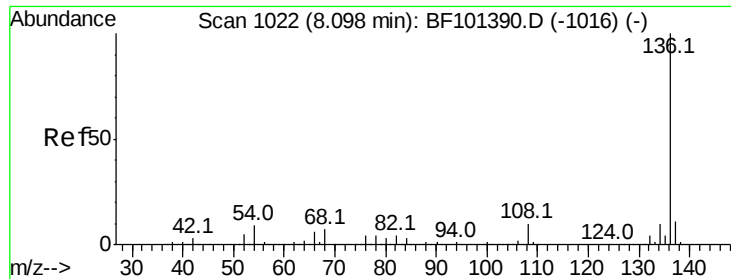




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.10 min Scan# 1022
Delta R.T. 0.00 min
Lab File: BF101469.D
Acq: 16 Dec 2017 3:56

Instrument :
BNA_F
ClientSampleId :

Tot Ion:	136	Resp:	605311
Ion	Ratio	Lower	Upper
136	100		
137	11.0	8.9	13.3
54	8.8	6.6	9.8
68	6.3	5.0	7.4

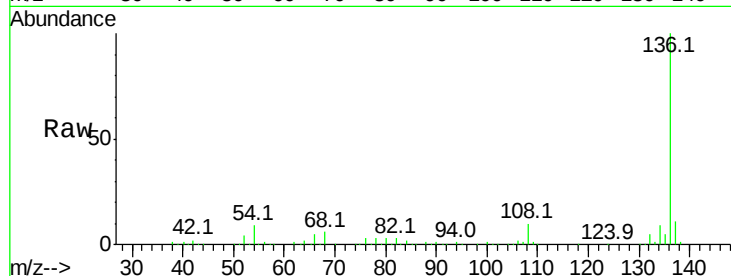


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

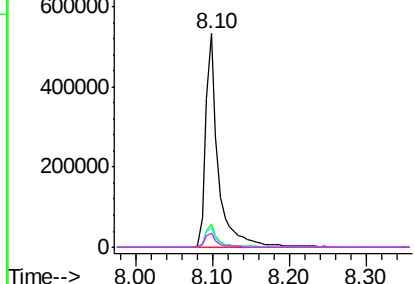




#23
Nitrobenzene-d5
Concen: 86.283 ng
RT: 7.39 min Scan# 901
Delta R.T. 0.00 min
Lab File: BF101469.D
Acq: 16 Dec 2017 3:56

Tgt Ion:	82	Resp:	938240
Ion	Ratio	Lower	Upper
82	100		
128	45.2	36.1	54.1
54	54.0	41.4	62.2



Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF1

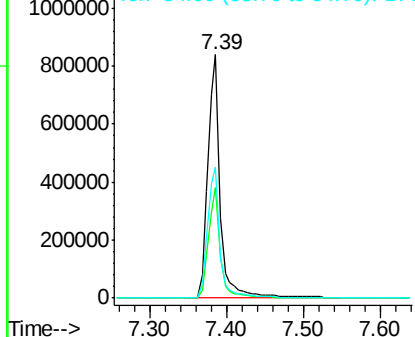

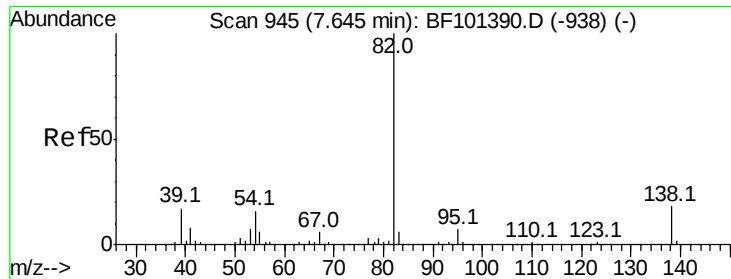

#25

Isophorone

Concen: 43.011 ng

RT: 7.39 min Scan# 901

Delta R.T. -0.25 min

Lab File: BF101469.D

Acq: 16 Dec 2017 3:56

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 82 Resp: 938232

Ion Ratio Lower Upper

82 100

95 0.0 5.2 7.8#




138 0.0 14.9 22.3#

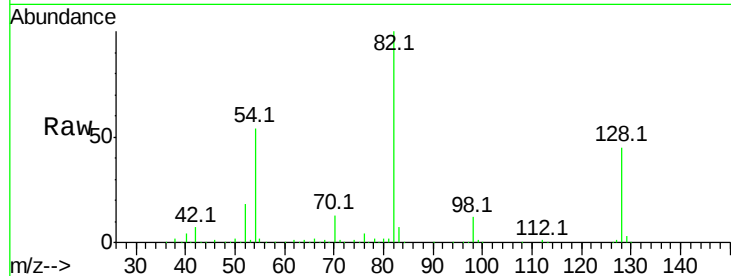

Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 95.00 (94.70 to 95.70): BF1

Ion 138.00 (137.70 to 138.70): BF1

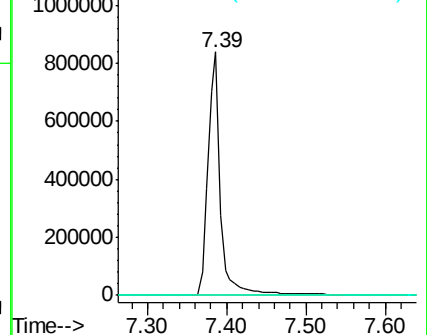

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.85 min Scan# 1320

Delta R.T. -0.01 min

Lab File: BF101469.D

Acq: 16 Dec 2017 3:56


Tgt Ion:164 Resp: 246066

Ion Ratio Lower Upper

164 100

162 102.9 86.1 129.1



160 47.7 38.3 57.5




Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

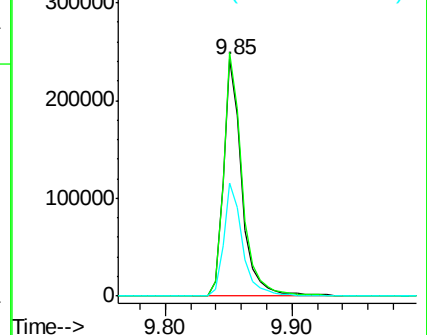


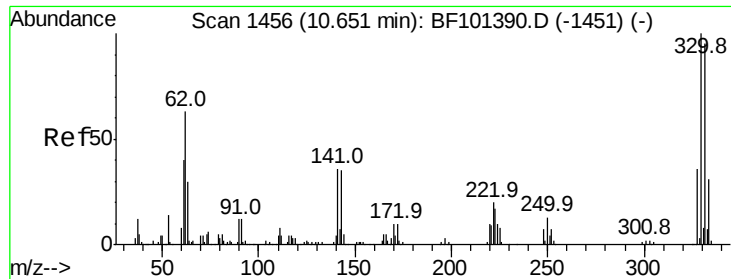




#41
 2,4,6-Tribromophenol
 Concen: 74.520 ng
 RT: 10.65 min Scan# 1456
 Delta R.T. 0.00 min
 Lab File: BF101469.D
 Acq: 16 Dec 2017 3:56

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
330	100		
332	95.7	77.0	115.6
141	33.0	29.9	44.9

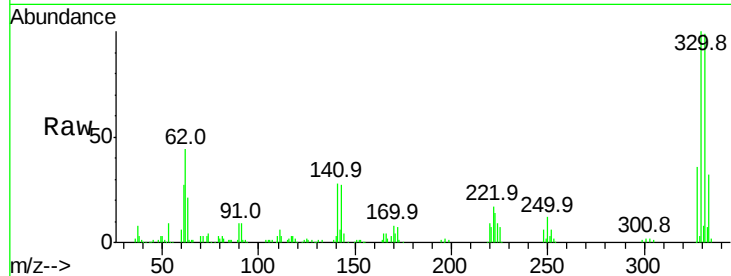


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E


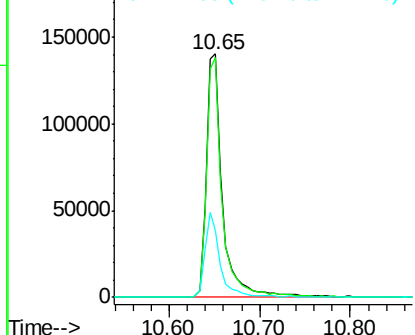



#44
 2-Fluorobiphenyl
 Concen: 94.198 ng
 RT: 9.17 min Scan# 1205
 Delta R.T. 0.00 min
 Lab File: BF101469.D
 Acq: 16 Dec 2017 3:56

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.4	29.7	44.5
170	24.2	19.6	29.4



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



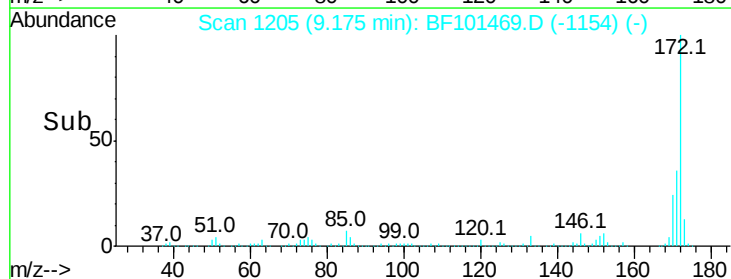
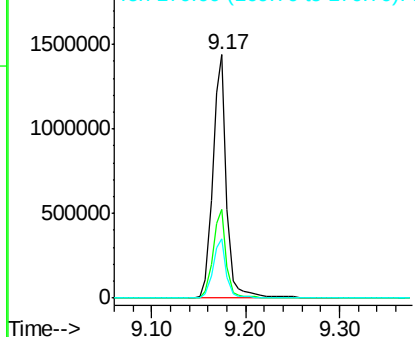




#50
2,6-Dinitrotoluene
Concen: 7.679 ng
RT: 9.85 min Scan# 1320
Delta R.T. 0.20 min
Lab File: BF101469.D
Acq: 16 Dec 2017 3:56




Instrument :
BNA_F
ClientSampleId :


Tot Ion	Ratio	Lower	Upper
165	100		
63	1.5	44.7	67.1#
89	1.3	44.0	66.0#

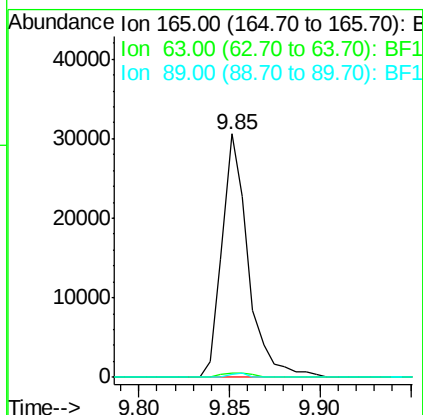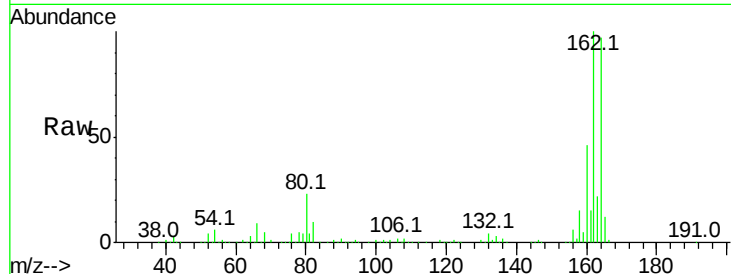

#56
2,4-Dinitrotoluene
Concen: 6.816 ng
RT: 9.85 min Scan# 1320
Delta R.T. -0.21 min
Lab File: BF101469.D
Acq: 16 Dec 2017 3:56

Tgt Ion	Ratio	Lower	Upper
165	100		
63	1.5	36.4	54.6#
89	1.3	57.8	86.6#
182	0.0	1.6	2.4#



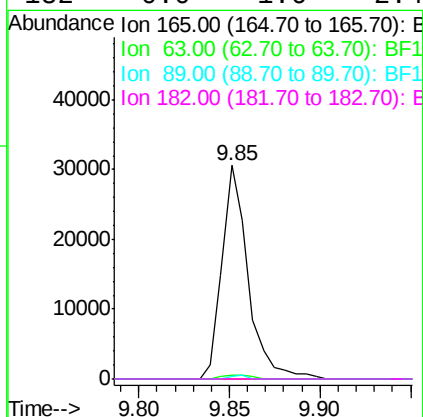





#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.35 min Scan# 1574
Delta R.T. 0.00 min
Lab File: BF101469.D
Acq: 16 Dec 2017 3:56




Instrument :
BNA_F
ClientSampleId :


Tot Ion:188 Resp: 393403
Ion Ratio Lower Upper
188 100
94 10.5 8.5 12.7
80 11.4 9.2 13.8

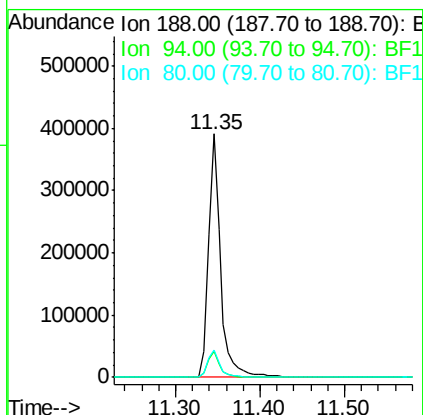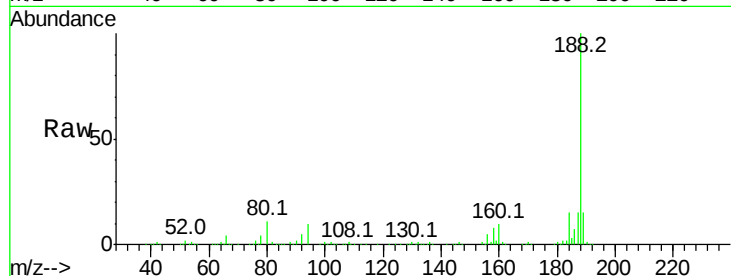

#66
4-Bromophenyl-phenylether
Concen: 2.485 ng
RT: 10.65 min Scan# 1456
Delta R.T. -0.24 min
Lab File: BF101469.D
Acq: 16 Dec 2017 3:56

Tgt Ion:248 Resp: 10986
Ion Ratio Lower Upper
248 100
250 184.7 76.9 115.3#
141 428.3 74.4 111.6#

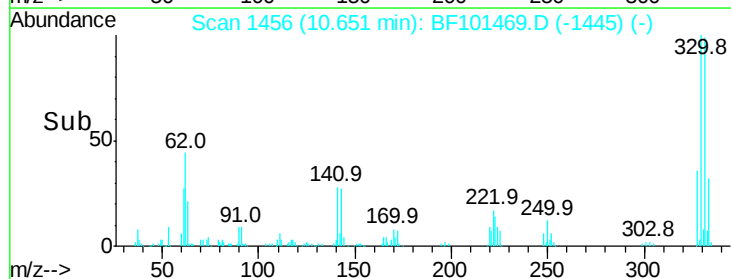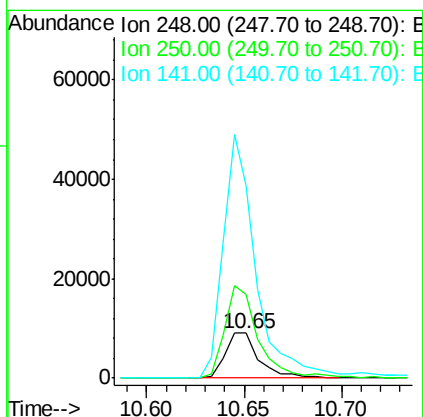



#75

Chrysene-d12

Concen: 20.000 ng

RT: 13.99 min Scan# 2024

Delta R.T. -0.01 min

Lab File: BF101469.D

Acq: 16 Dec 2017 3:56

Instrument :

BNA_F

ClientSampleId :


Tot Ion:240 Resp: 287305

Ion Ratio Lower Upper

240 100

120 13.2 9.5 14.3




236 24.7 20.7 31.1



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

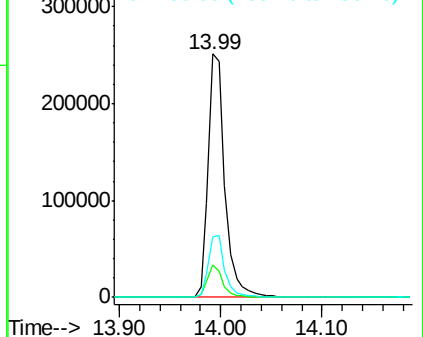

#78

Terphenyl-d14

Concen: 88.388 ng

RT: 12.93 min Scan# 1843

Delta R.T. -0.01 min

Lab File: BF101469.D

Acq: 16 Dec 2017 3:56


Tgt Ion:244 Resp: 1053370

Ion Ratio Lower Upper

244 100

212 7.3 5.4 8.0



122 12.3 11.0 16.4




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

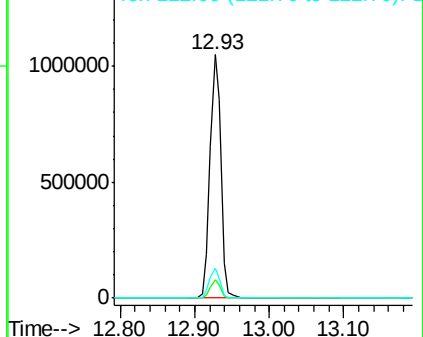


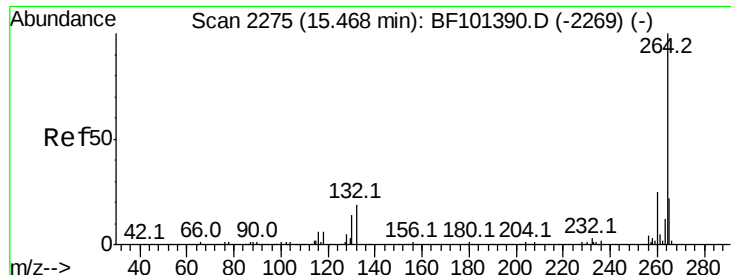

#86
Pervlene-d12
Concen: 20.000 ng
RT: 15.47 min Scan# 2275
Delta R.T. 0.00 min
Lab File: BF101469.D
Acq: 16 Dec 2017 3:56

Instrument :
BNA_F
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.3	19.2	28.8
265	21.6	17.5	26.3



Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

