

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF121517\
 Data File : BF101466.D
 Acq On : 16 Dec 2017 2:36
 Operator : SJ/JU
 Sample : I6882-03
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 121117-JETT-E-U-B

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.846	296	299	313	rBV2	33910	99983	2.43%	0.417%
2	5.034	498	501	512	rBV	30452	64504	1.57%	0.269%
3	5.434	566	569	595	rBV	685578	1056166	25.65%	4.403%
4	6.457	739	743	761	rBV2	349512	622643	15.12%	2.596%
5	6.587	761	765	778	rVV	1990153	2046274	49.70%	8.531%
6	6.816	800	804	812	rBV	888212	879672	21.37%	3.667%
7	6.969	826	830	846	rBV	3042116	3115875	75.68%	12.990%
8	7.387	896	901	924	rBV	2516447	2697136	65.51%	11.244%
9	7.716	954	957	961	rBV	68069	91265	2.22%	0.380%
10	7.751	961	963	973	rVV2	31634	73268	1.78%	0.305%
11	7.845	975	979	991	rVB2	23277	53588	1.30%	0.223%
12	8.098	1018	1022	1043	rBV	1065385	1162084	28.22%	4.845%
13	8.598	1104	1107	1115	rBV	58096	72351	1.76%	0.302%
14	8.969	1167	1170	1174	rBV5	47643	82355	2.00%	0.343%
15	9.004	1174	1176	1187	rVB5	24306	53373	1.30%	0.223%
16	9.175	1200	1205	1208	rBV	4180423	4117260	100.00%	17.164%
17	9.616	1277	1280	1292	rBV6	17787	47096	1.14%	0.196%
18	9.851	1317	1320	1335	rVB	1117431	1133196	27.52%	4.724%
19	10.569	1438	1442	1451	rVB	51274	50683	1.23%	0.211%
20	10.645	1451	1455	1466	rBV	1150243	1264224	30.71%	5.270%
21	11.269	1557	1561	1570	rVB	39525	62341	1.51%	0.260%
22	11.345	1570	1574	1587	rBV	1037249	991598	24.08%	4.134%
23	12.927	1839	1843	1847	rBV	2892051	2959462	71.88%	12.338%
24	13.998	2021	2025	2034	rBV	718825	769709	18.69%	3.209%
25	15.474	2272	2276	2289	rVB2	150971	243415	5.91%	1.015%
26	18.392	2763	2772	2779	rBV3	56061	177822	4.32%	0.741%


Sum of corrected areas: 23987343

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF121517\
Data File : BF101466.D
Acq On : 16 Dec 2017 2:36
Operator : SJ/JU
Sample : I6882-03
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
121117-JETT-E-U-B

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

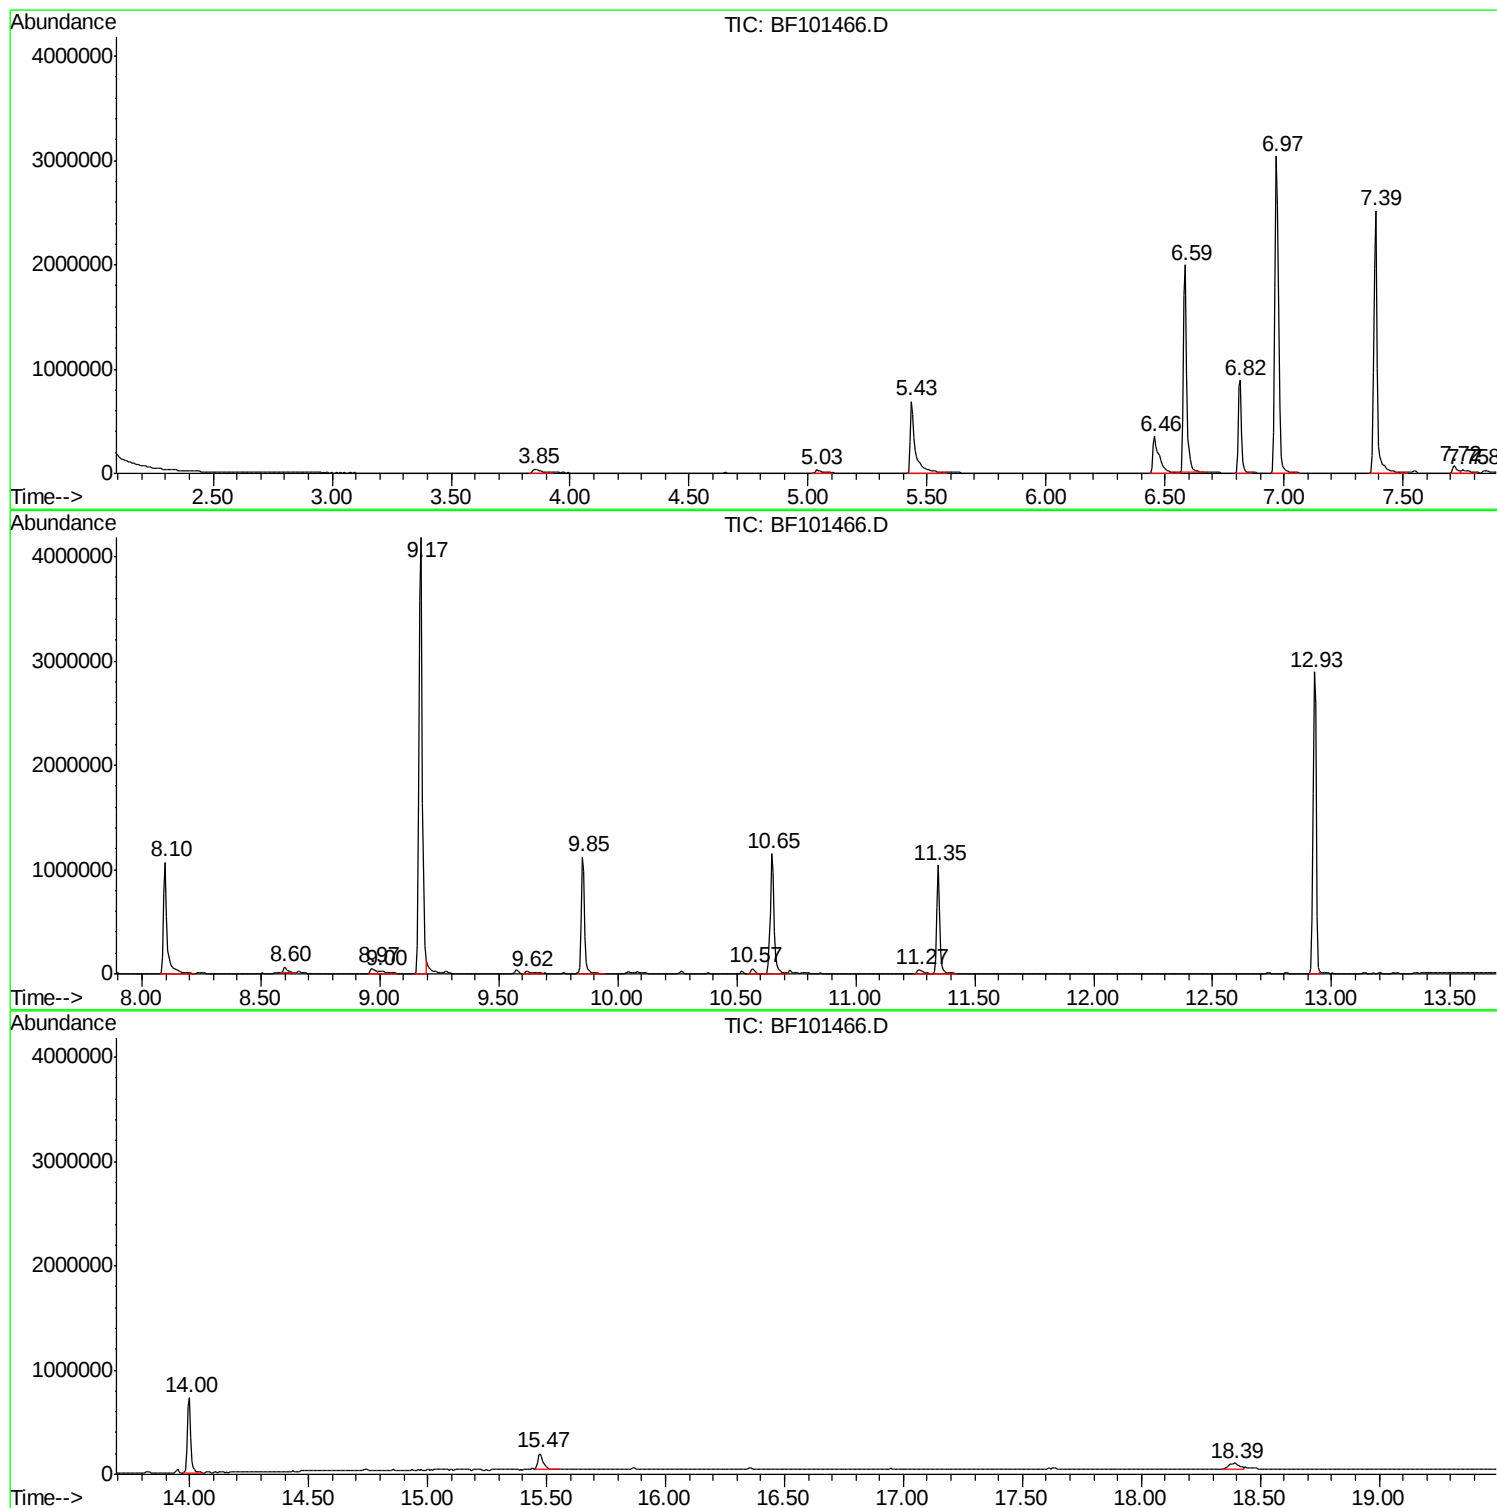

DbaaaPathh::ZZ\NRPBHM1BNAFNDAAABBE22551X\
 DbaaaFile::BBEQ01066DD
 Aeqq00n ::106DDec2007 22386
 Opeaaor ::SSJUU
 Sample ::I08822003
 Misc ::
 ASSVaal ::227 SampleMultiplier:11

Instrument :
 BNA_F
 ClientSampleId :
 121117-JETT-E-U-B

QqaabMebbdd::ZZ\NRPBHM1BNAFMEH00S8200BBE22447MM
 QqaabTfile ::ASBPBNASSANDABBSF00R55P000NTCALIBRATION

TICCLibbaay ::CC\DAABASSEN0\$T11LL
 TICIntegratíonPaaameess:LS6CNTTP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
