

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF121517\
 Data File : BF101468.D
 Acq On : 16 Dec 2017 3:29
 Operator : SJ/JU
 Sample : I6882-05
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 121117-TIDO-E-D-M

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.863	297	302	313	rBV	35076	63725	1.54%	0.236%
2	5.034	498	501	512	rBV	35931	72932	1.77%	0.270%
3	5.434	565	569	593	rBV	909759	1327538	32.15%	4.919%
4	6.451	739	742	761	rBV2	574638	931895	22.57%	3.453%
5	6.587	761	765	772	rBV	2313434	2325731	56.32%	8.618%
6	6.816	800	804	813	rBV	922255	916889	22.20%	3.398%
7	6.969	826	830	847	rBV	3169082	3128759	75.77%	11.594%
8	7.386	896	901	926	rBV	2408363	2704927	65.50%	10.023%
9	8.098	1018	1022	1046	rBV	1056862	1214837	29.42%	4.502%
10	8.910	1150	1160	1169	rBV	74722	93584	2.27%	0.347%
11	9.175	1200	1205	1208	rBV	4186314	4129501	100.00%	15.302%
12	9.275	1219	1222	1230	rVB	56006	65554	1.59%	0.243%
13	9.569	1270	1272	1277	rVB	44583	48514	1.17%	0.180%
14	9.851	1317	1320	1323	rBV2	1171635	1053643	25.52%	3.904%
15	9.886	1323	1326	1333	rVB	384659	384847	9.32%	1.426%
16	10.063	1351	1356	1366	rBV	137144	154909	3.75%	0.574%
17	10.404	1411	1414	1420	rBV	167961	153821	3.72%	0.570%
18	10.569	1438	1442	1449	rVB2	55499	70789	1.71%	0.262%
19	10.645	1451	1455	1470	rBV	1396446	1595142	38.63%	5.911%
20	11.345	1570	1574	1583	rBV	1115819	1109913	26.88%	4.113%
21	11.427	1585	1588	1593	rVB	37350	43189	1.05%	0.160%
22	11.592	1613	1616	1622	rBV	37646	45799	1.11%	0.170%
23	11.963	1676	1679	1688	rVB3	46587	60280	1.46%	0.223%
24	12.563	1778	1781	1787	rBV	188582	177713	4.30%	0.659%
25	12.792	1814	1820	1827	rBV	97910	128653	3.12%	0.477%
26	12.927	1839	1843	1847	rBV	2955229	2985509	72.30%	11.063%
27	13.815	1990	1994	2002	rBV5	28931	56175	1.36%	0.208%
28	13.992	2020	2024	2035	rBV	734468	824404	19.96%	3.055%
29	15.439	2266	2270	2271	rBV	53252	58705	1.42%	0.218%
30	15.468	2271	2275	2286	rVB	484857	708078	17.15%	2.624%
31	15.862	2338	2342	2348	rVB2	57038	81604	1.98%	0.302%
32	16.356	2421	2426	2431	rBV3	62822	104812	2.54%	0.388%
33	16.939	2518	2525	2532	rBV3	45109	91896	2.23%	0.341%
34	17.621	2636	2641	2649	rVB3	31021	71724	1.74%	0.266%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF121517\
Data File : BF101468.D
Acq On : 16 Dec 2017 3:29
Operator : SJ/JU
Sample : I6882-05
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
121117-TIDO-E-D-M

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION


Sum of corrected areas: 26985991

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF121517\
Data File : BF101468.D
Acq On : 16 Dec 2017 3:29
Operator : SJ/JU
Sample : I6882-05
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
121117-TIDO-E-D-M

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

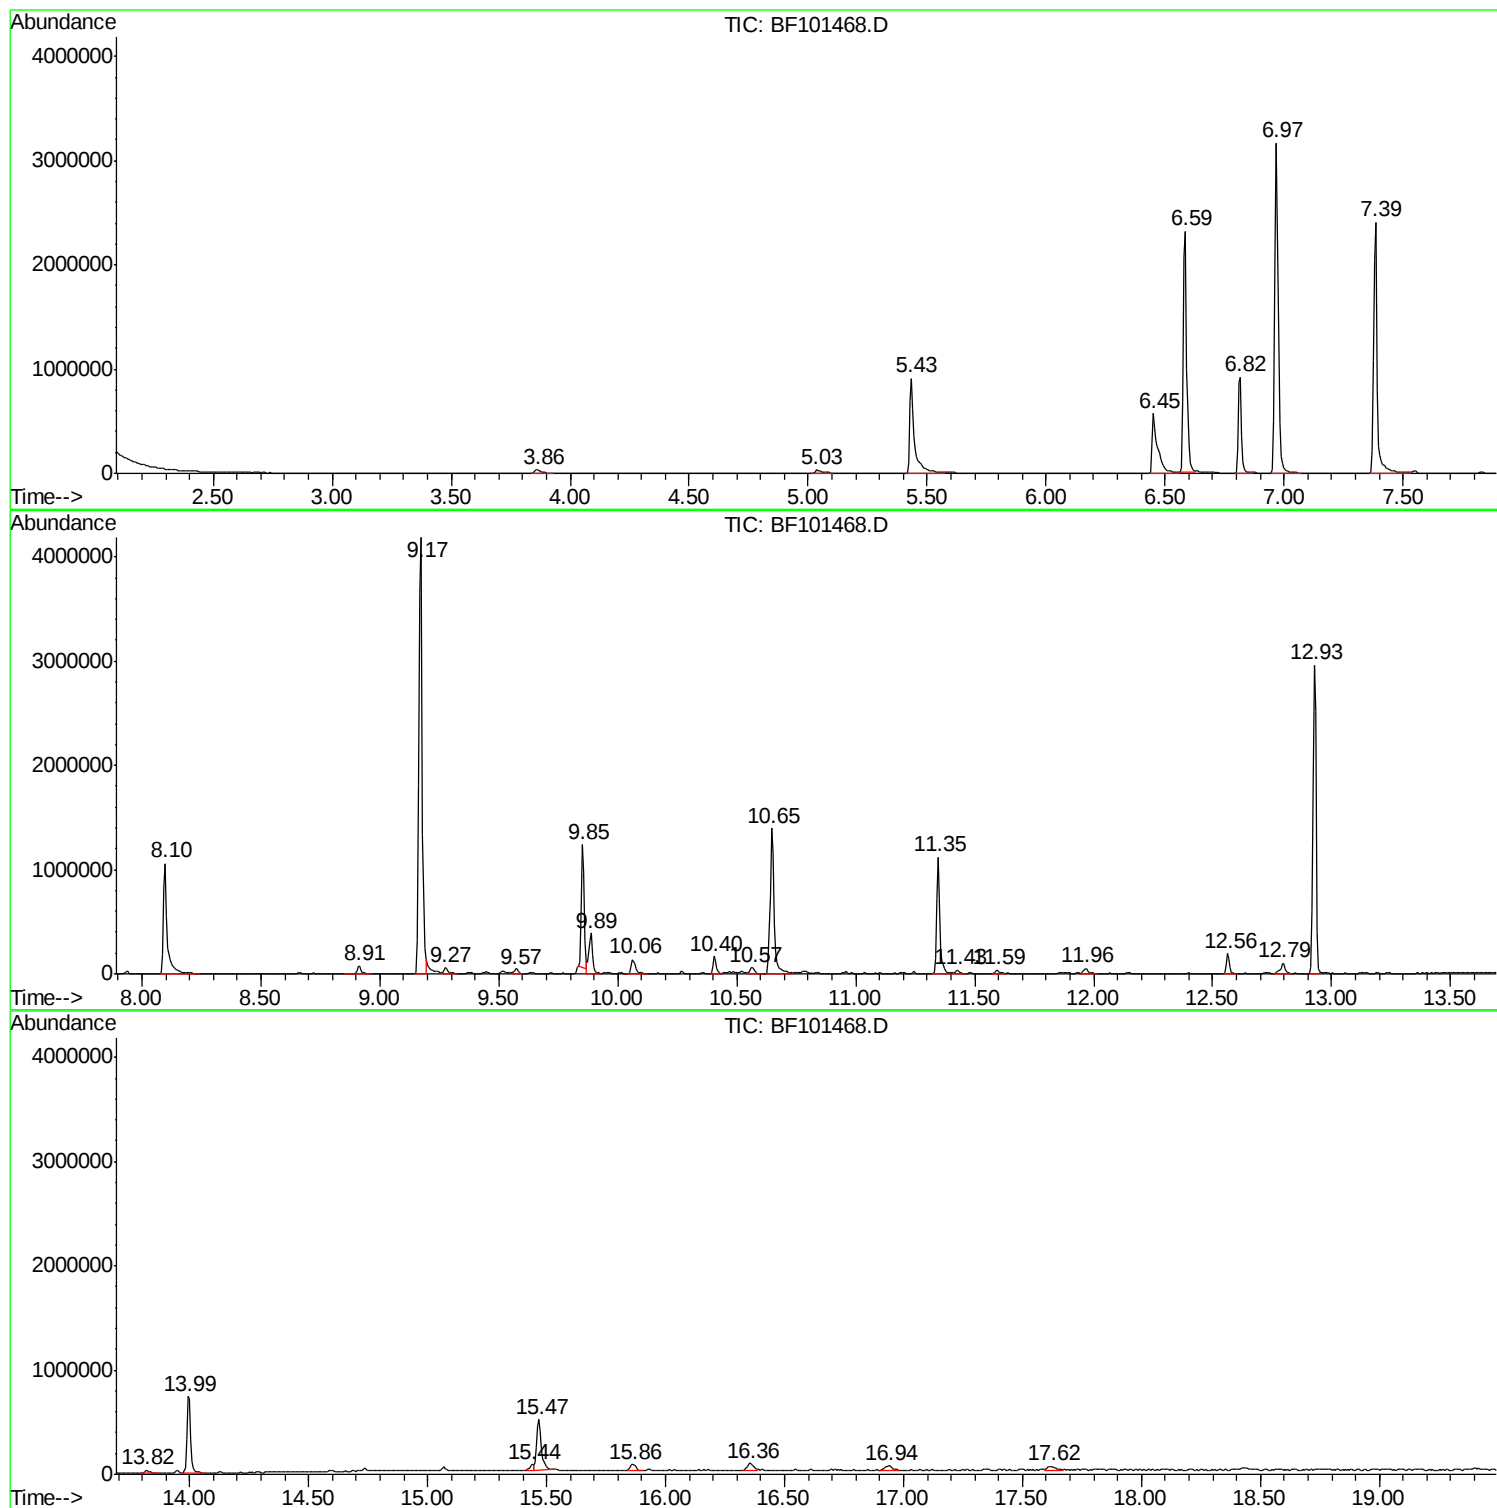

DbaaaPath::ZZ\NRPBMM1BNAFNDAAABBE22551X\
 DbaaaFile::BBE001088DD
 AcqQ00n ::166DDec2007 33299
 Operator::SJUU
 Sample::I6882005
 Misc::
 ASSVaal::299 SampleMultiplier:11

Instrument :
 BNA_F
 ClientSampleId :
 121117-TIDO-E-D-M

QqaabMebbdd::ZZ\NRPBMM1BNAFMEH00S8200BBE22447MM
 QqaabTitle::ASBPBNASSANDABBSF00R55P000NTCALIBRATION

TICLibrary::CC\DATAABSENDSST11LL
 TICIntegratIonParameters:LS6CNTTP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
