

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF121517\
 Data File : BF101471.D
 Acq On : 16 Dec 2017 4:50
 Operator : SJ/JU
 Sample : I6882-08
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 121117-FOPI-E-U-M

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.034	498	501	516	rBV	40696	84587	1.98%	0.337%
2	5.434	566	569	591	rBV	937600	1287712	30.17%	5.124%
3	6.451	739	742	761	rBV	571582	907572	21.26%	3.612%
4	6.587	761	765	777	rVV	2145880	2292500	53.71%	9.123%
5	6.810	800	803	814	rBV	950694	961492	22.53%	3.826%
6	6.969	826	830	849	rVB	3148899	3137333	73.51%	12.485%
7	7.386	896	901	925	rBV	2436873	2734040	64.06%	10.880%
8	8.098	1018	1022	1041	rBV	1082355	1260418	29.53%	5.016%
9	9.175	1200	1205	1220	rBV	4030485	4268005	100.00%	16.985%
10	9.575	1268	1273	1280	rBV	57440	70006	1.64%	0.279%
11	9.851	1317	1320	1335	rVB2	1102152	1217676	28.53%	4.846%
12	10.569	1438	1442	1452	rBV	48567	52820	1.24%	0.210%
13	10.645	1452	1455	1475	rBV	1252316	1431548	33.54%	5.697%
14	11.345	1570	1574	1592	rBV	1012072	1077161	25.24%	4.287%
15	12.927	1839	1843	1847	rBV	2962240	2877059	67.41%	11.449%
16	13.998	2021	2025	2032	rBV	705053	809291	18.96%	3.221%
17	15.468	2270	2275	2284	rVB	458889	659577	15.45%	2.625%


Sum of corrected areas: 25128797

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF121517\
Data File : BF101471.D
Acq On : 16 Dec 2017 4:50
Operator : SJ/JU
Sample : I6882-08
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
121117-FOPI-E-U-M

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

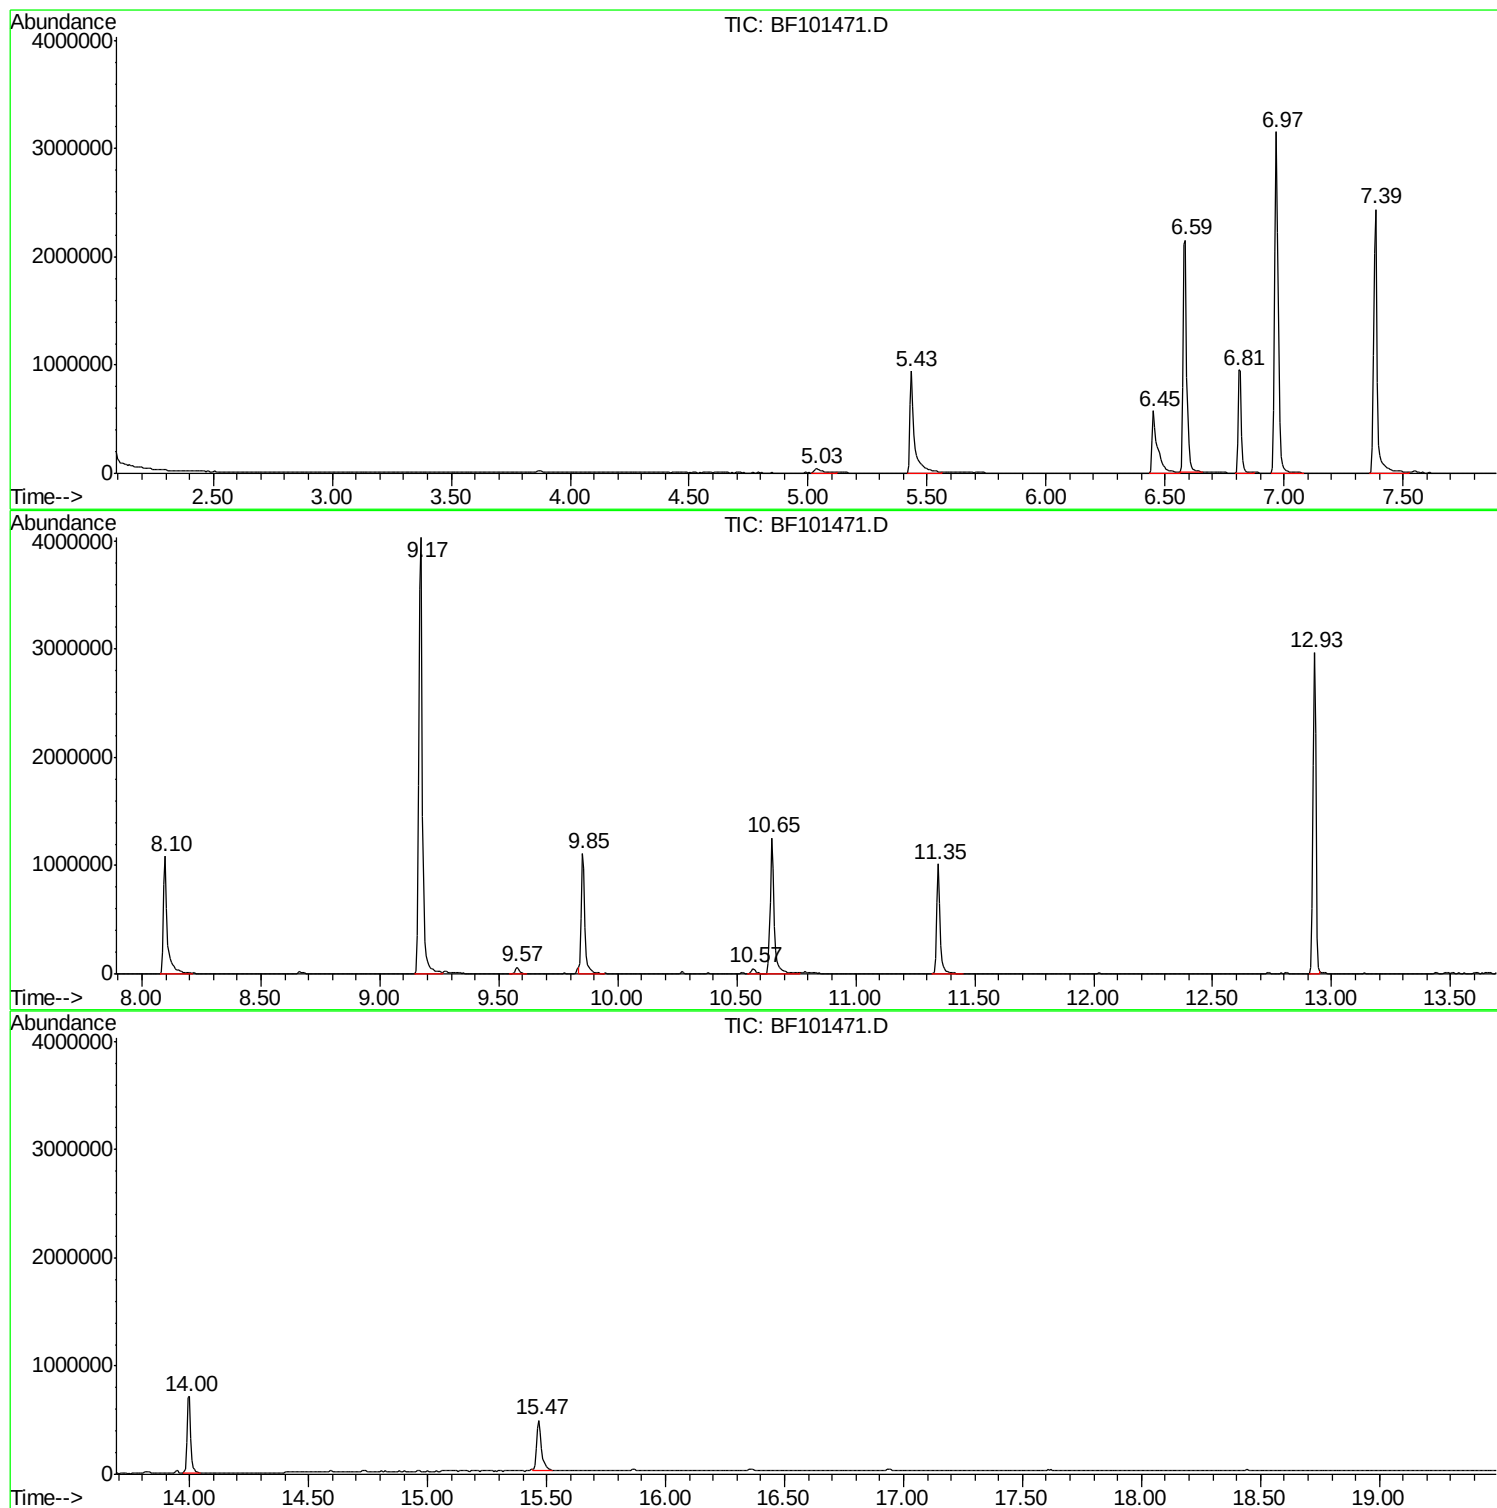

DbaaaPbath::ZZ\NRPBEMM\BBAFNDAAABBE2255IX\
 DbaaaFfile::BBEQ047I1DD
 Aeqq00n ::166DDec2007 44500
 Opeaaor ::SSJUU
 Samplee ::I6882008
 Misc ::
 AASSVaal ::322 SampleeMMultiplier:11

Instrument :
 BNA_F
 ClientSampleId :
 121117-FOPI-E-U-M

QqaabMebbdd::ZZ\NRPBEMM\BBAFMEH00S88200BBE22447MM
 QqaabTfile ::ASBPBNASSANDABBSF00R55P000NTCABBRATION

TICCLibbaay ::CC\DAABASSEN0\$T11LL
 TICInteggaionPaaameess:LS6CNTTP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
