


Data Path : Z:\HPCHEM1\BNA_F\Data\BF121517\
 Data File : BF101438.D
 Acq On : 15 Dec 2017 12:37
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 15 17:36:17 2017

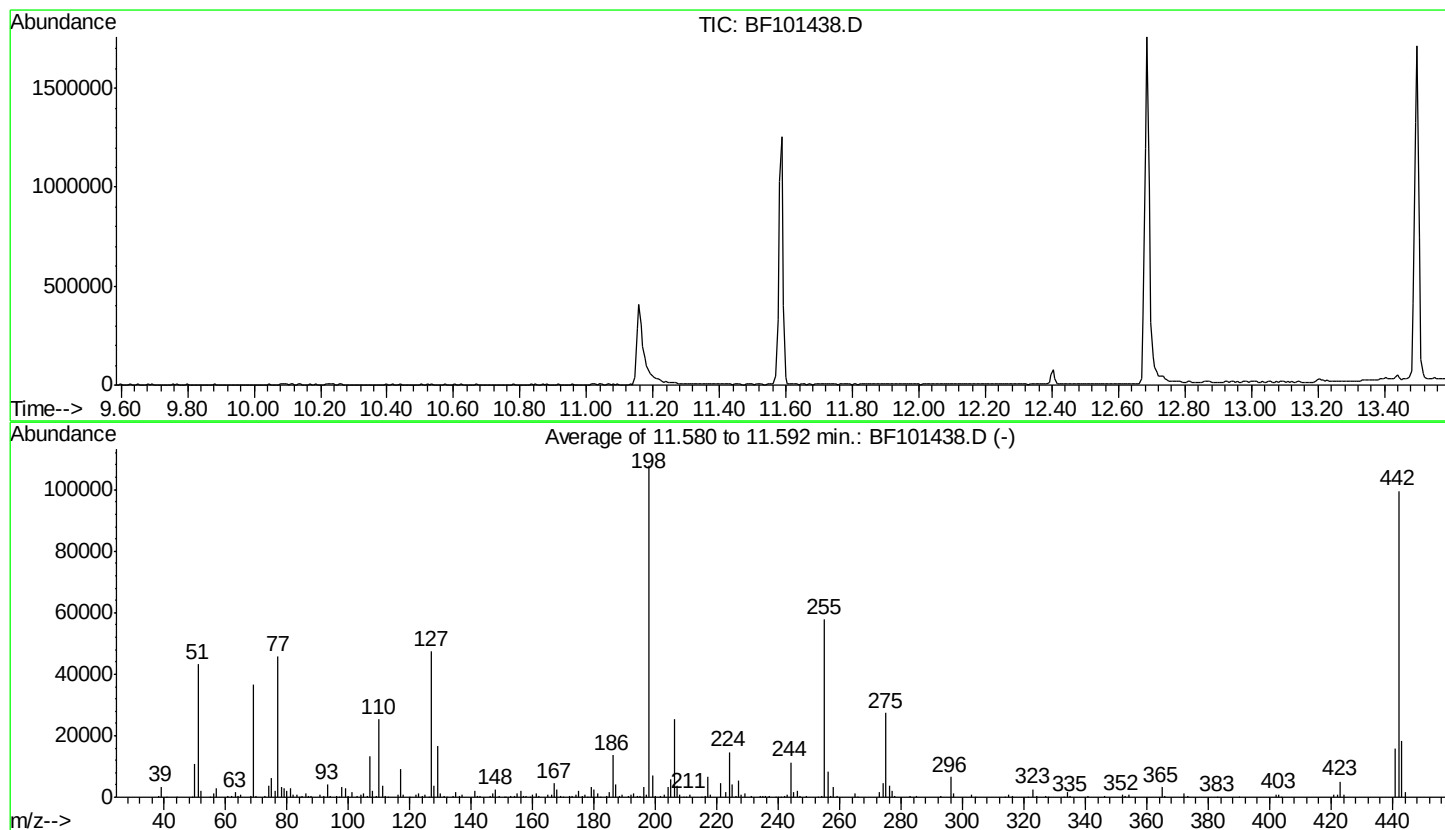

AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.1	43176	PASS
68	69	0.00	2	1.2	455	PASS
69	198	0.00	100	34.1	36753	PASS
70	69	0.00	2	0.6	235	PASS
127	198	10	80	43.9	47364	PASS
197	198	0.00	2	0.8	842	PASS
198	198	100	100	100.0	107792	PASS
199	198	5	9	6.6	7103	PASS
275	198	10	60	25.3	27273	PASS
365	198	1	100	3.0	3181	PASS
441	443	0.01	100	86.7	15718	PASS
442	198	50	100	92.4	99562	PASS
443	442	15	24	18.2	18135	PASS