


Data Path : Z:\HPCHEM1\BNA_F\Data\BF121517\
Data File : BF101464.D
Acq On : 16 Dec 2017 1:42
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Dec 15 17:36:17 2017

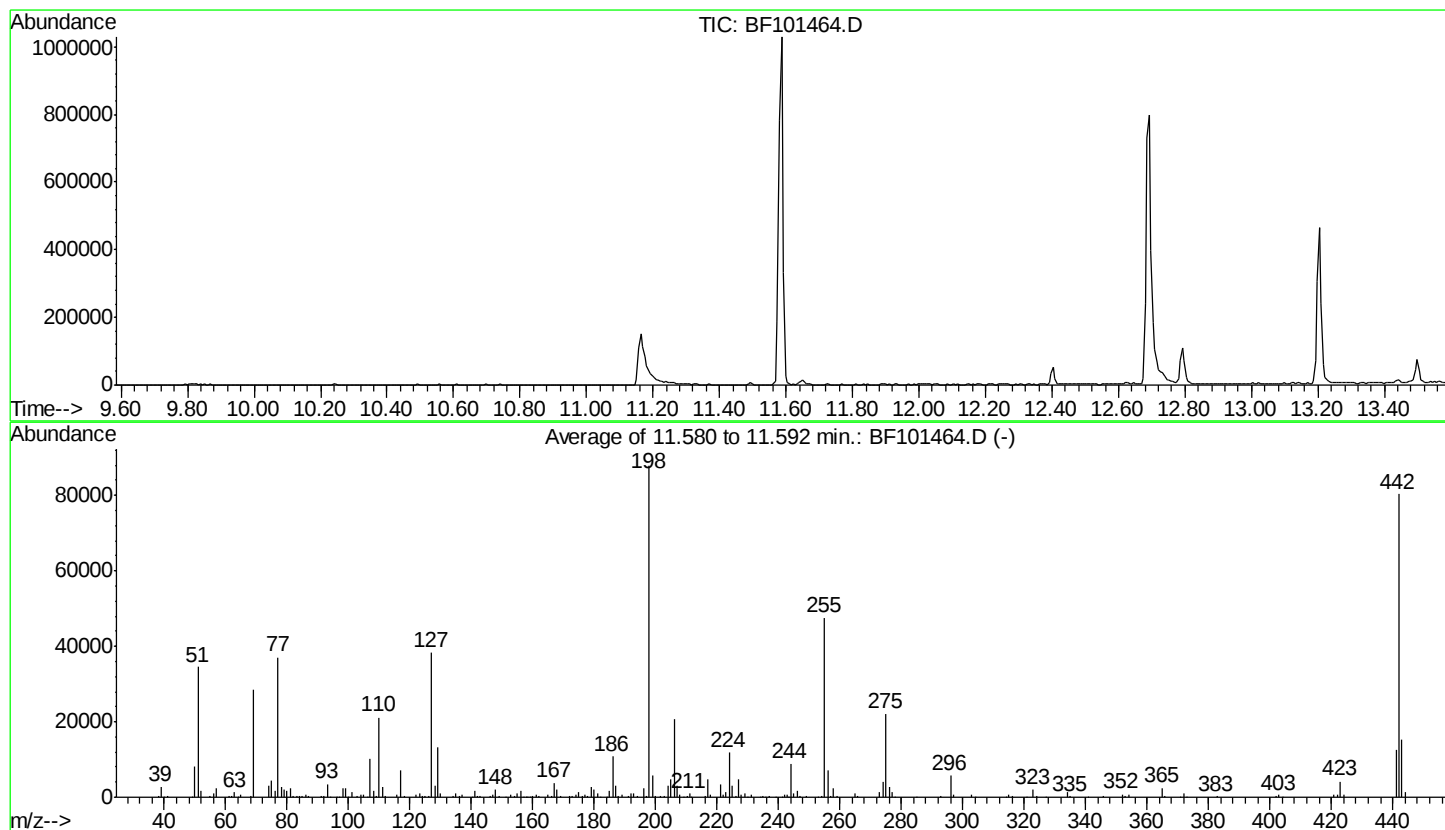

AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.2	34493	PASS
68	69	0.00	2	1.8	504	PASS
69	198	0.00	100	32.6	28613	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.5	38200	PASS
197	198	0.00	2	0.3	259	PASS
198	198	100	100	100.0	87898	PASS
199	198	5	9	6.4	5616	PASS
275	198	10	60	25.1	22096	PASS
365	198	1	100	2.9	2551	PASS
441	443	0.01	100	82.0	12576	PASS
442	198	50	100	91.4	80309	PASS
443	442	15	24	19.1	15342	PASS