
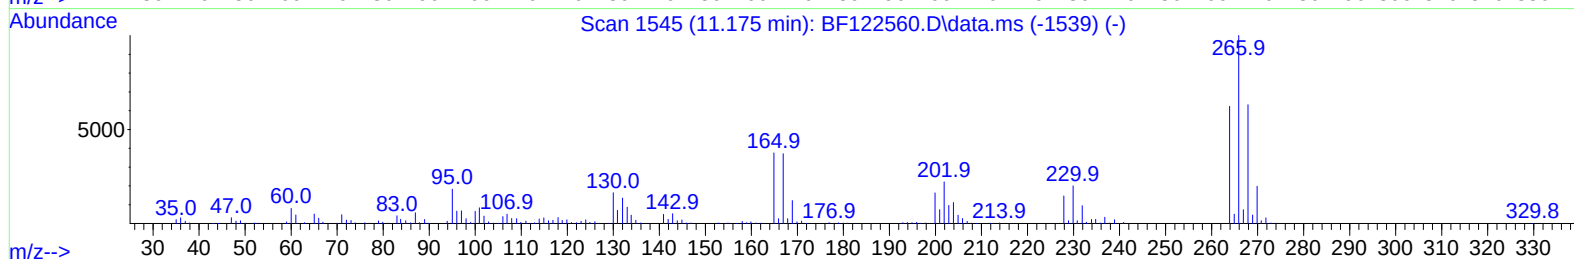
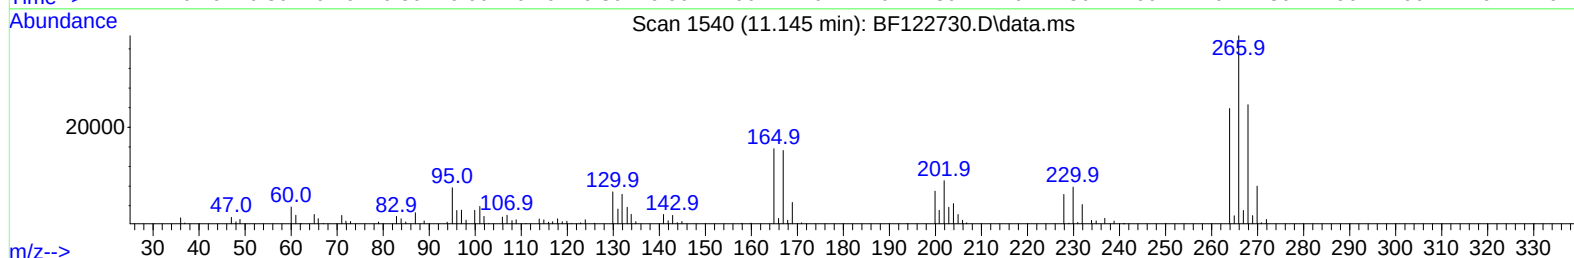


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121520\
Data File : BF122730.D
Acq On : 15 Dec 2020 23:19
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 16 06:21:13 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 15 18:14:23 2020
Response via : Initial Calibration

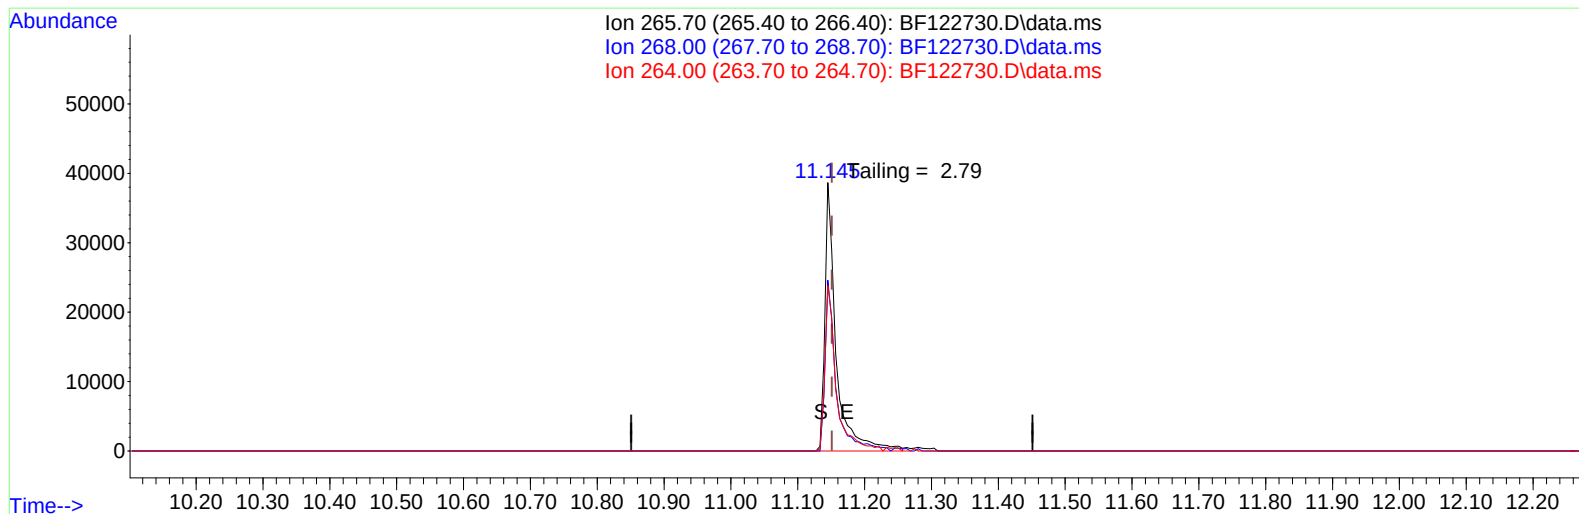

TIC: BF122730.D\data.ms

(70) Pentachlorophenol (C)




11.145min (-0.006) 53804.12 ng

response 45692

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.63
264.00	62.30	61.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121520\
Data File : BF122730.D
Acq On : 15 Dec 2020 23:19
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 16 06:21:13 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 15 18:14:23 2020
Response via : Initial Calibration

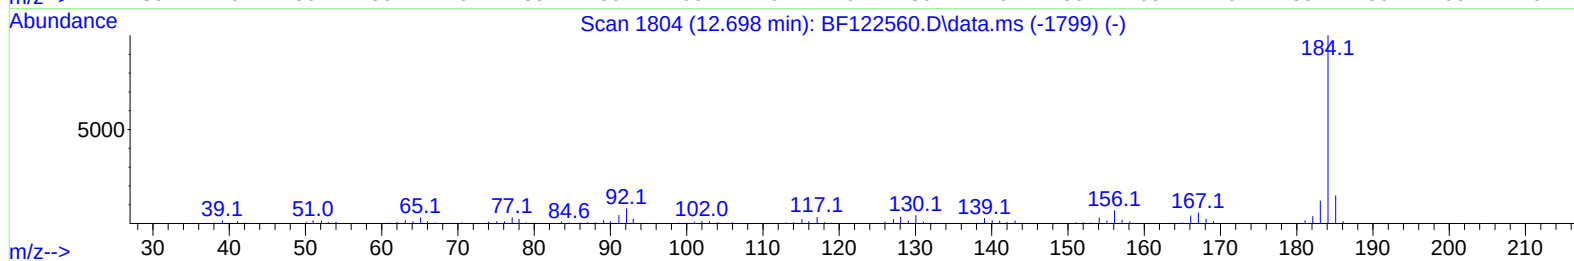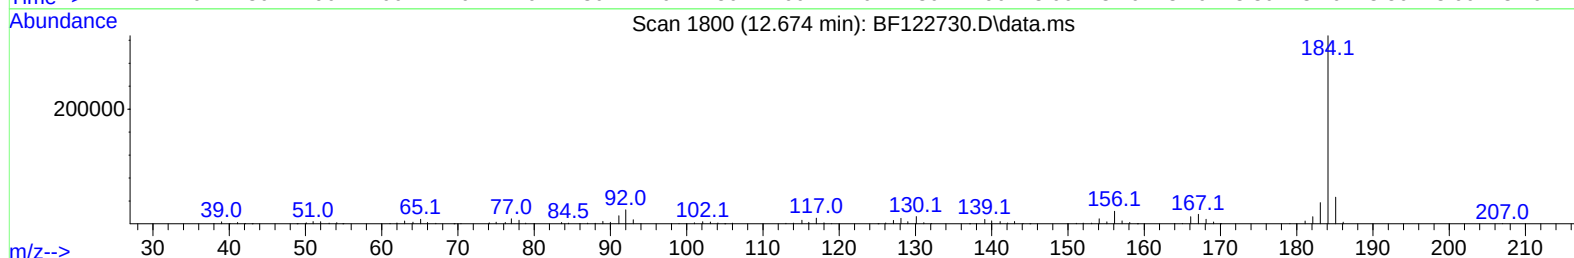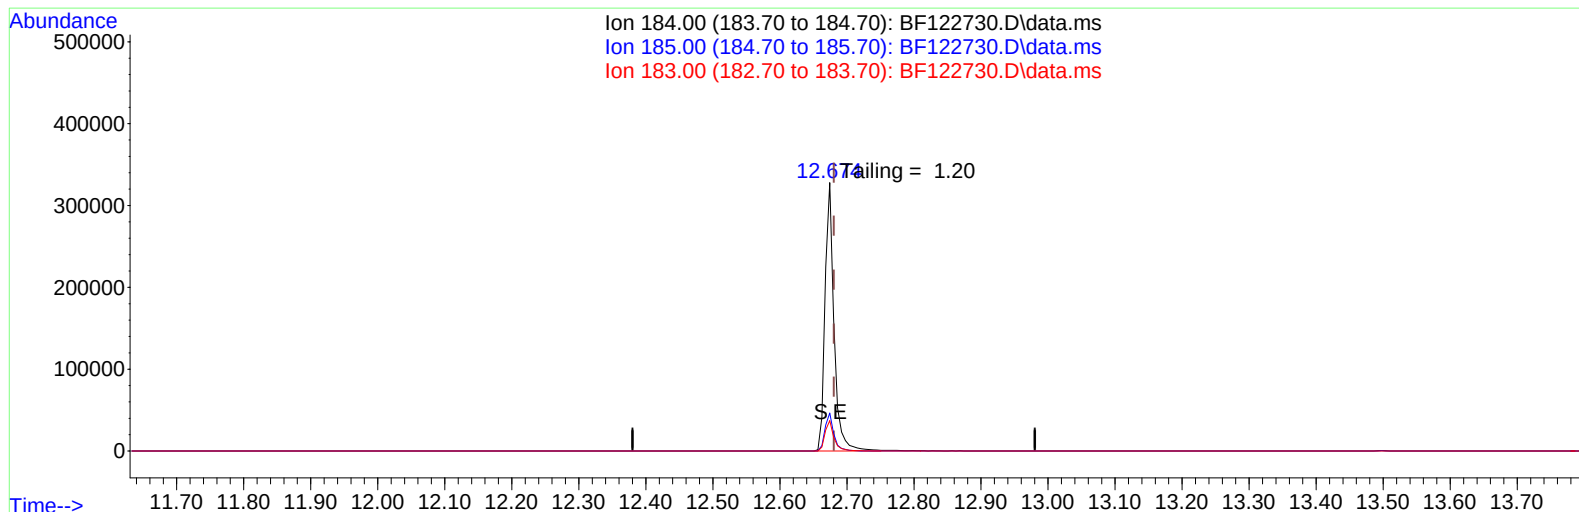

TIC: BF122730.D\data.ms

(77) Benzidine

12.674min (-0.006) 0.00 ng

response 309730

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.23
183.00	12.10	11.35
0.00	0.00	0.00