

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121520\
 Data File : BF122718.D
 Acq On : 15 Dec 2020 16:23
 Operator : JU/CG
 Sample : PB133592BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB133592BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF122718.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.451	566	572	575	rBV	4551376	5108160	61.89%	11.202%
2	6.457	736	743	746	rBV	4102447	5233661	63.41%	11.477%
3	6.816	800	804	808	rBV	1510442	1206169	14.61%	2.645%
4	7.381	894	900	903	rBV	2946704	3650726	44.23%	8.006%
5	8.098	1017	1022	1026	rBV	1622459	1681099	20.37%	3.686%
6	9.181	1199	1206	1209	rBV	5825448	7024848	85.11%	15.405%
7	9.857	1315	1321	1324	rBV	2190702	2146625	26.01%	4.707%
8	10.651	1449	1456	1459	rBV	4137804	4933313	59.77%	10.818%
9	11.339	1567	1573	1577	rBV	2510923	2306668	27.95%	5.058%
10	12.939	1837	1845	1848	rBV	6413322	8253847	100.00%	18.100%
11	13.980	2018	2022	2026	rBV	2381974	2164270	26.22%	4.746%
12	15.439	2264	2270	2280	rVB	1413670	1892437	22.93%	4.150%




Sum of corrected areas: 45601823

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121520\
Data File : BF122718.D
Acq On : 15 Dec 2020 16:23
Operator : JU/CG
Sample : PB133592BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB133592BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

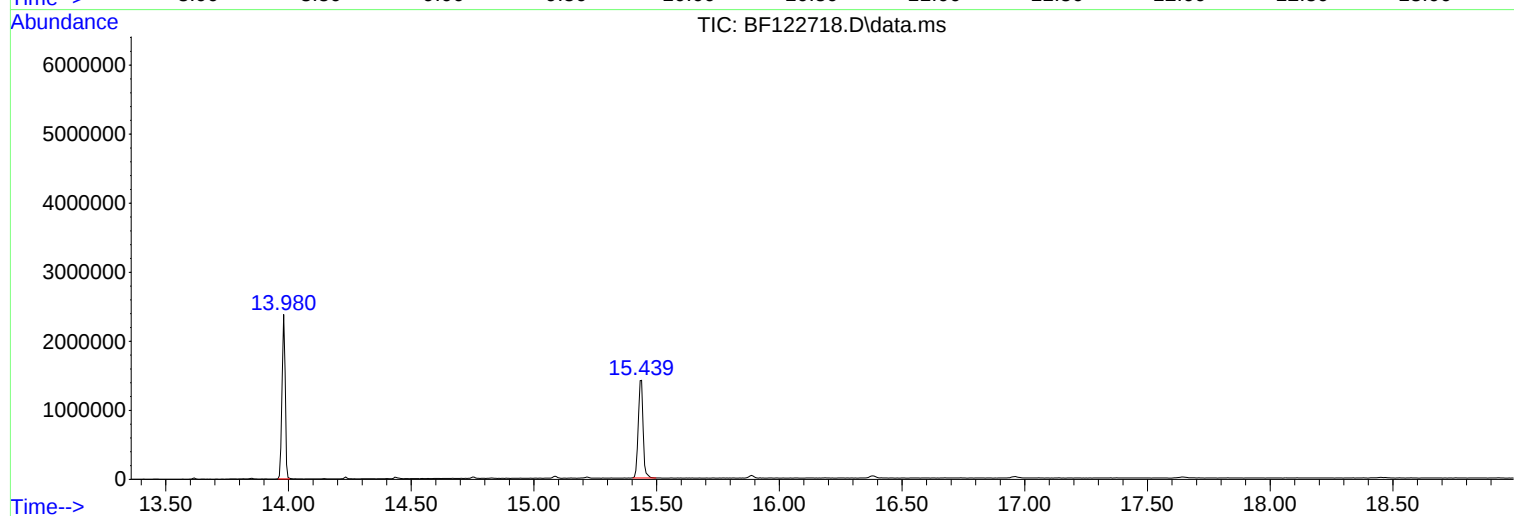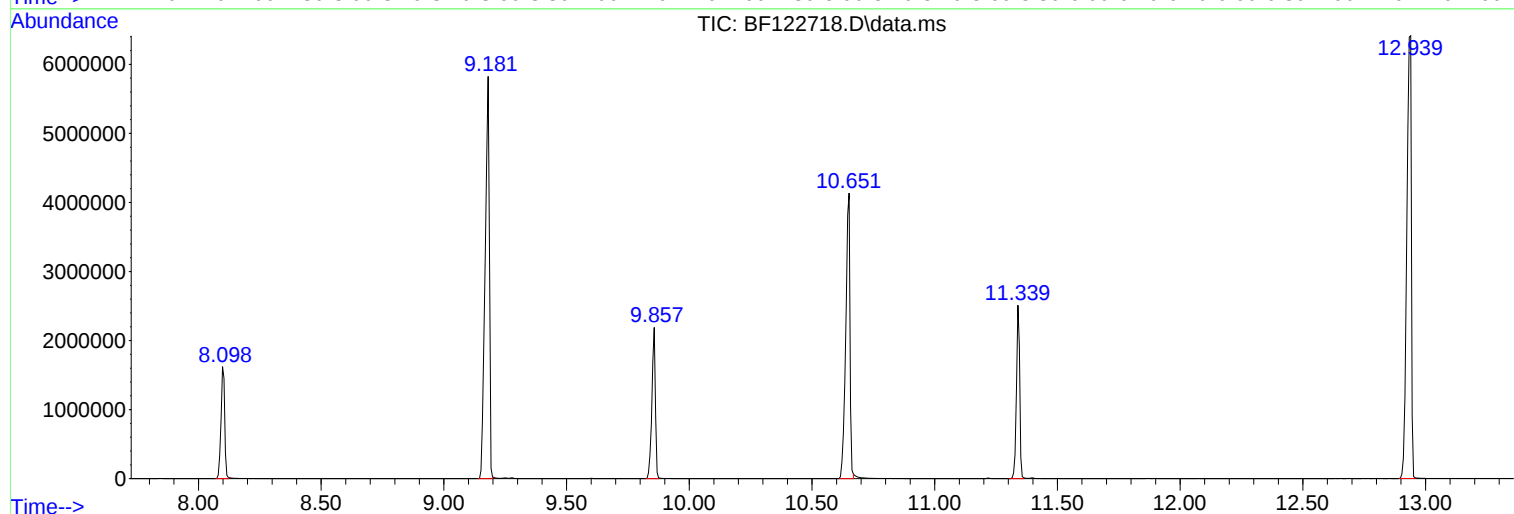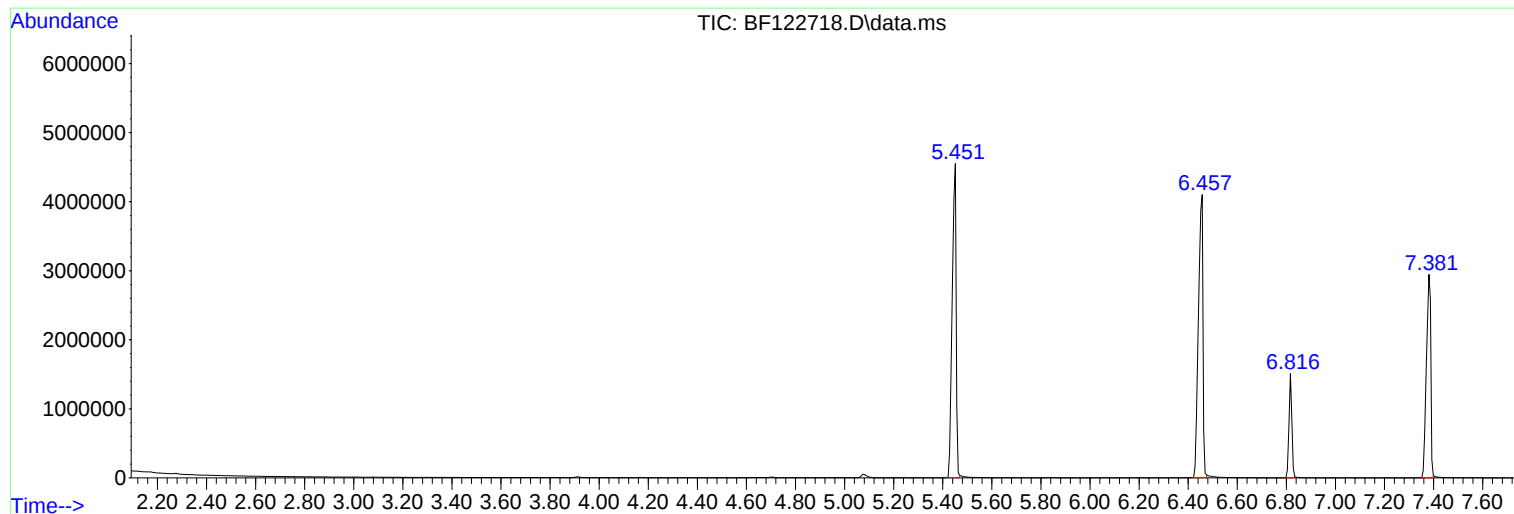

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121520\
Data File : BF122718.D
Acq On : 15 Dec 2020 16:23
Operator : JU/CG
Sample : PB133592BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB133592BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121520\
Data File : BF122718.D
Acq On : 15 Dec 2020 16:23
Operator : JU/CG
Sample : PB133592BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB133592BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------