


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121520\
 Data File : BF122716.D
 Acq On : 15 Dec 2020 11:40
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 15 18:14:23 2020

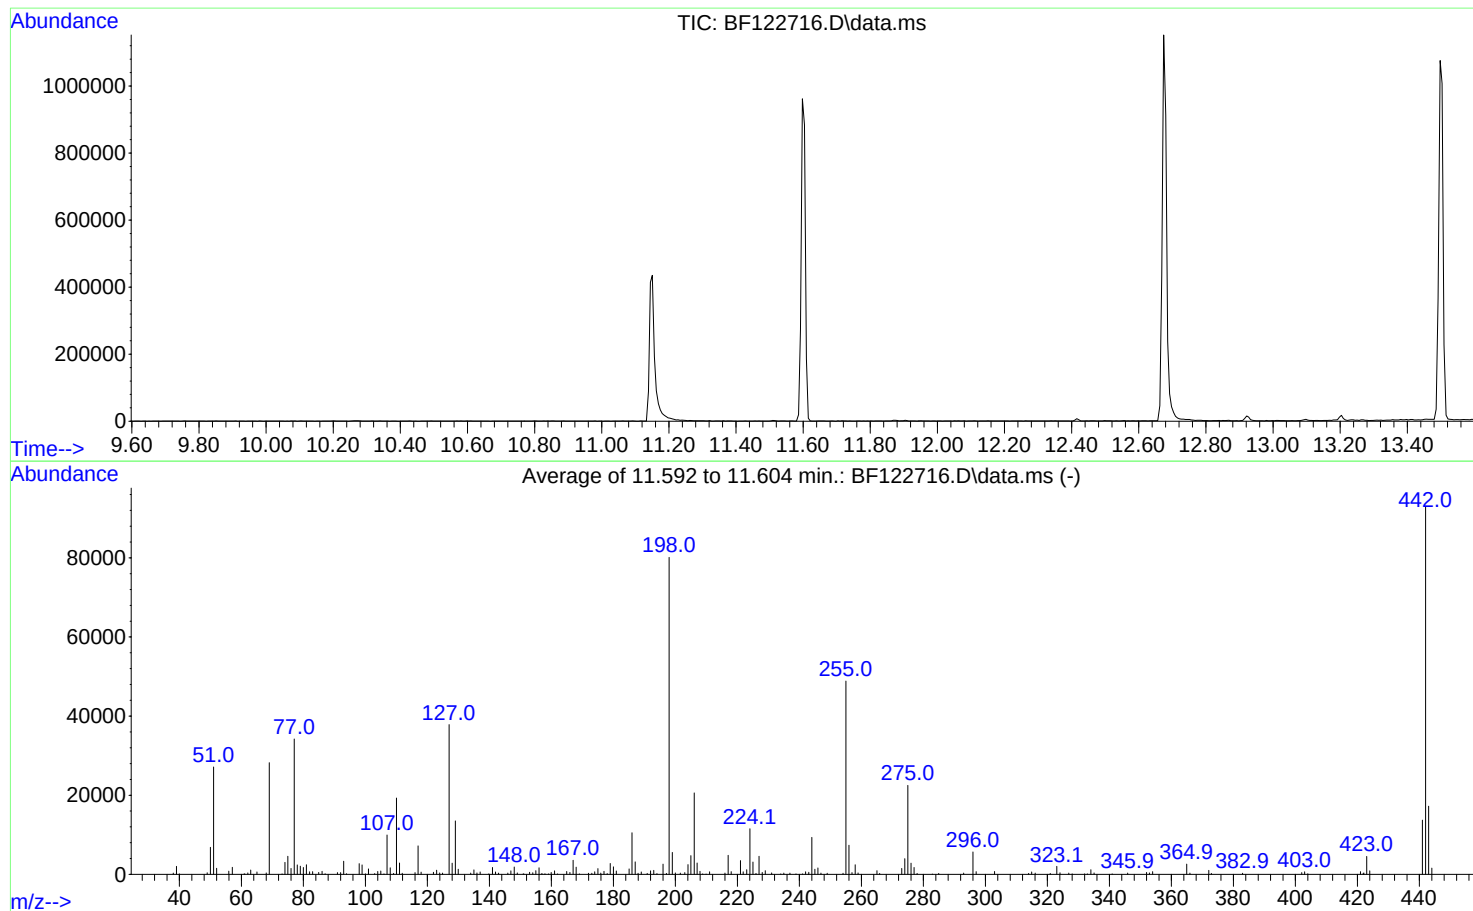

AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1612

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.9	27136	PASS
68	69	0.00	2	1.3	358	PASS
69	198	0.00	100	35.2	28240	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.2	37851	PASS
197	198	0.00	2	0.3	266	PASS
198	198	100	100	100.0	80139	PASS
199	198	5	9	6.9	5544	PASS
275	198	10	60	28.1	22490	PASS
365	198	1	100	3.2	2604	PASS
441	198	0.01	100	17.1	13709	PASS
442	442	100	100	100.0	92980	PASS
443	442	15	24	18.5	17245	PASS