
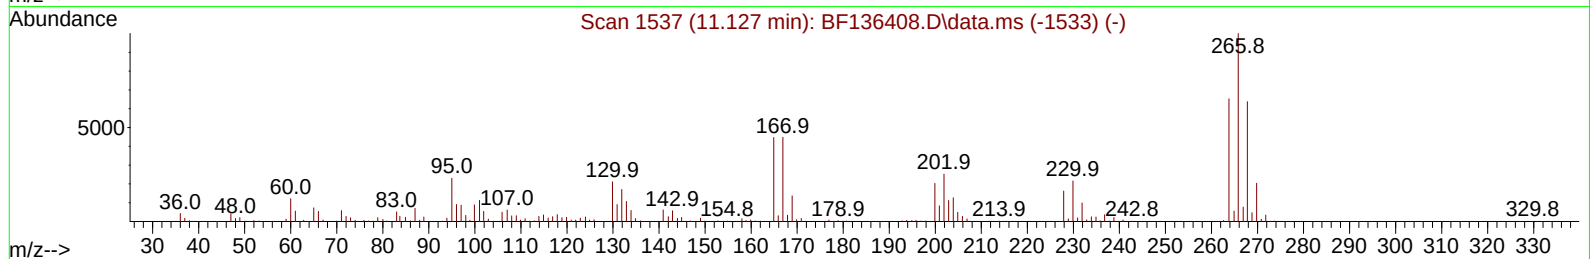
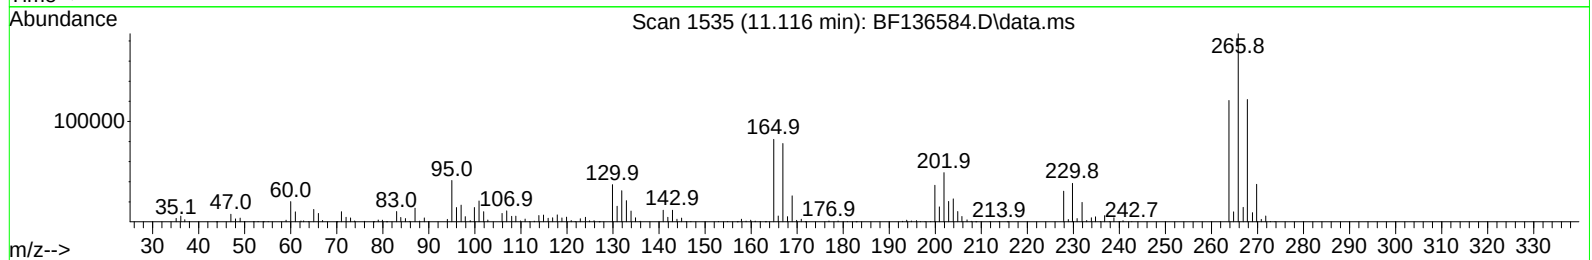


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121523\
Data File : BF136584.D
Acq On : 15 Dec 2023 09:49
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 15 11:34:41 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 15 00:33:23 2023
Response via : Initial Calibration

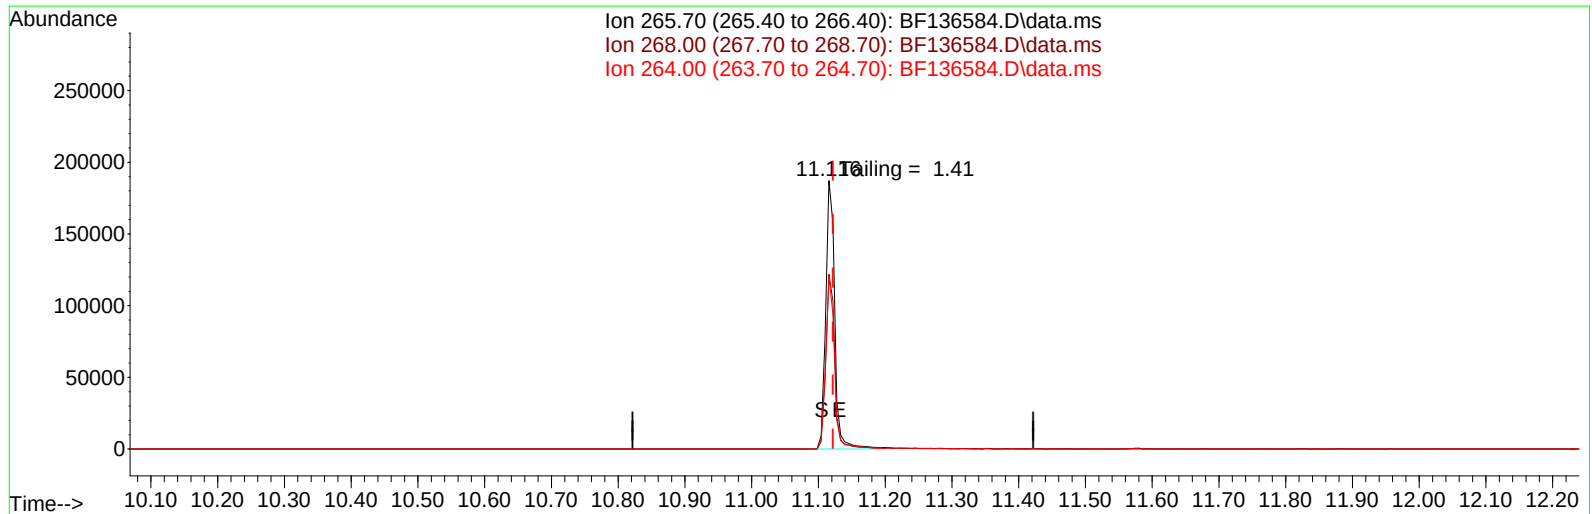

TIC: BF136584.D\data.ms

(70) Pentachlorophenol (C)




11.116min (-0.006) 128028.17 ng

response 176716

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	65.06
264.00	65.30	64.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121523\
Data File : BF136584.D
Acq On : 15 Dec 2023 09:49
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 15 11:34:41 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 15 00:33:23 2023
Response via : Initial Calibration

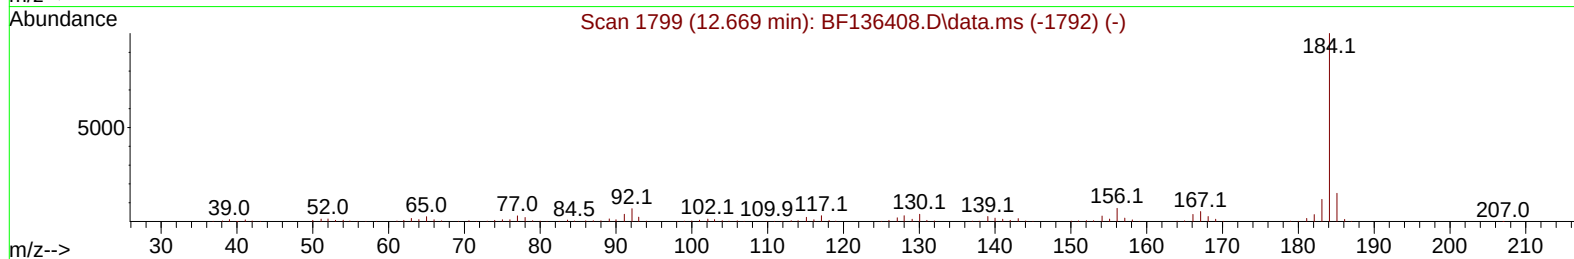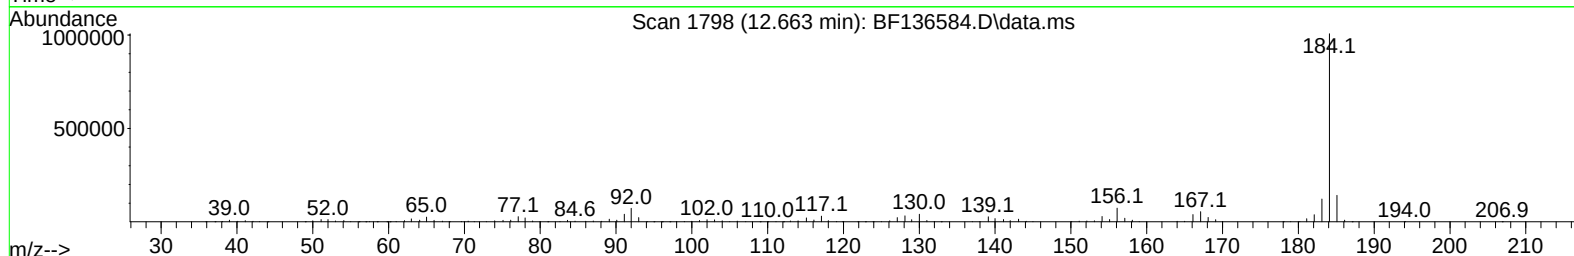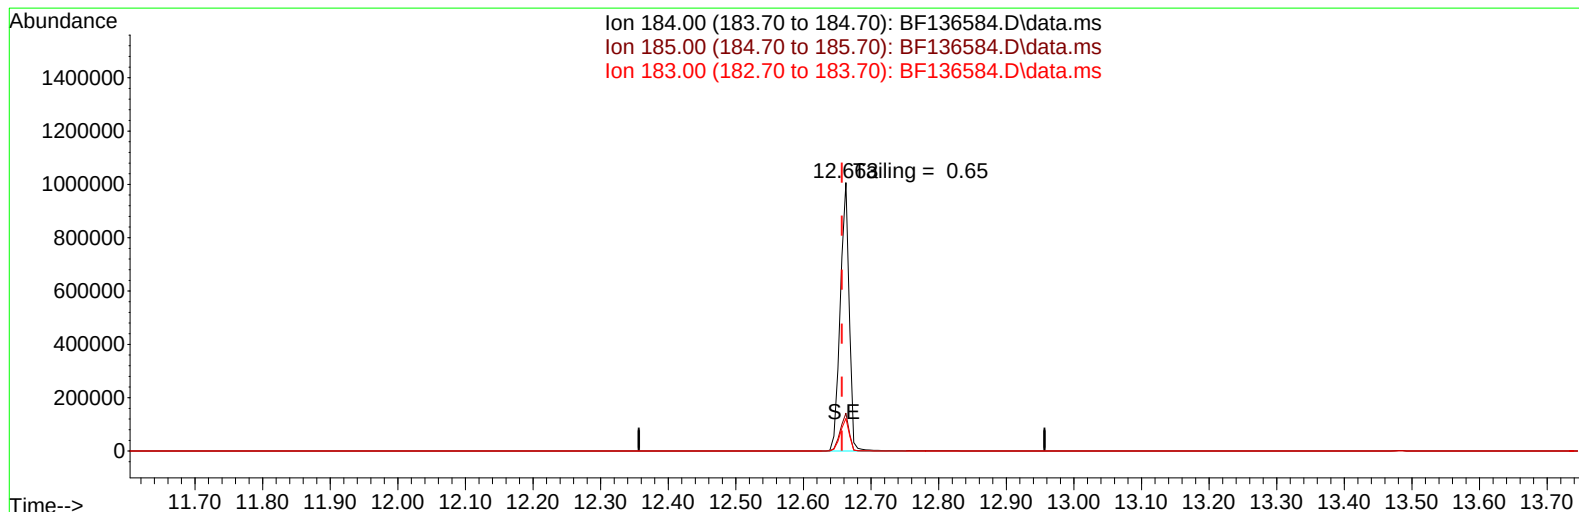

TIC: BF136584.D\data.ms

(77) Benzidine

12.663min (+ 0.006) 0.00 ng m

response 925421

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.10
183.00	11.70	12.09
0.00	0.00	0.00