

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121523\
 Data File : BF136586.D
 Acq On : 15 Dec 2023 11:23
 Operator : CG\JU
 Sample : PB157778BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB157778BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF136586.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.045	499	503	509	rVB	43821	55867	1.27%	0.244%
2	5.434	565	569	572	rBV	2646994	2725129	61.87%	11.883%
3	6.434	733	739	742	rBV	2545142	2702408	61.36%	11.784%
4	6.787	795	799	802	rBV	673930	600843	13.64%	2.620%
5	7.345	888	894	897	rBV	1668559	1818463	41.29%	7.929%
6	8.063	1011	1016	1019	rBV	920422	830059	18.85%	3.619%
7	9.145	1193	1200	1203	rBV	4134125	3873180	87.94%	16.889%
8	9.816	1309	1314	1318	rBV	1102368	1026645	23.31%	4.477%
9	10.616	1445	1450	1453	rBV	2582036	2333908	52.99%	10.177%
10	11.310	1564	1568	1571	rBV	1467210	1122571	25.49%	4.895%
11	12.910	1835	1840	1843	rBV	4566048	4404327	100.00%	19.205%
12	13.963	2014	2019	2022	rBV	818061	800388	18.17%	3.490%
13	15.433	2264	2269	2276	rBV	493720	640025	14.53%	2.791%




Sum of corrected areas: 22933813

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121523\
Data File : BF136586.D
Acq On : 15 Dec 2023 11:23
Operator : CG\JU
Sample : PB157778BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157778BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

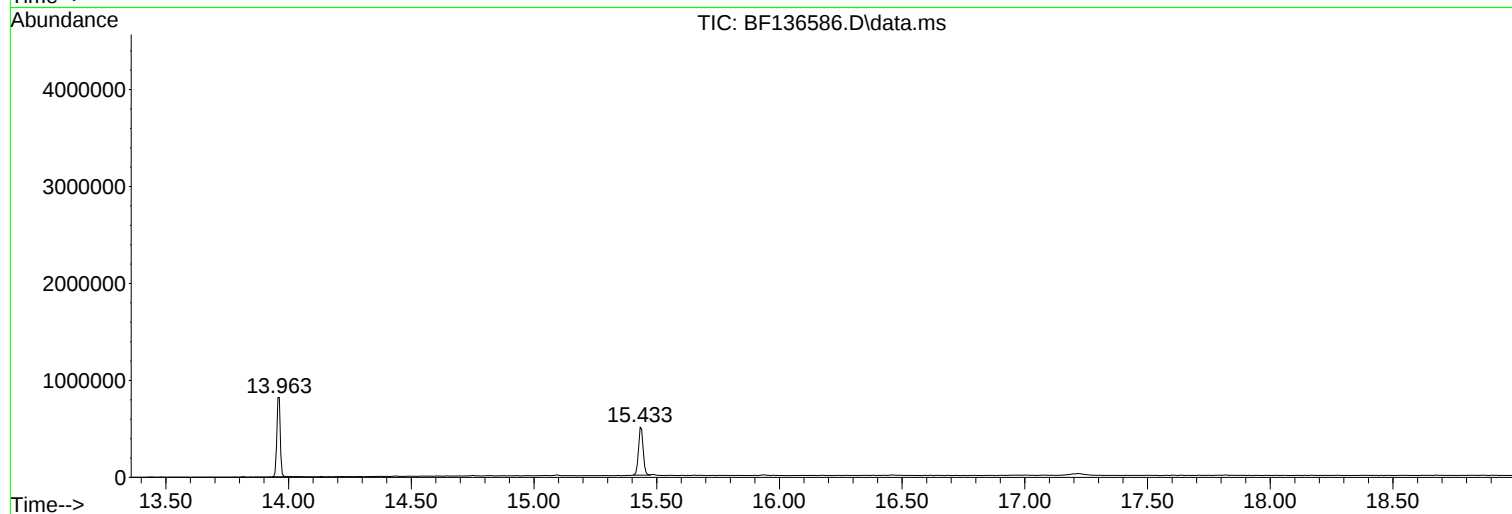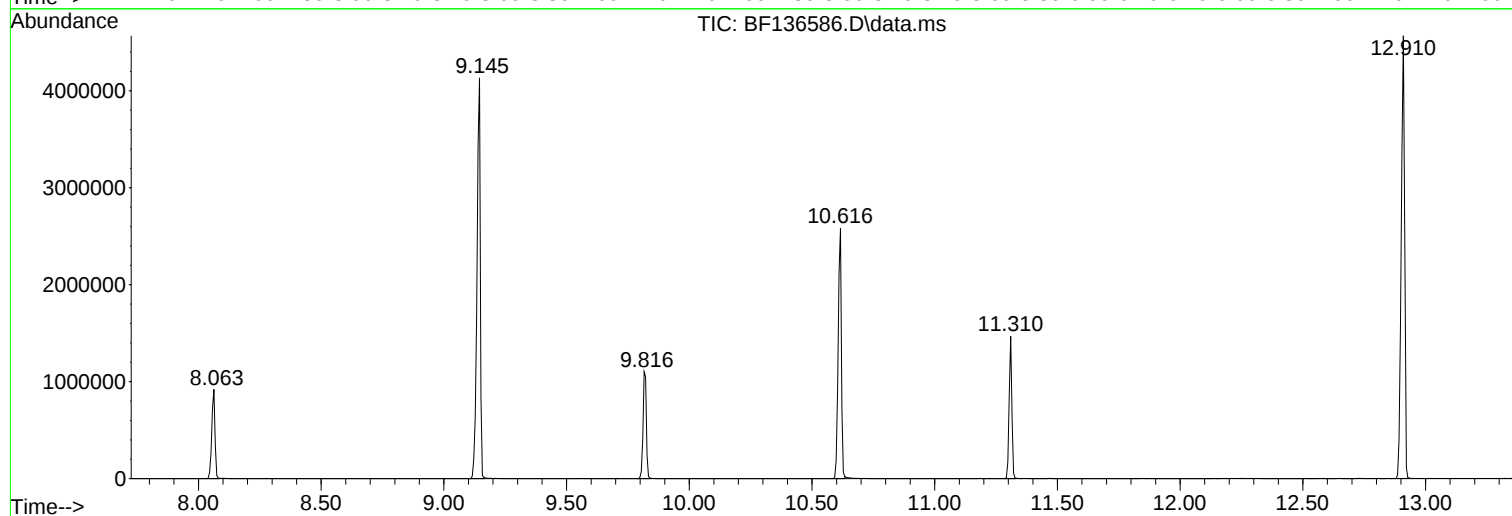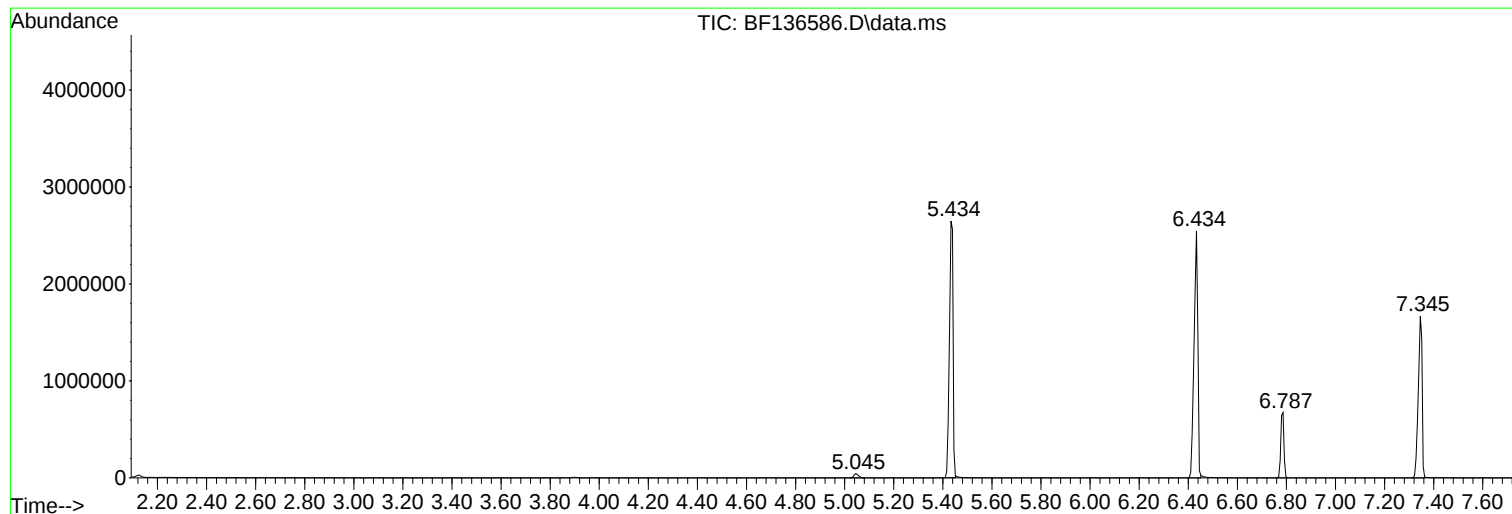

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121523\
Data File : BF136586.D
Acq On : 15 Dec 2023 11:23
Operator : CG\JU
Sample : PB157778BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157778BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121523\
Data File : BF136586.D
Acq On : 15 Dec 2023 11:23
Operator : CG\JU
Sample : PB157778BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157778BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------