


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF121523\  
Data File : BF136584.D  
Acq On : 15 Dec 2023 09:49  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF120523.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Tue Dec 19 00:56:37 2023

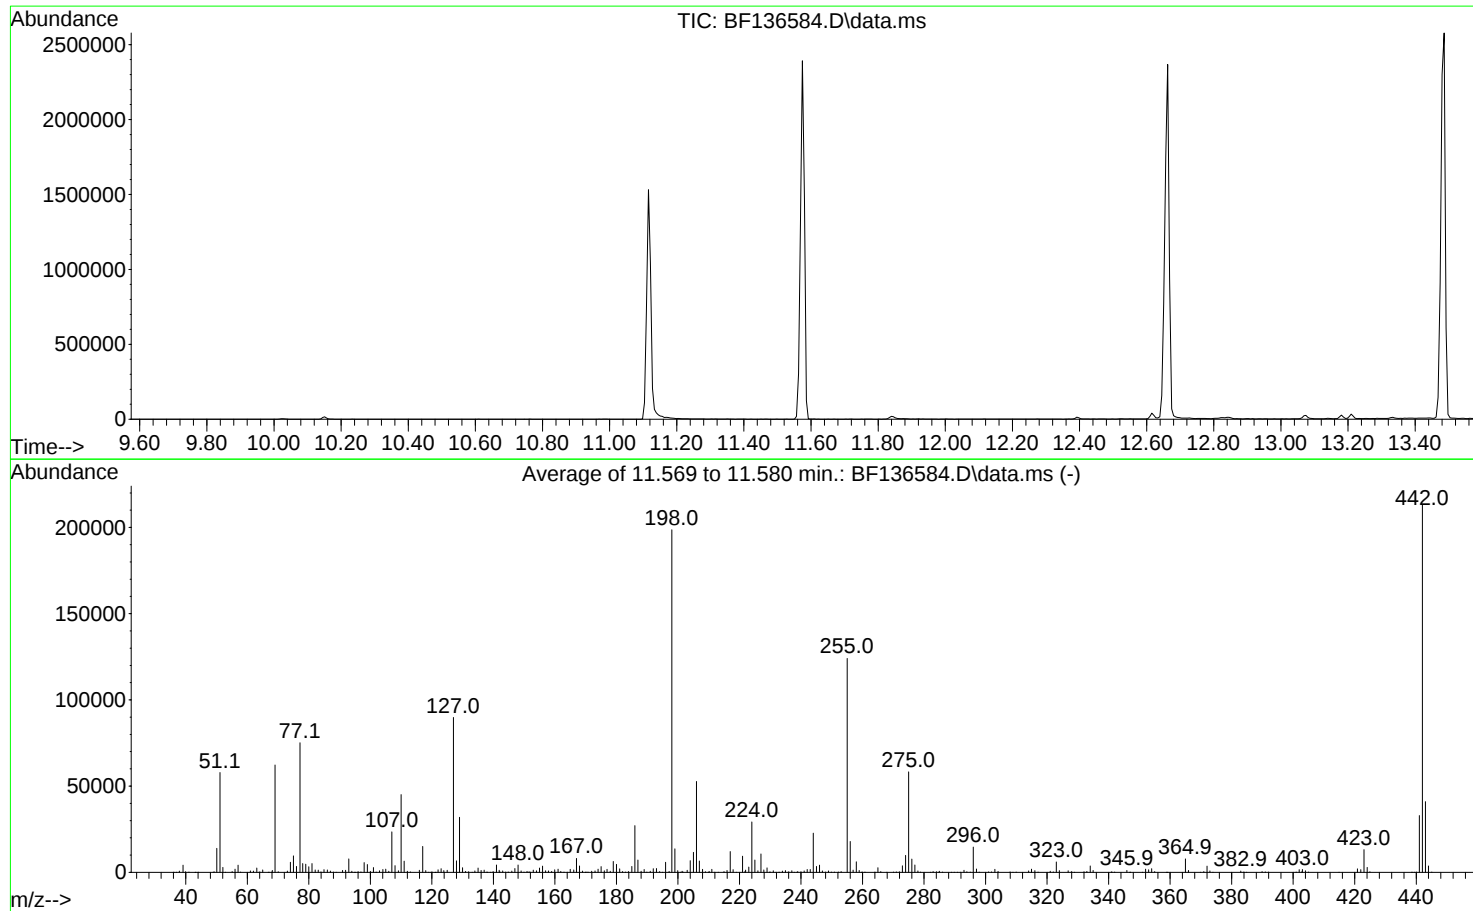




AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1607

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 29.1         | 57883      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.7          | 1073       | PASS                |
| 69             | 198             | 0.00            | 100             | 31.3         | 62227      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.6          | 348        | PASS                |
| 127            | 198             | 10              | 80              | 45.2         | 89805      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.3          | 560        | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 198592     | PASS                |
| 199            | 198             | 5               | 9               | 6.9          | 13610      | PASS                |
| 275            | 198             | 10              | 60              | 29.3         | 58267      | PASS                |
| 365            | 198             | 1               | 100             | 3.9          | 7811       | PASS                |
| 441            | 198             | 0.01            | 100             | 16.6         | 32935      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 213291     | PASS                |
| 443            | 442             | 15              | 24              | 19.2         | 41035      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF121523\  
Data File : BF136584.D  
Acq On : 15 Dec 2023 09:49  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Dec 15 11:34:41 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF120523.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Dec 15 00:33:23 2023  
Response via : Initial Calibration

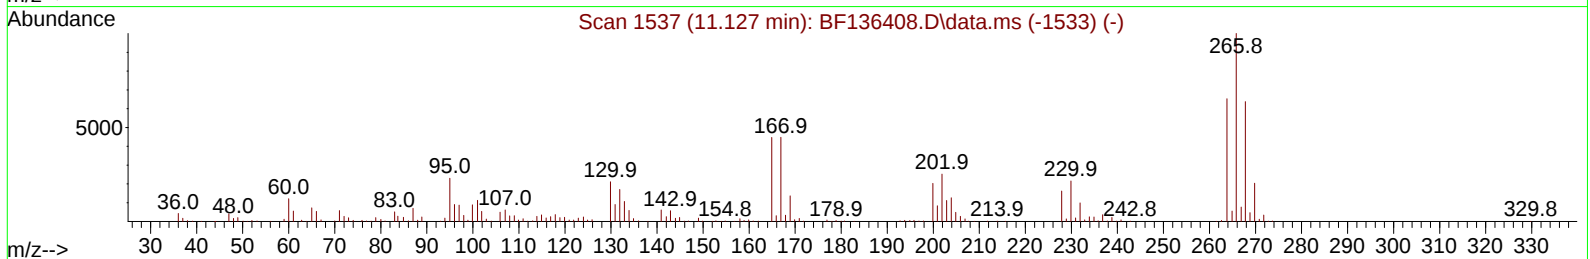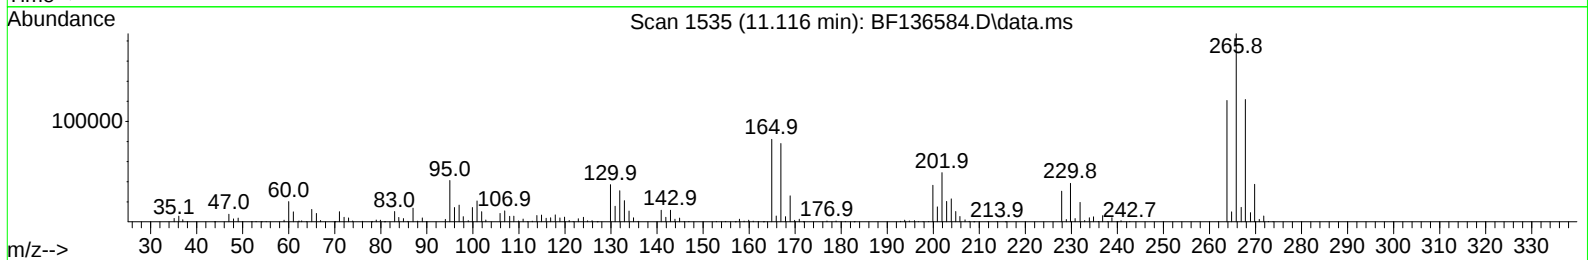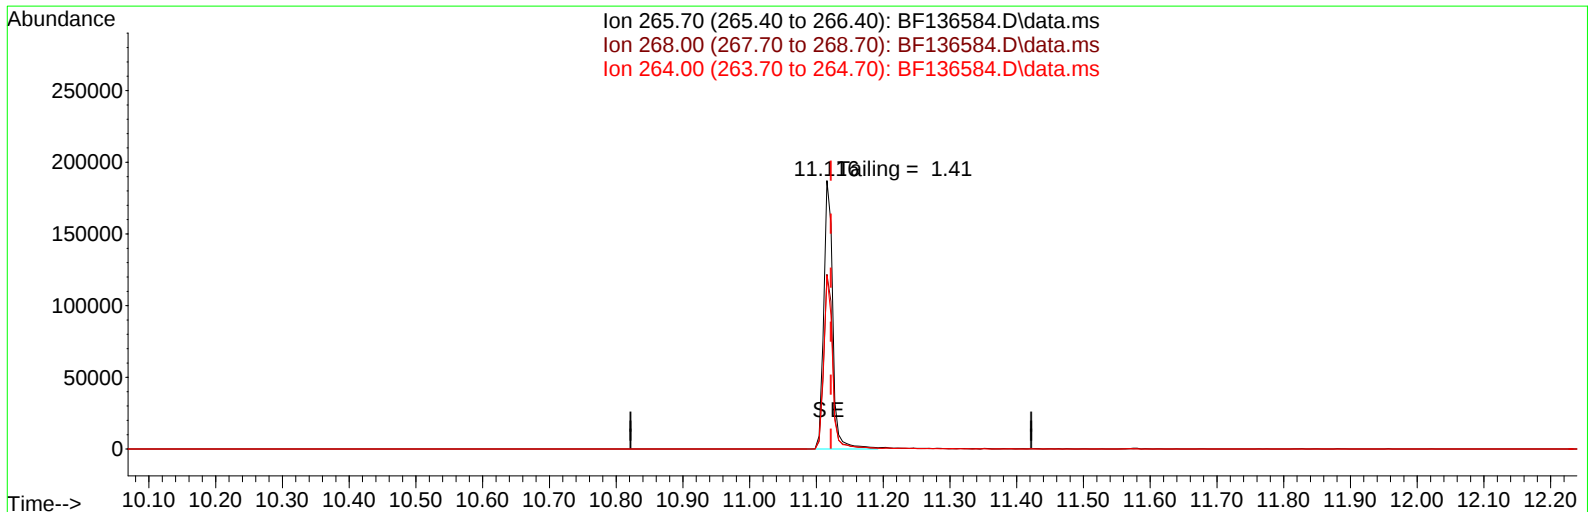

TIC: BF136584.D\data.ms

**(70) Pentachlorophenol (C)**

**11.116min (-0.006) 128028.17 ng**




**response 176716**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.80  | 65.06  |
| 264.00 | 65.30  | 64.57  |
| 0.00   | 0.00   | 0.00   |

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121523\  
Data File : BF136584.D  
Acq On    : 15 Dec 2023  09:49  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

**Instrument :**  
BNA\_F  
**ClientSampleId :**  
DFTPP

Quant Time: Dec 15 11:34:41 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF120523.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Dec 15 00:33:23 2023  
Response via : Initial Calibration

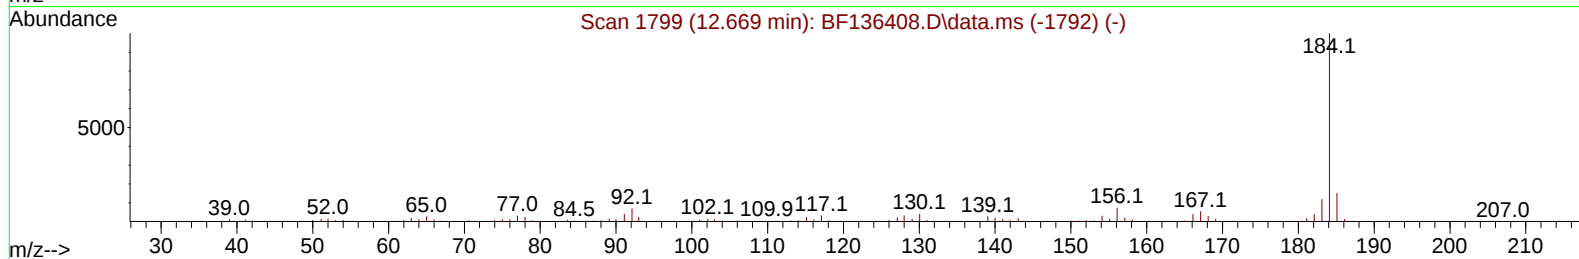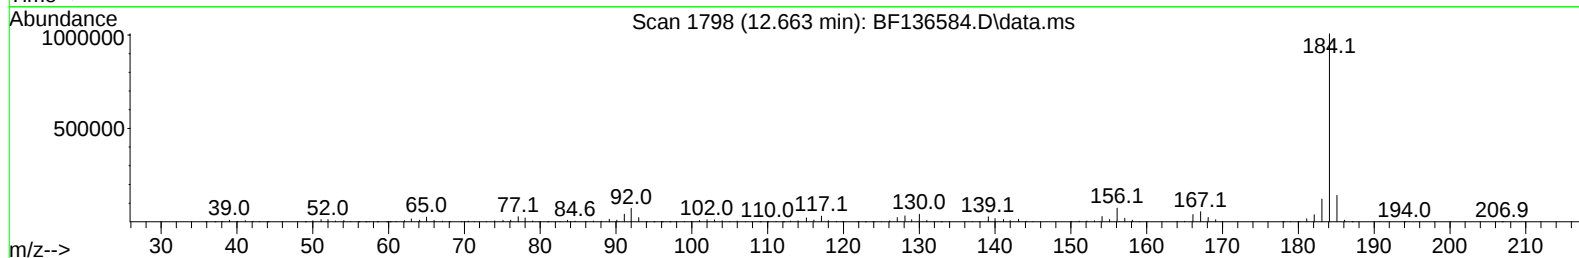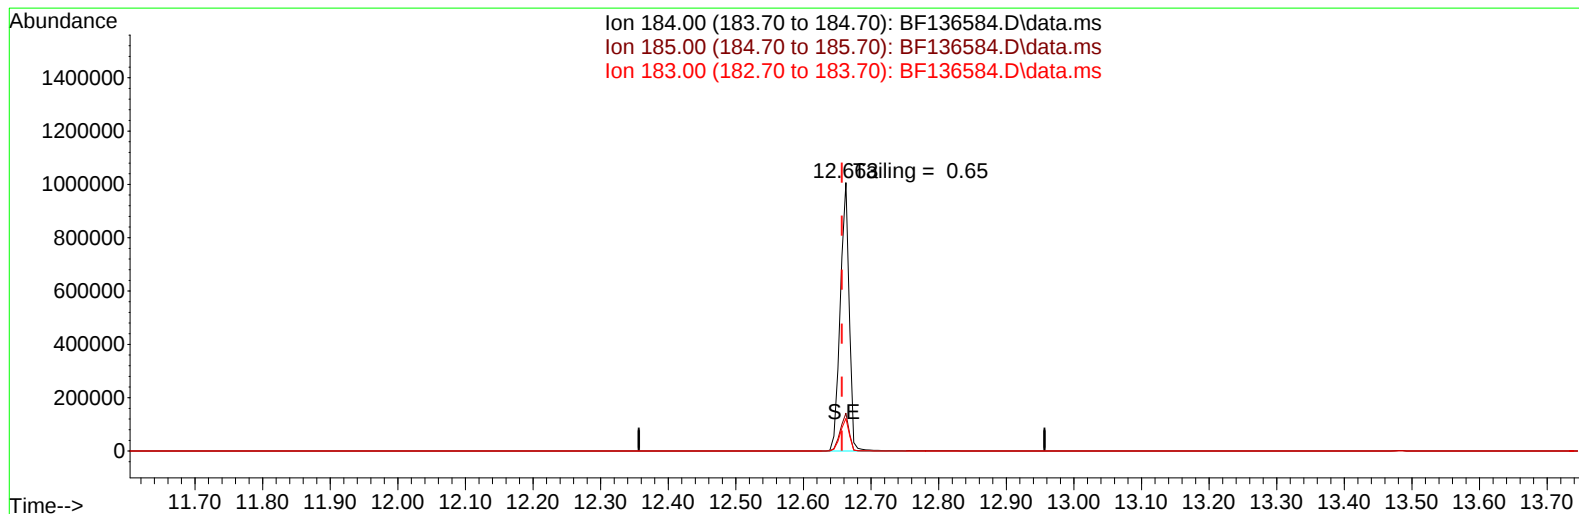

TIC: BF136584.D\data.ms

(77) Benzidine

12.663min (+ 0.006) 0.00 ng m

**response**      **925421**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.00  | 14.10  |
| 183.00 | 11.70  | 12.09  |
| 0.00   | 0.00   | 0.00   |

### DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 12/15/2023    | BNA_F            | <u>BF136584.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 492162           | 13.486             |
| DDD           | 9558             | 13.21              |
| DDE           | 1771             | 12.845             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 11329         | 503491           | 2.25               |
|               |                  |                    |

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP