
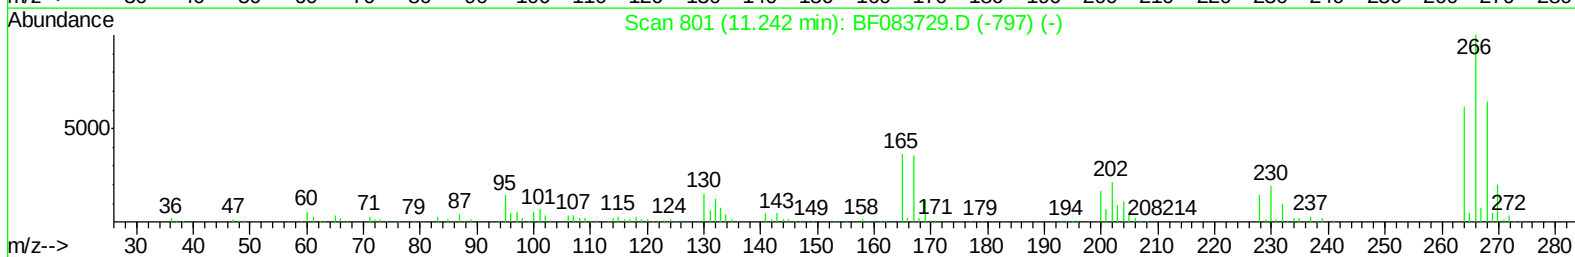
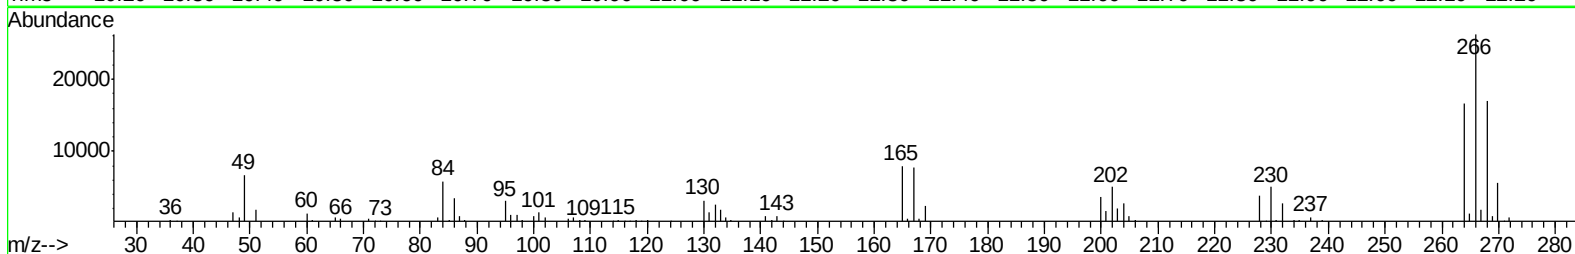


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF121615\
Data File : BF083842.D
Acq On : 16 Dec 2015 11:18
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 17 04:52:53 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 14 01:30:12 2015
Response via : Initial Calibration

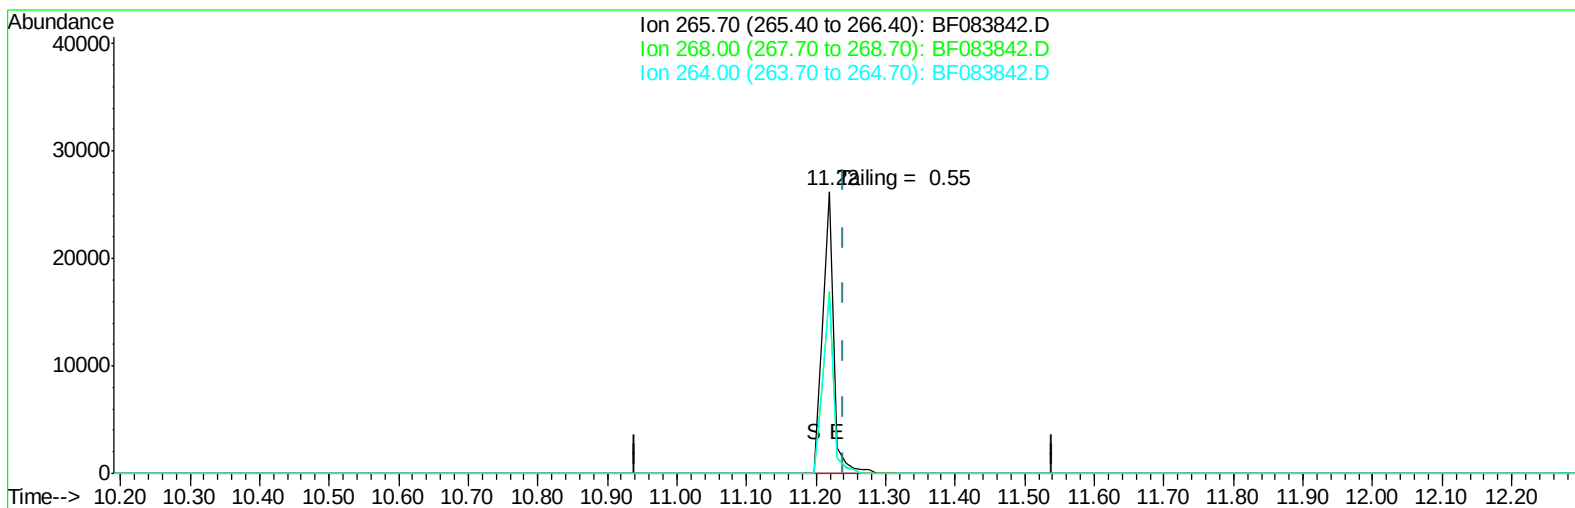

TIC: BF083842.D

(69) Pentachlorophenol (C)




11.219min (-0.022) 0.00ng

response 29598

Ion	Exp%	Act%
265.70	100	100
268.00	62.70	64.69
264.00	64.30	63.56
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF121615\
 Data File : BF083842.D
 Acq On : 16 Dec 2015 11:18
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 17 04:52:53 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121315.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 14 01:30:12 2015
 Response via : Initial Calibration

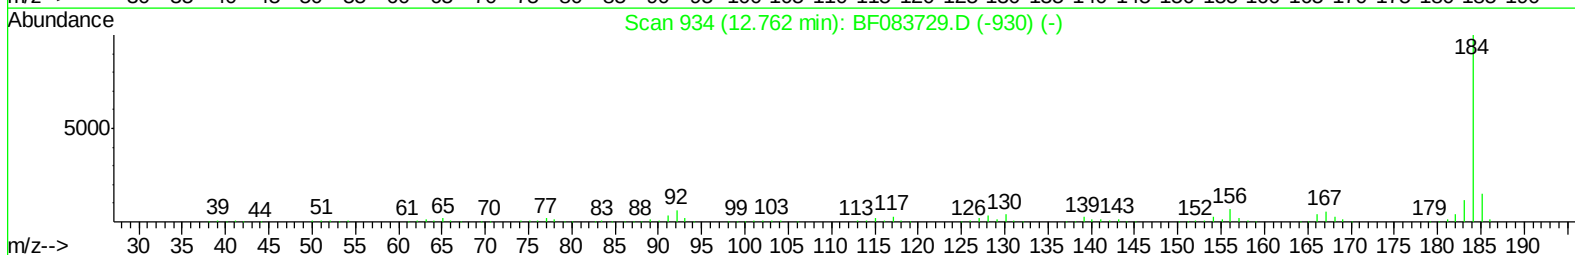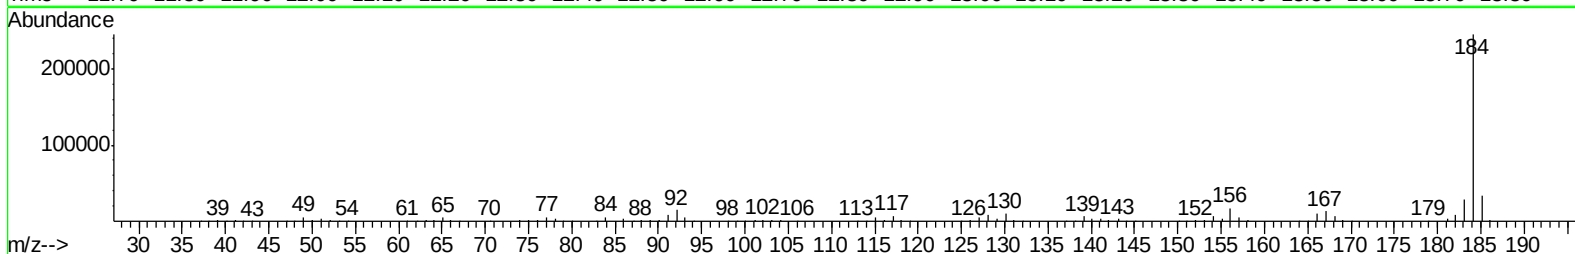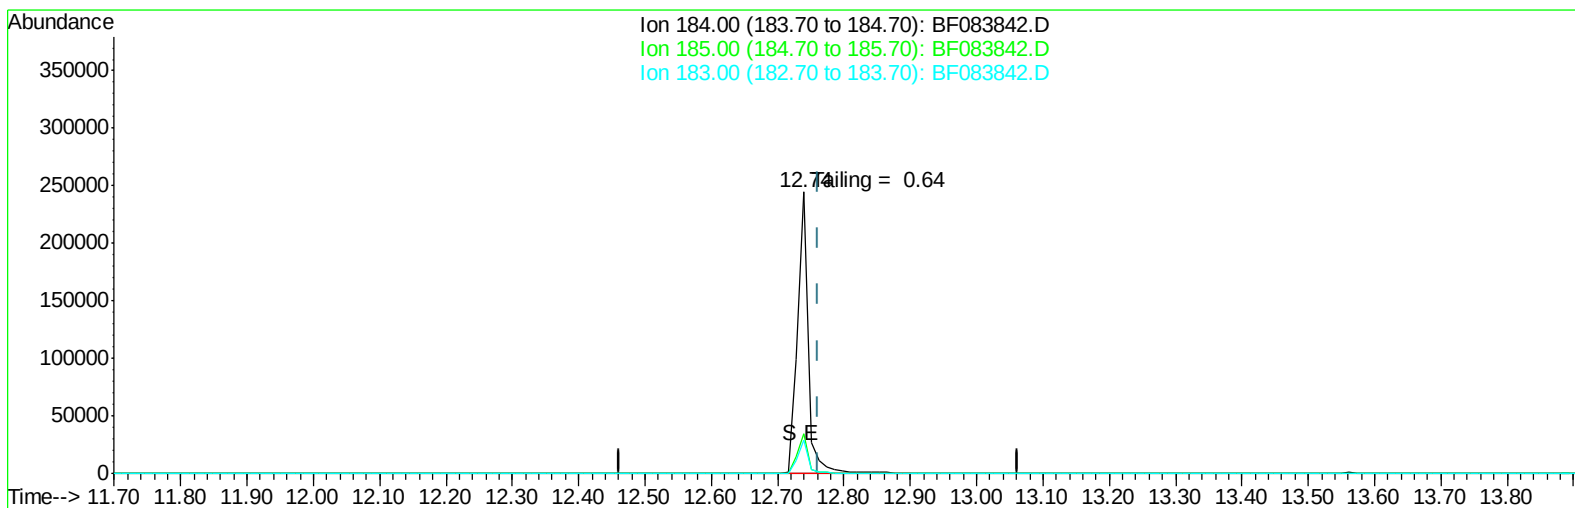

TIC: BF083842.D

(76) Benzidine

12.739min (-0.023) 0.00ng

response 273113

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	13.92
183.00	11.20	11.64
0.00	0.00	0.00