

Data Path : Z:\HPCHEM1\BNA F\DATA\BF121615\
 Data File : BF083859.D
 Acq On : 16 Dec 2015 20:21
 Operator : UM/SJ
 Sample : G4775-13
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 COMPOSITE-B-20150873

Quant Time: Dec 17 04:32:41 2015
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121315.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 14 01:30:12 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.89	152	86080	20.00	ng	-0.03
21) Naphthalene-d8	8.18	136	358450	20.00	ng	-0.03
38) Acenaphthene-d10	9.93	164	181554	20.00	ng	-0.03
63) Phenanthrene-d10	11.41	188	310383	20.00	ng	-0.03
75) Chrysene-d12	14.04	240	214041	20.00	ng	-0.03
86) Perylene-d12	15.47	264	173823	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.50	112	756933	141.86	ng	-0.02
7) Phenol-d6	6.53	99	987292	146.11	ng	-0.01
23) Nitrobenzene-d5	7.46	82	649959	101.45	ng	-0.02
41) 2,4,6-Tribromophenol	10.72	330	246533	133.26	ng	-0.03
44) 2-Fluorobiphenyl	9.25	172	1089410	89.31	ng	-0.03
78) Terphenyl-d14	12.99	244	897548	90.20	ng	-0.03
Target Compounds						
49) Dimethylphthalate	9.64	163	299982	21.19	ng	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF121615\
Data File : BF083859.D
Acq On : 16 Dec 2015 20:21
Operator : UM/SJ
Sample : G4775-13
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
COMPOSITE-B-20150873

Quant Time: Dec 17 04:32:41 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 14 01:30:12 2015
Response via : Initial Calibration

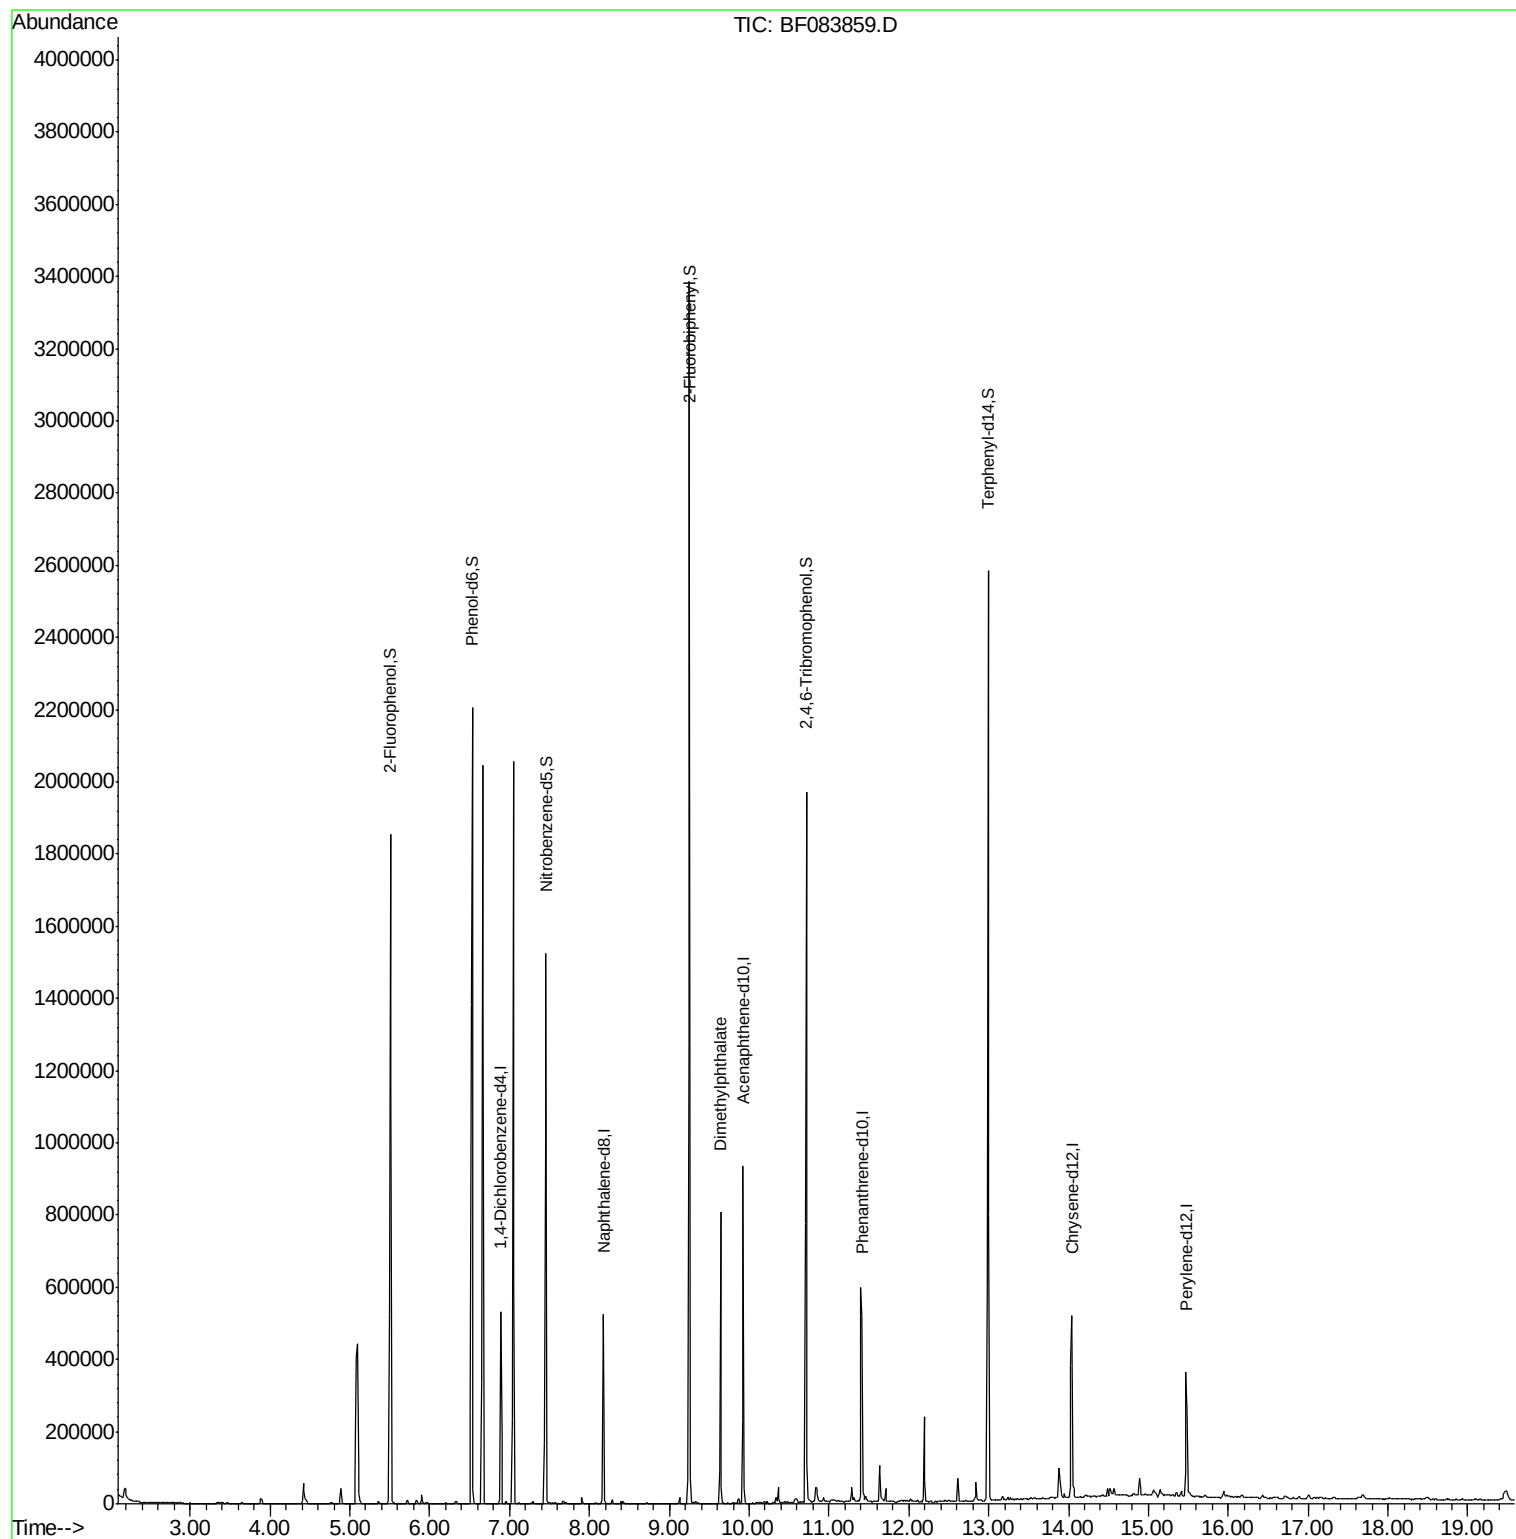

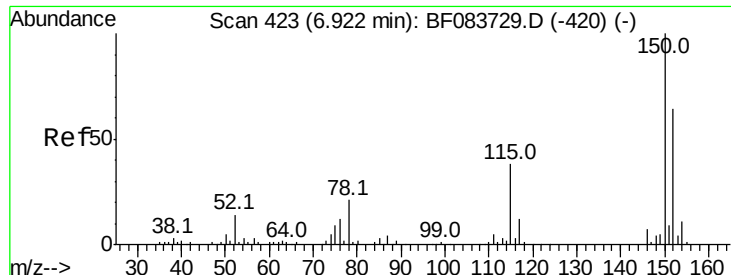

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.89 min Scan# 420

Delta R.T. -0.03 min

Lab File: BF083859.D

Acq: 16 Dec 2015 20:21

Instrument :

BNA_F

ClientSampleId :

COMPOSITE-B-20150873


Tot Ion:152 Resp: 86080

Ion Ratio Lower Upper

152 100

150 159.9 126.5 189.7




115 71.0 52.3 78.5

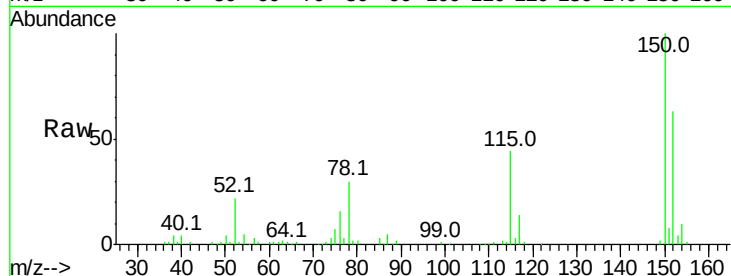

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

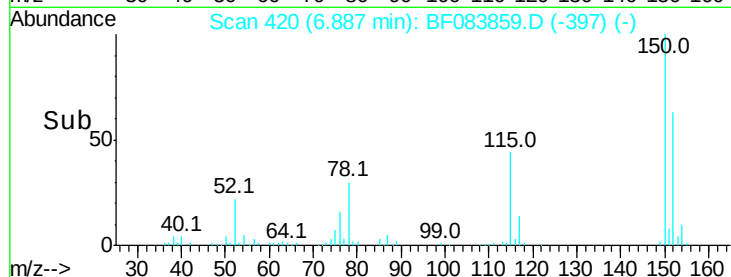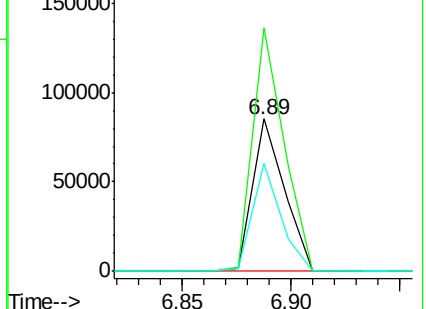

#5

2-Fluorophenol

Concen: 141.86 ng

RT: 5.50 min Scan# 299

Delta R.T. -0.02 min

Lab File: BF083859.D

Acq: 16 Dec 2015 20:21


Tgt Ion:112 Resp: 756933

Ion Ratio Lower Upper

112 100

64 58.5 50.5 75.7



63 31.0 25.8 38.6




Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

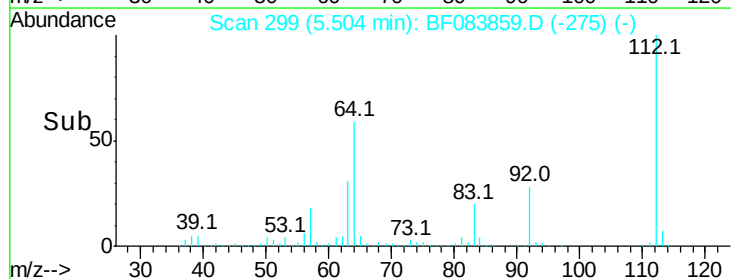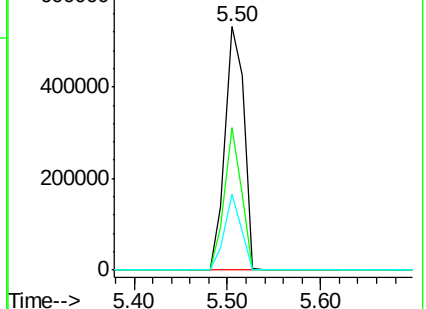

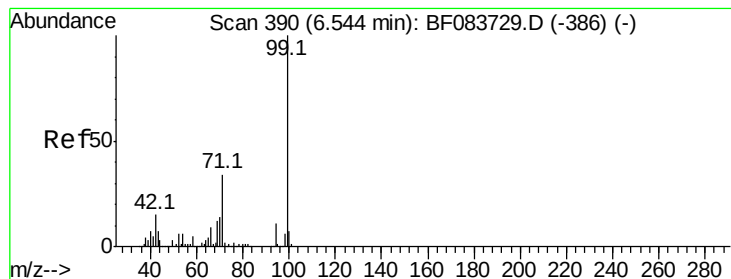

#7

Phenol-d6

Concen: 146.11 ng

RT: 6.53 min Scan# 389

Delta R.T. -0.01 min

Lab File: BF083859.D

Acq: 16 Dec 2015 20:21

Instrument :

BNA_F

ClientSampleId :

COMPOSITE-B-20150873


Tot Ion: 99 Resp: 987292

Ion Ratio Lower Upper

99 100

42 15.4 17.3 25.9#




71 36.9 26.6 40.0

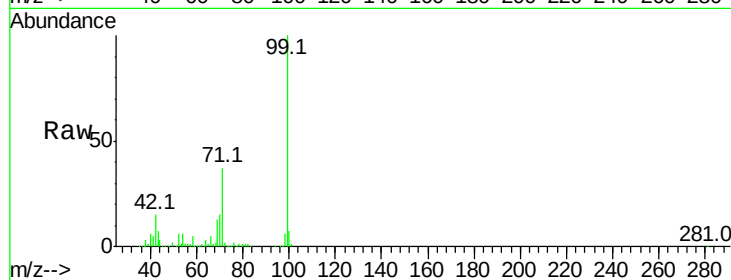

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

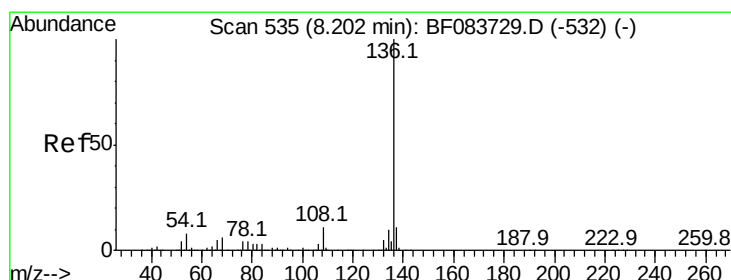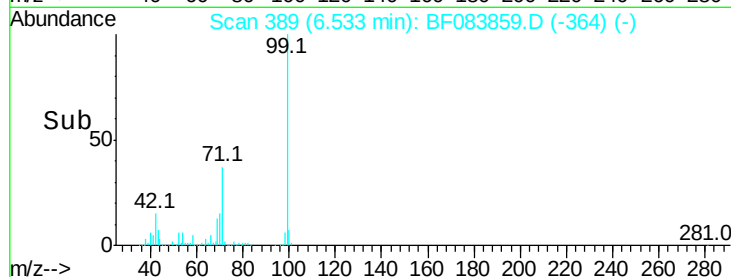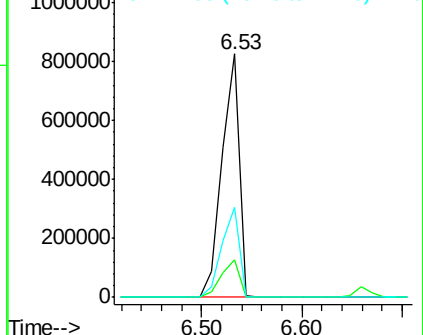

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.18 min Scan# 533

Delta R.T. -0.03 min

Lab File: BF083859.D

Acq: 16 Dec 2015 20:21

Tgt Ion: 136 Resp: 358450


Ion Ratio Lower Upper

136 100

137 10.7 8.7 13.1

54 4.3 7.8 11.6#

68 3.8 5.7 8.5#


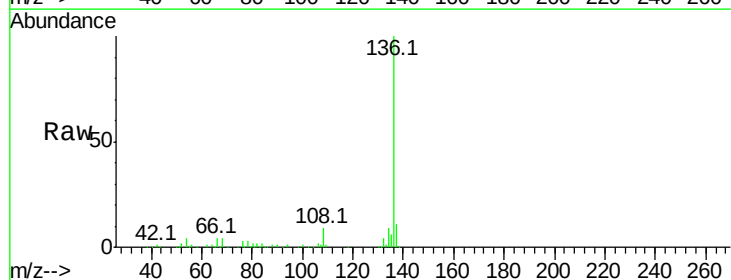



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0



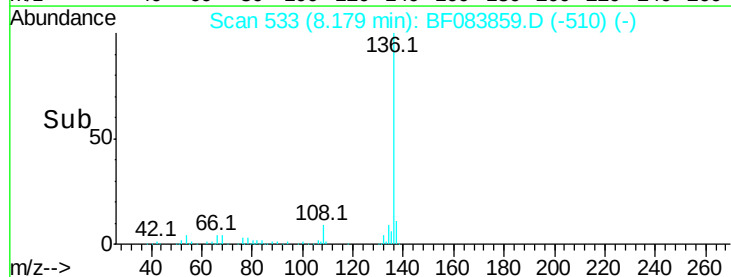
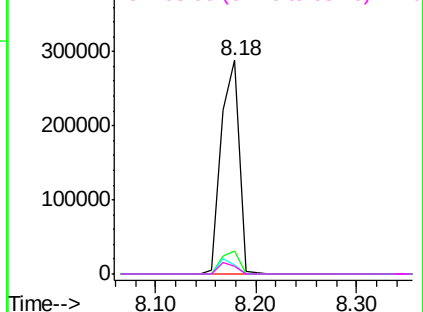


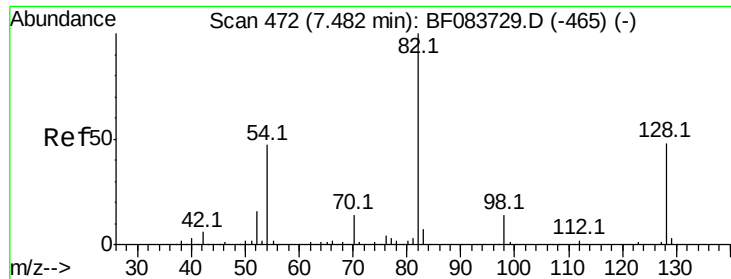

#23
Nitrobenzene-d5
Concen: 101.45 ng
RT: 7.46 min Scan# 470
Delta R.T. -0.02 min
Lab File: BF083859.D
Acq: 16 Dec 2015 20:21




Instrument :
BNA_F
ClientSampleId :
COMPOSITE-B-20150873


Tot Ion: 82 Resp: 649959
Ion Ratio Lower Upper
82 100
128 53.0 30.7 46.1#
54 42.7 42.5 63.7

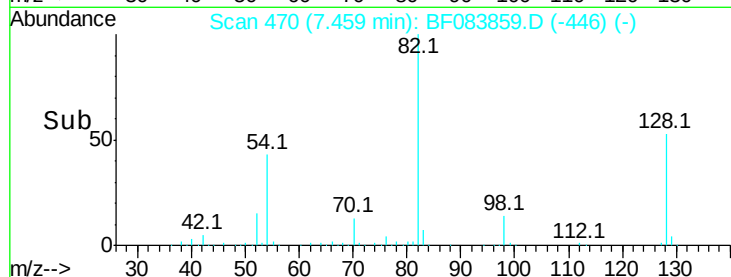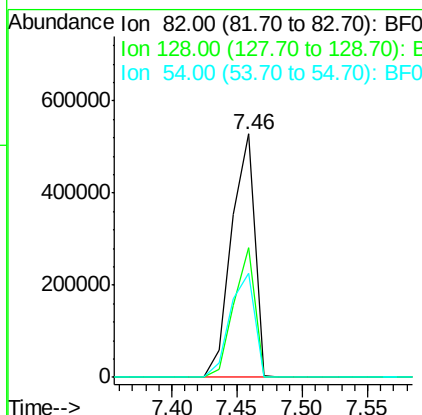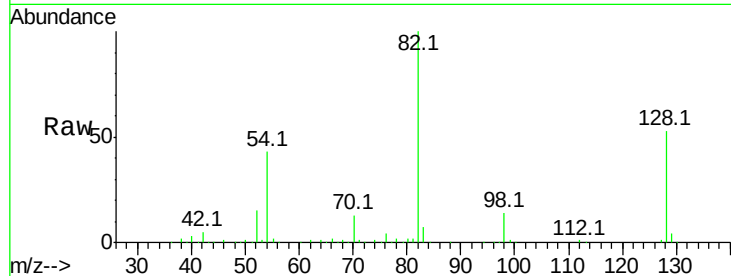

#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.93 min Scan# 686
Delta R.T. -0.03 min
Lab File: BF083859.D
Acq: 16 Dec 2015 20:21

Tgt Ion:164 Resp: 181554
Ion Ratio Lower Upper
164 100
162 103.6 78.8 118.2
160 46.3 33.4 50.2

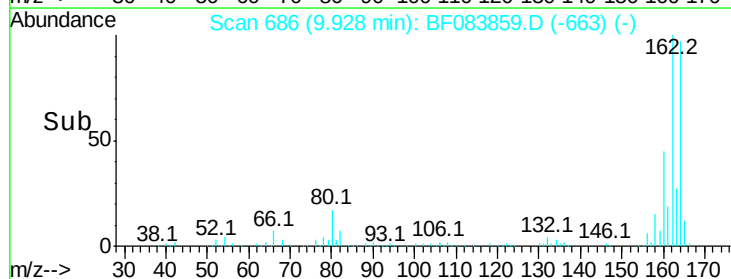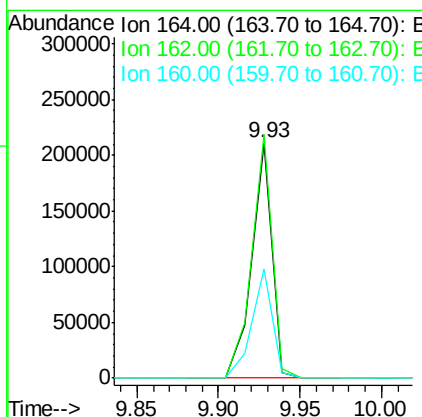


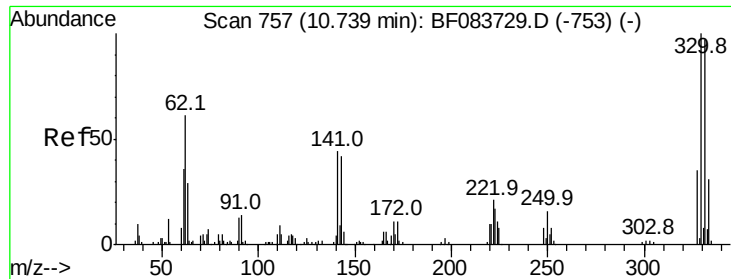




#41
 2,4,6-Tribromophenol
 Concen: 133.26 ng
 RT: 10.72 min Scan# 755
 Delta R.T. -0.03 min
 Lab File: BF083859.D
 Acq: 16 Dec 2015 20:21

Instrument :
 BNA_F
 ClientSampleId :
 COMPOSITE-B-20150873

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.5	0.0	0.0#
141	39.1	0.0	0.0#




Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

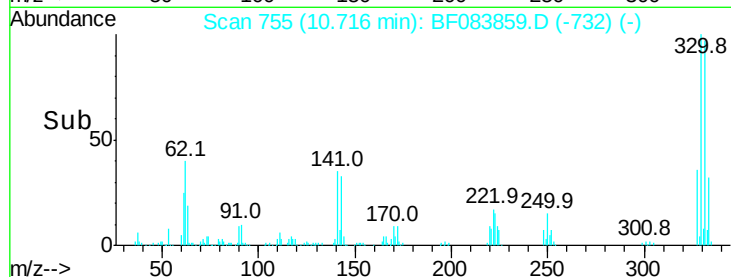
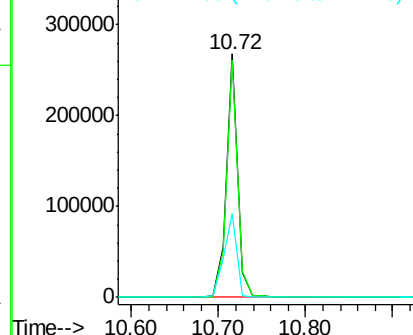



#44
 2-Fluorobiphenyl
 Concen: 89.31 ng
 RT: 9.25 min Scan# 627
 Delta R.T. -0.03 min
 Lab File: BF083859.D
 Acq: 16 Dec 2015 20:21

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.7	28.6	42.8
170	25.0	19.4	29.0



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

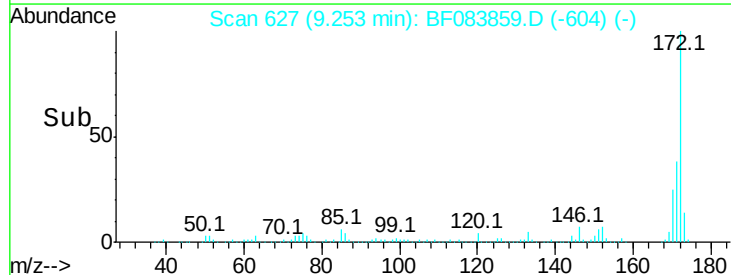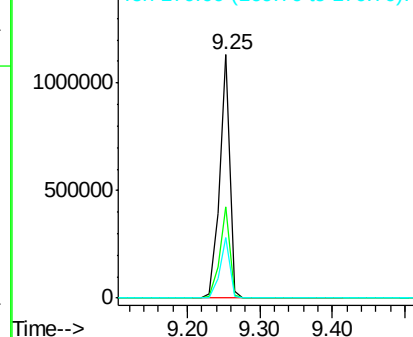

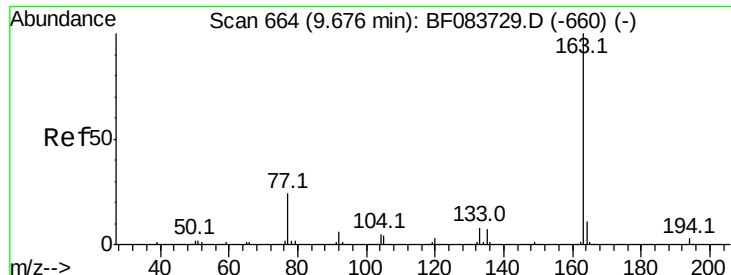

#49

Dimethylphthalate

Concen: 21.19 ng

RT: 9.64 min Scan# 661

Delta R.T. -0.05 min

Lab File: BF083859.D

Acq: 16 Dec 2015 20:21

Instrument :

BNA_F

ClientSampleId :

COMPOSITE-B-20150873


Tot Ion:163 Resp: 299982

Ion Ratio Lower Upper

163 100

194 3.2 2.8 4.2




164 10.0 8.6 13.0

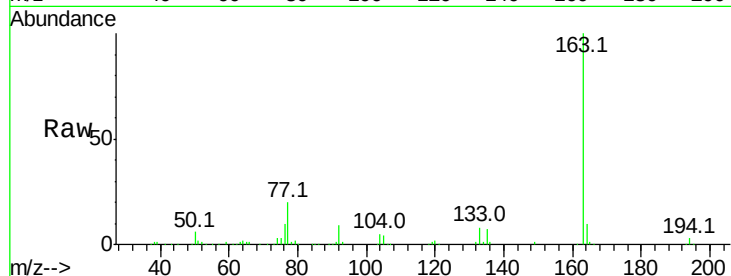

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

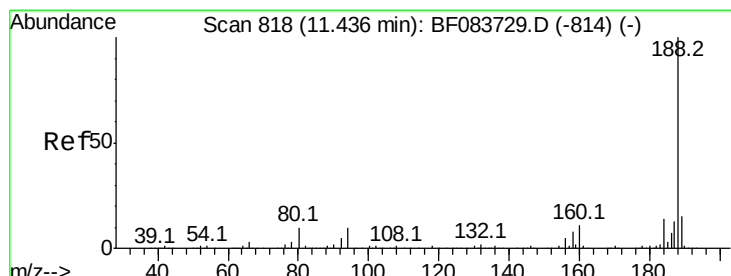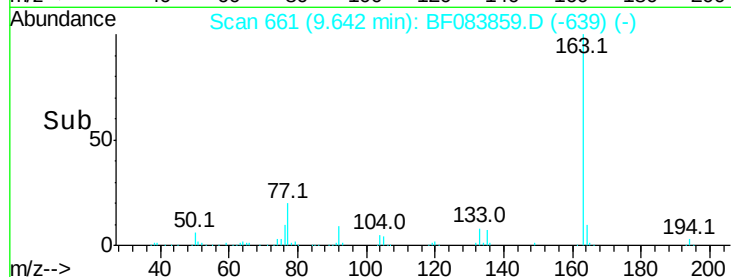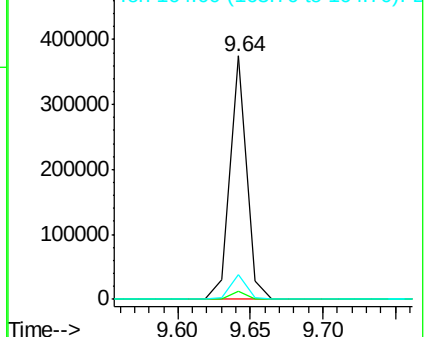

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.41 min Scan# 816

Delta R.T. -0.03 min

Lab File: BF083859.D

Acq: 16 Dec 2015 20:21


Tgt Ion:188 Resp: 310383

Ion Ratio Lower Upper

188 100

94 5.6 9.4 14.2#



80 5.7 10.6 16.0#

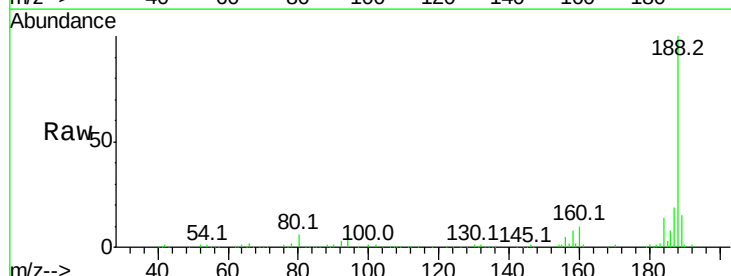


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

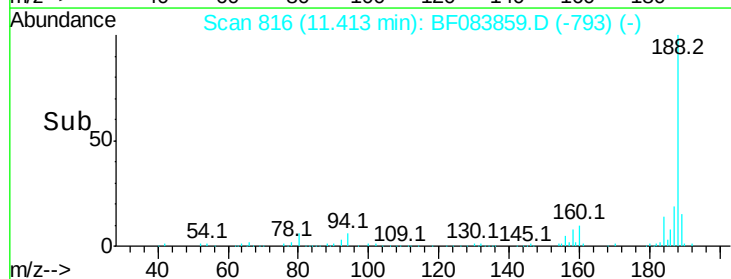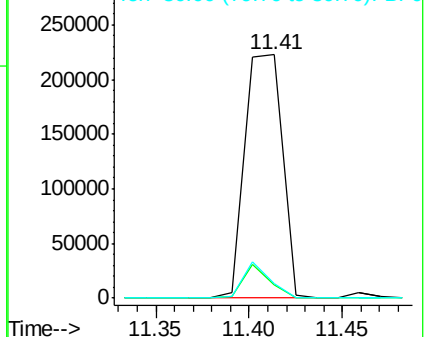

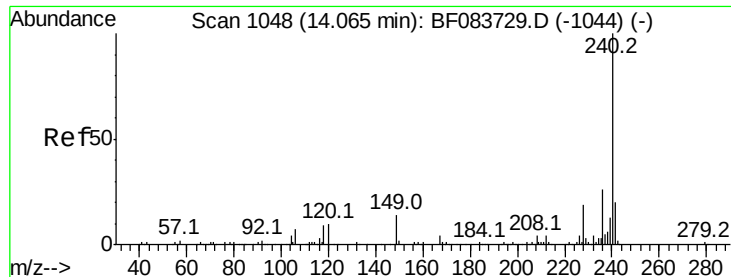

#75

Chrysene-d12

Concen: 20.00 ng

RT: 14.04 min Scan# 1046

Delta R.T. -0.03 min

Lab File: BF083859.D

Acq: 16 Dec 2015 20:21

Instrument :

BNA_F

ClientSampleId :

COMPOSITE-B-20150873


Tot Ion:240 Resp: 214041

Ion Ratio Lower Upper

240 100

120 8.6 8.1 12.1




236 25.1 20.8 31.2



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

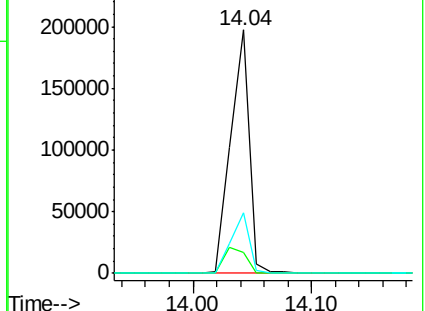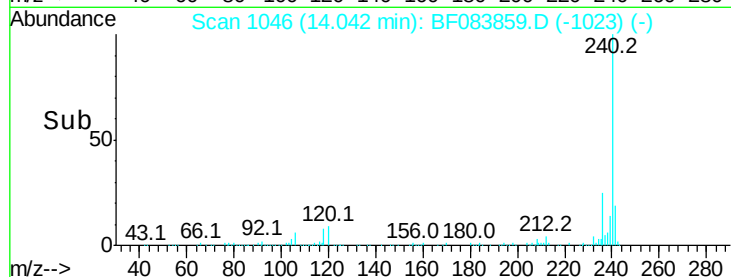

#78

Terphenyl-d14

Concen: 90.20 ng

RT: 12.99 min Scan# 954

Delta R.T. -0.03 min

Lab File: BF083859.D

Acq: 16 Dec 2015 20:21


Tgt Ion:244 Resp: 897548

Ion Ratio Lower Upper

244 100

212 7.6 6.1 9.1



122 13.5 11.0 16.6




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

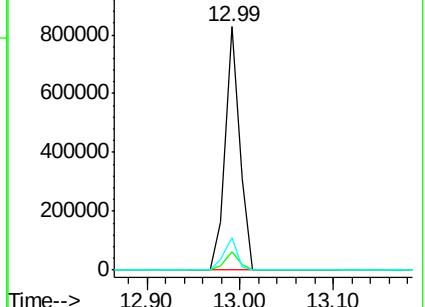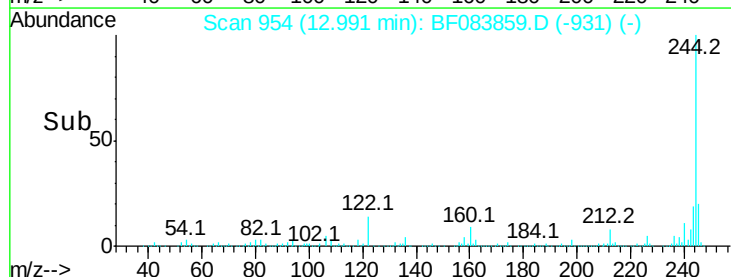

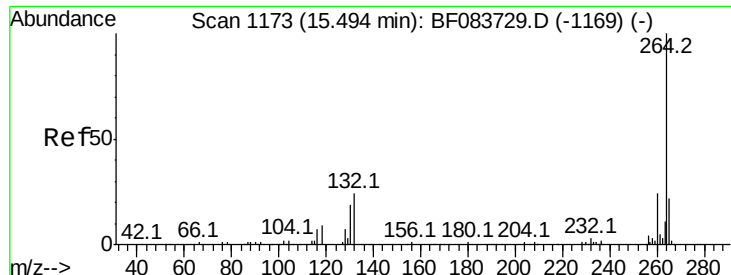


#86
Pervlene-d12
Concen: 20.00 ng
RT: 15.47 min Scan# 1171
Delta R.T. -0.03 min
Lab File: BF083859.D
Acq: 16 Dec 2015 20:21

Instrument :
BNA_F
ClientSampleId :
COMPOSITE-B-20150873

Tot Ion:264 Resp: 173823

Ion	Ratio	Lower	Upper
264	100		
260	22.8	19.4	29.0
265	21.7	17.8	26.6

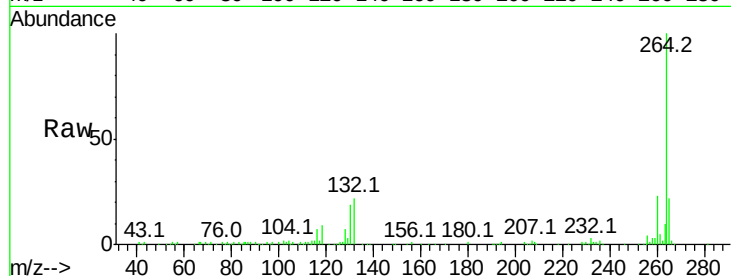

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

