


Data Path : Z:\HPCHEM1\BNA F\Data\BF121615\
 Data File : BF083842.D
 Acq On : 16 Dec 2015 11:18
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 14 01:30:12 2015

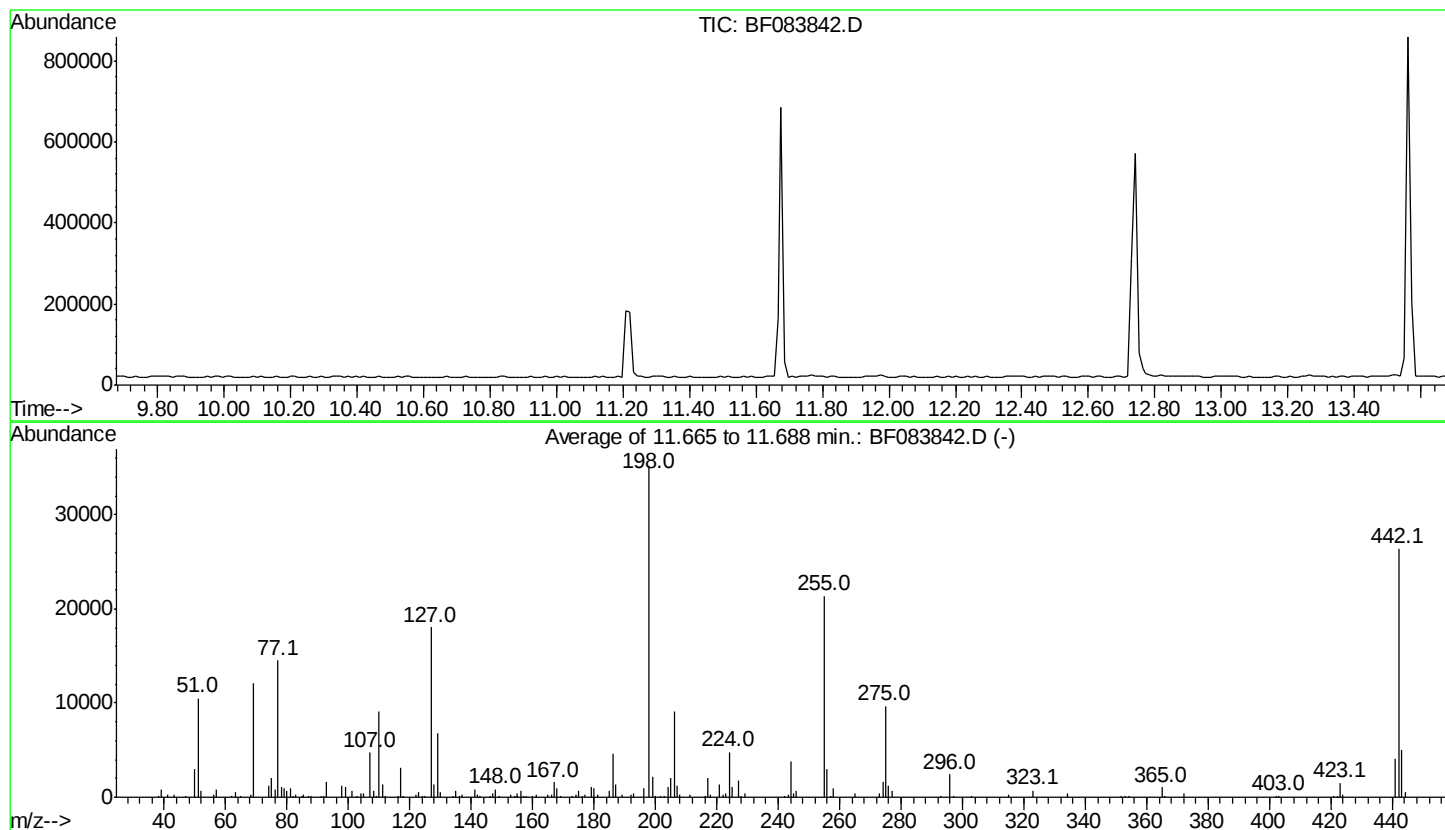

AutoFind: Scans 838, 839, 840; Background Corrected with Scan 835

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.9	10540	PASS
68	69	0.00	2	2.1	252	PASS
69	198	0.00	100	34.2	12058	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.3	18082	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	35221	PASS
199	198	5	9	6.3	2217	PASS
275	198	10	60	27.6	9720	PASS
365	198	1	100	3.0	1040	PASS
441	442	0.01	24	15.5	4093	PASS
442	198	50	100	75.0	26427	PASS
443	442	15	24	18.9	4993	PASS