
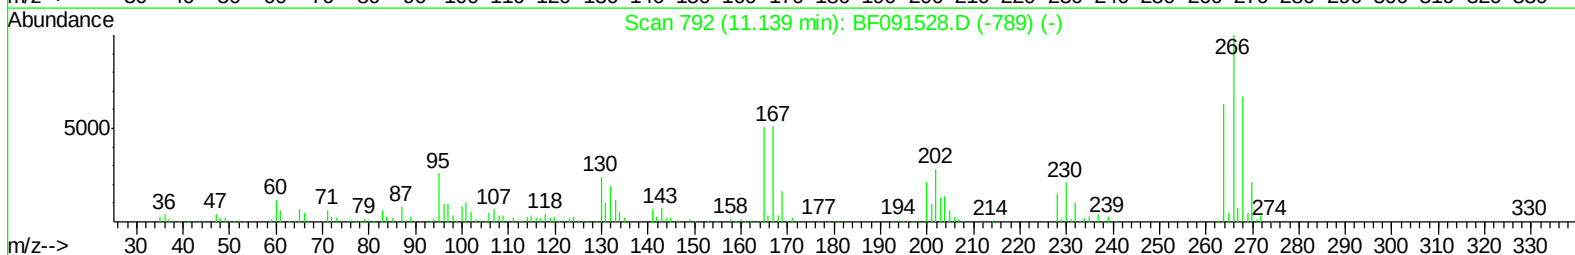
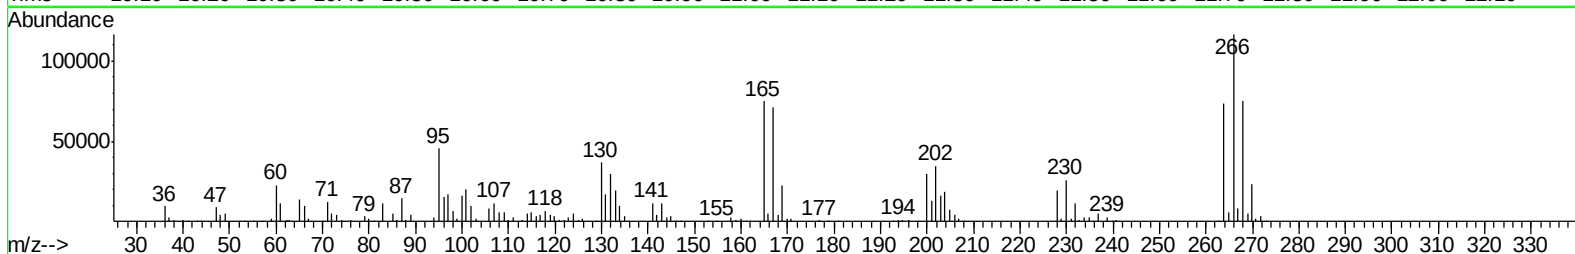


Data Path : Z:\HPCHEM1\BNA_F\Data\BF121616\
Data File : BF091672.D
Acq On : 16 Dec 2016 14:59
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 19 05:01:07 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF120916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 16 00:35:41 2016
Response via : Initial Calibration

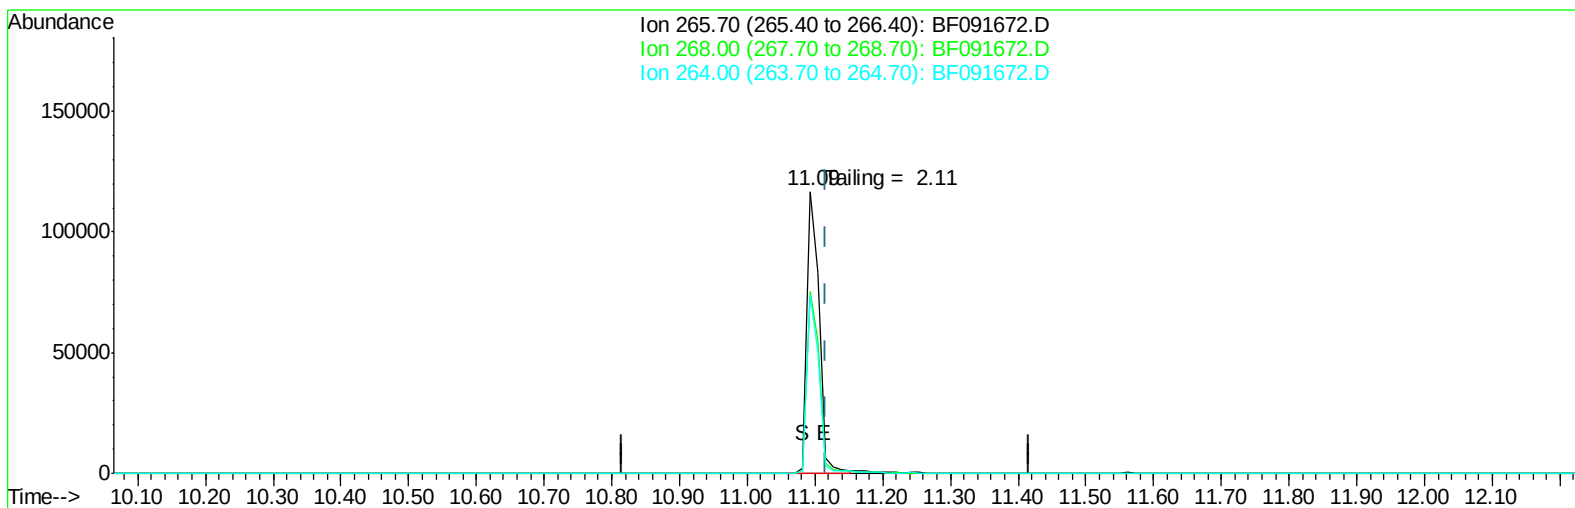

TIC: BF091672.D

(69) Pentachlorophenol (C)




11.093min (-0.023) 57297.46ng

response 149538

Ion	Exp%	Act%
265.70	100	100
268.00	62.90	64.61
264.00	60.20	63.30
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF121616\
Data File : BF091672.D
Acq On : 16 Dec 2016 14:59
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 19 05:01:07 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF120916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 16 00:35:41 2016
Response via : Initial Calibration

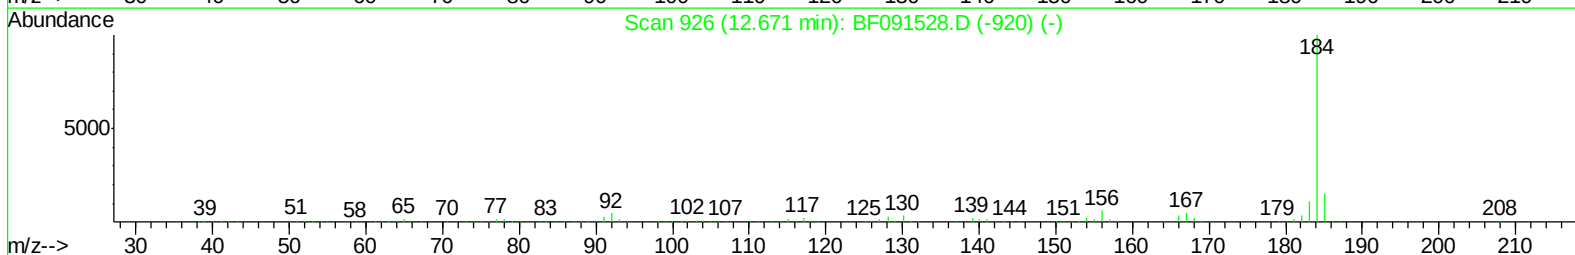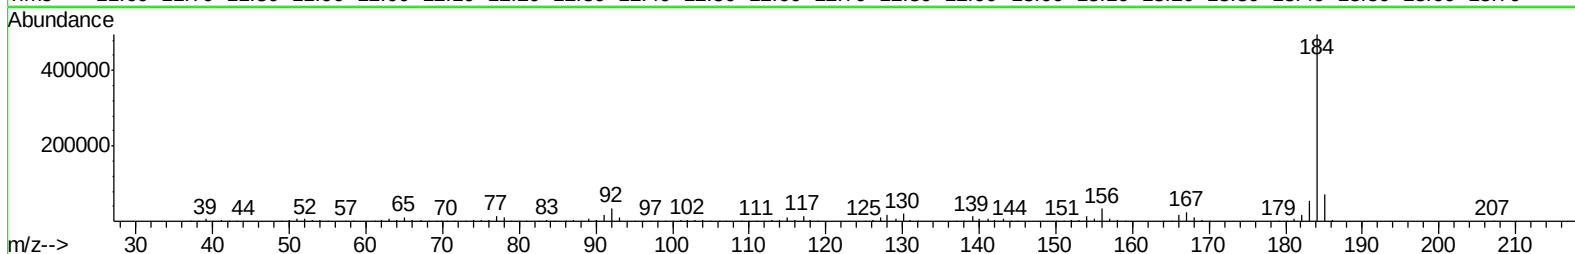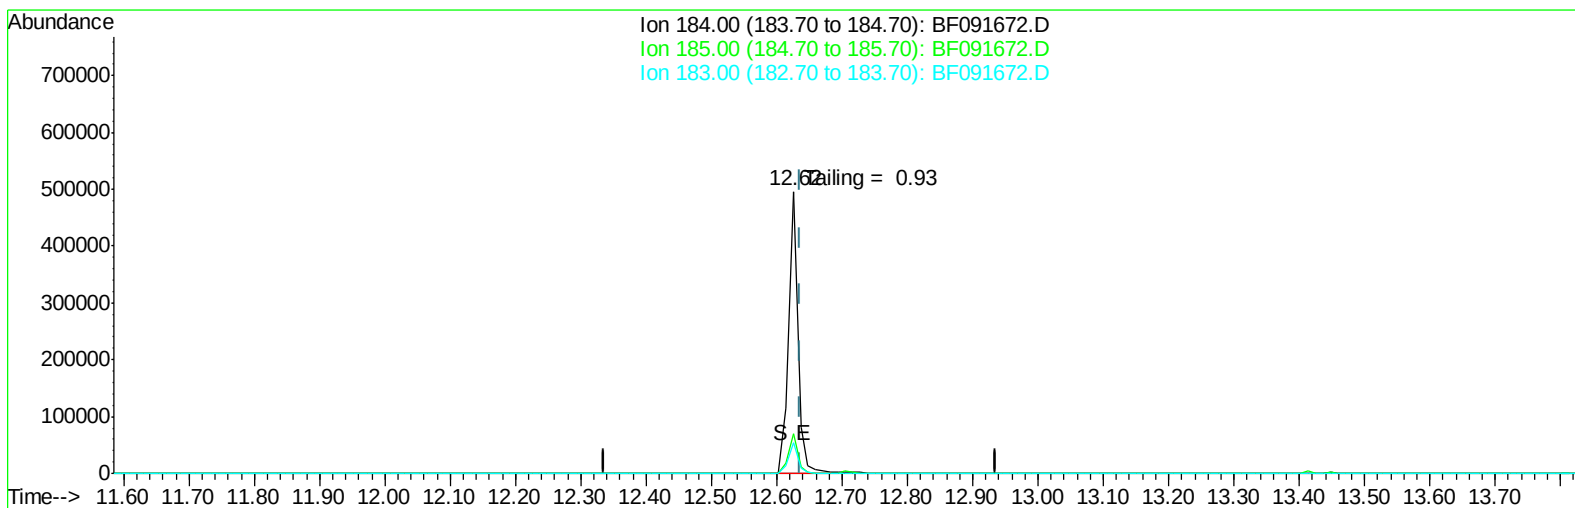

TIC: BF091672.D

(76) Benzidine

12.625min (-0.011) 22347.60ng

response 503044

Ion	Exp%	Act%
184.00	100	100
185.00	16.40	14.22
183.00	11.10	11.14
0.00	0.00	0.00