
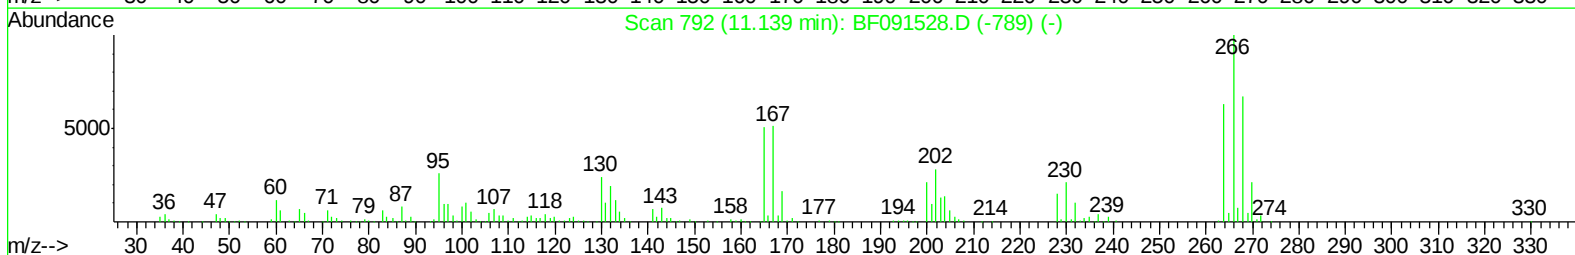
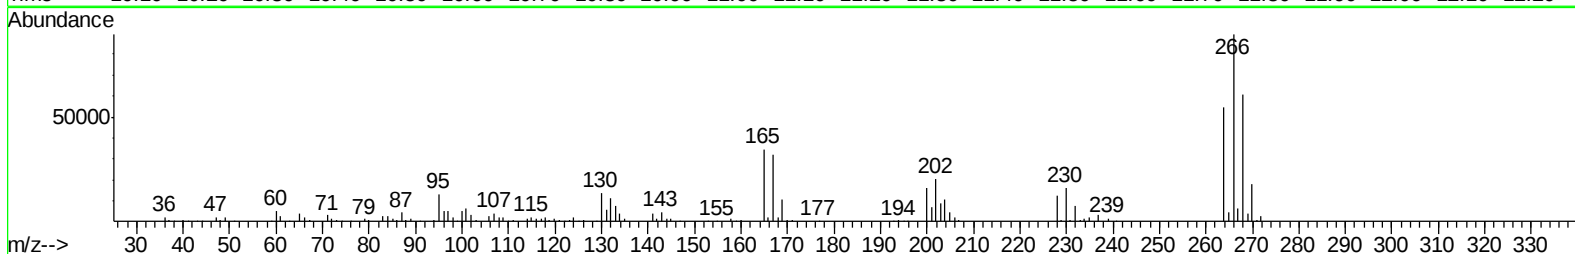


Data Path : Z:\HPCHEM1\BNA\_F\Data\BF121616\  
Data File : BF091698.D  
Acq On : 17 Dec 2016 3:57  
Operator : UM/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 19 05:02:39 2016  
Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF120916.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Dec 16 00:35:41 2016  
Response via : Initial Calibration

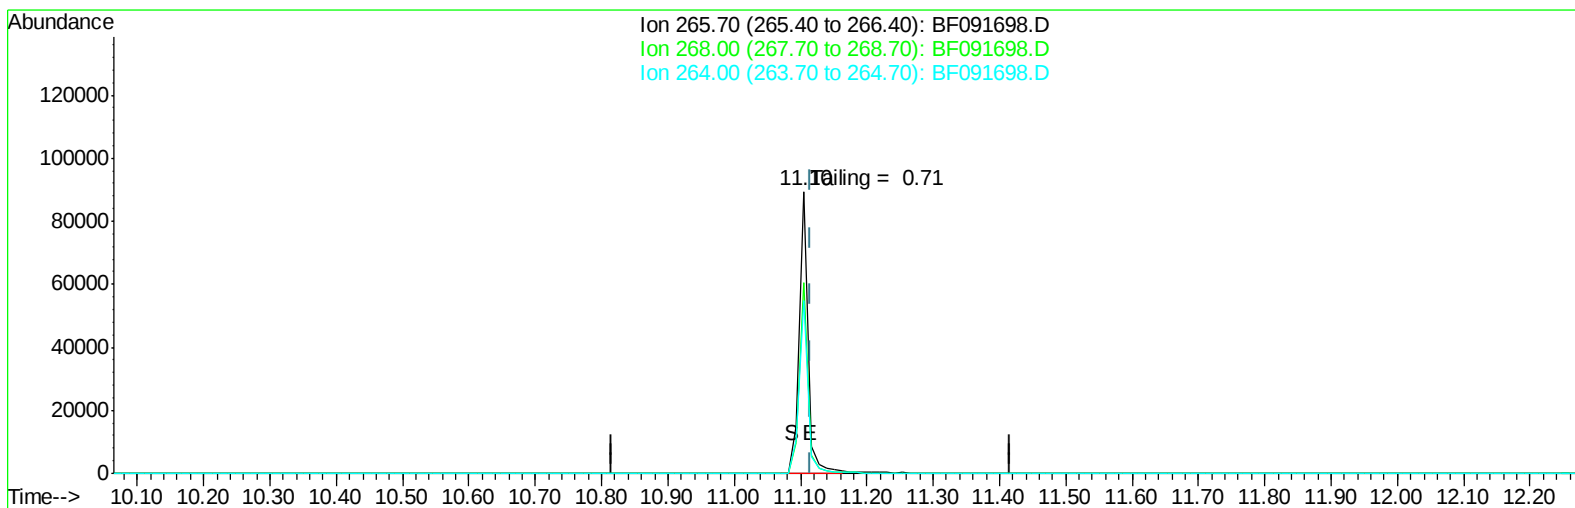

TIC: BF091698.D

(69) Pentachlorophenol (C)




11.105min (-0.012) 40770.99ng

response 83902

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 62.90 | 67.96 |
| 264.00 | 60.20 | 61.39 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA\_F\Data\BF121616\  
Data File : BF091698.D  
Acq On : 17 Dec 2016 3:57  
Operator : UM/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 19 05:02:39 2016  
Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF120916.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Dec 16 00:35:41 2016  
Response via : Initial Calibration

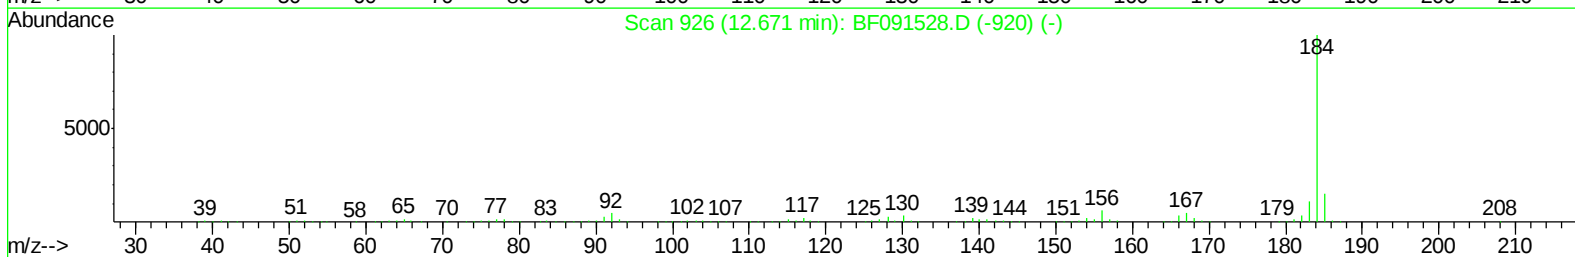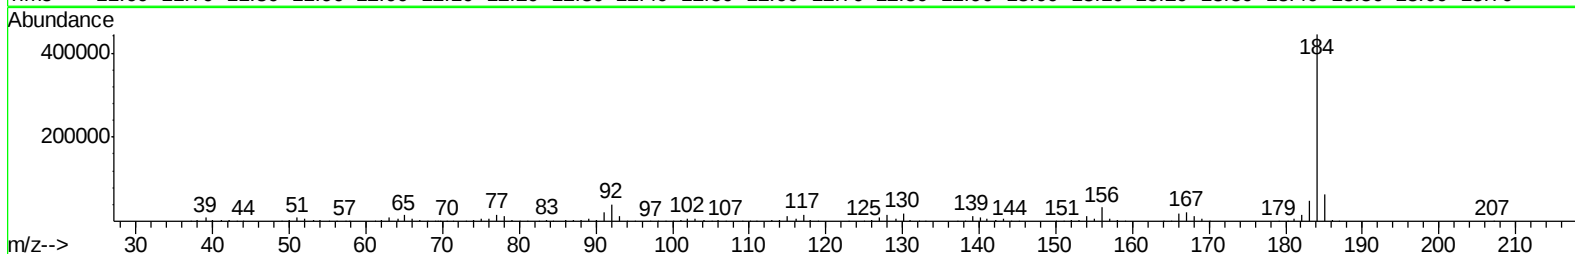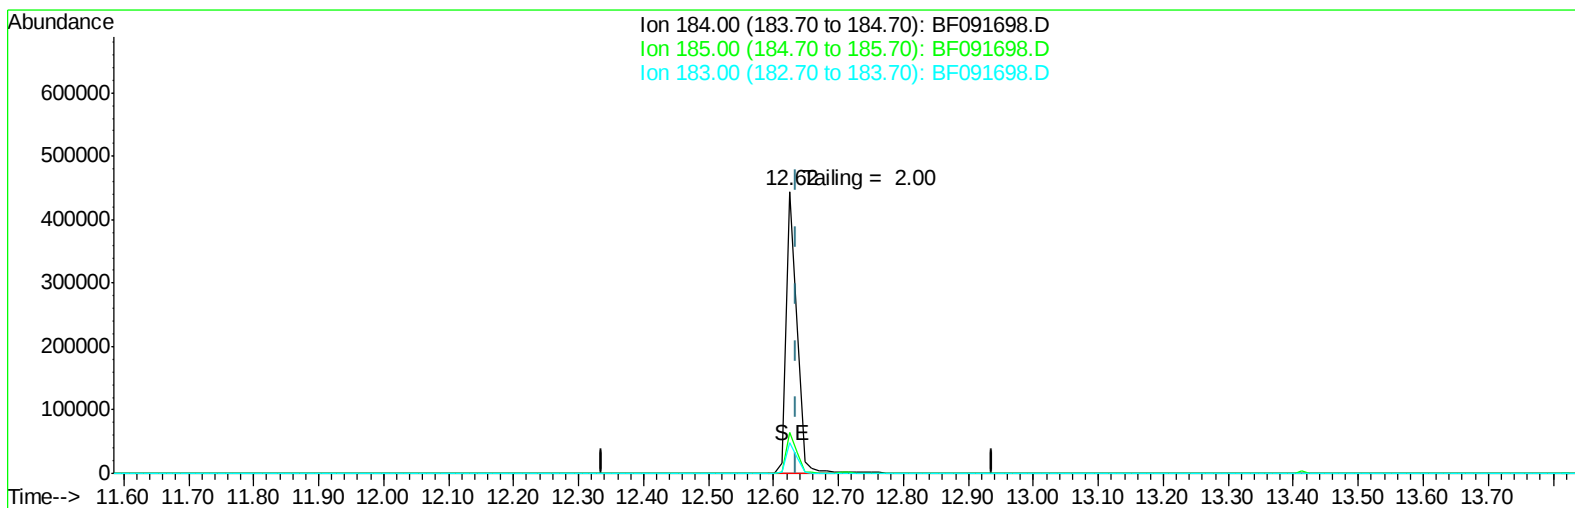

TIC: BF091698.D

(76) Benzidine

12.625min (-0.012) 13412.85ng

response 505555

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 16.40 | 14.75 |
| 183.00 | 11.10 | 11.07 |
| 0.00   | 0.00  | 0.00  |