


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF121616\
Data File : BF091672.D
Acq On : 16 Dec 2016 14:59
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF120916.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Dec 16 00:35:41 2016

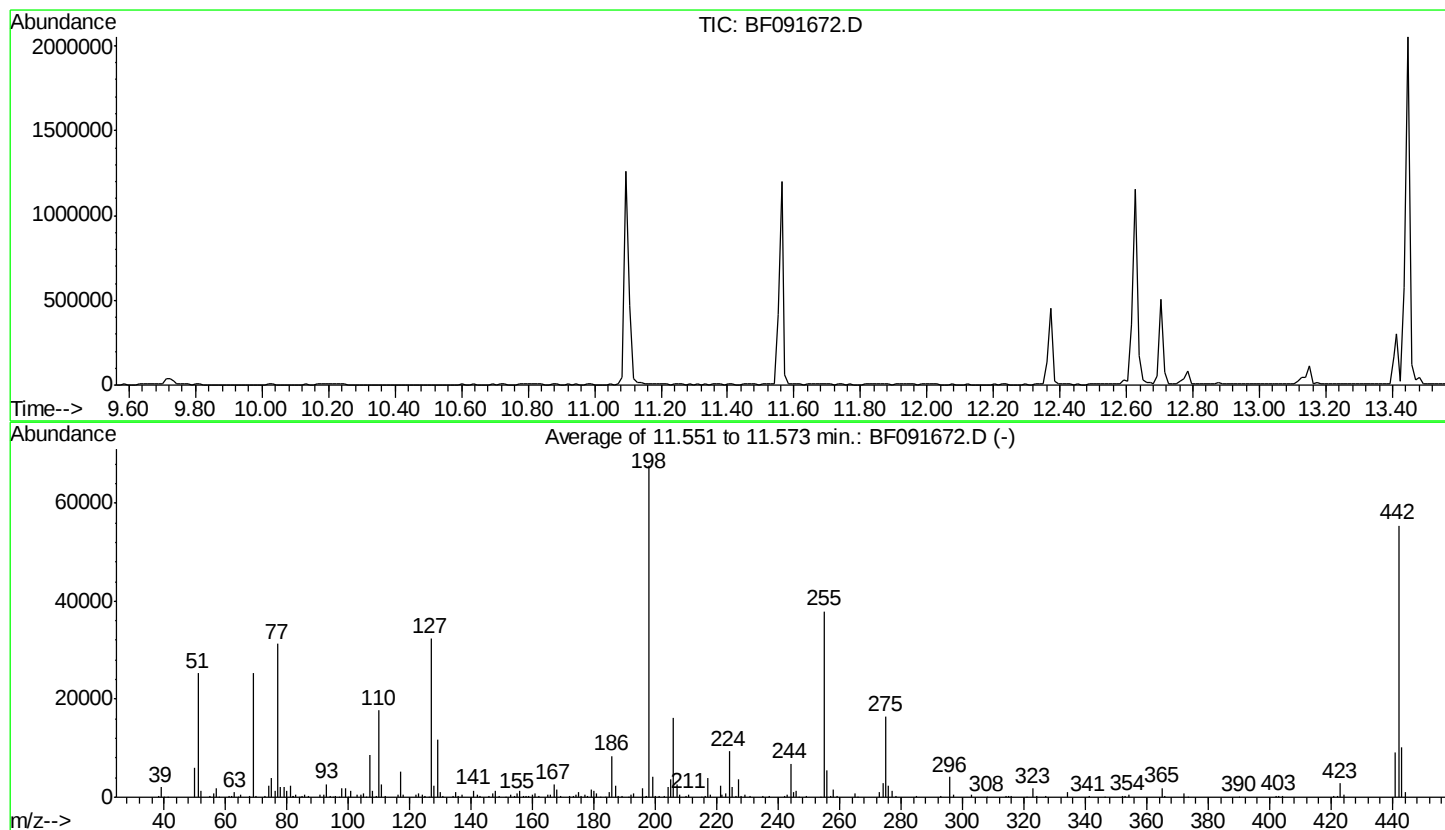

AutoFind: Scans 828, 829, 830; Background Corrected with Scan 824

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.4	25321	PASS
68	69	0.00	2	1.5	375	PASS
69	198	0.00	100	37.6	25425	PASS
70	69	0.00	2	0.6	140	PASS
127	198	10	80	47.8	32363	PASS
197	198	0.00	2	0.5	332	PASS
198	198	100	100	100.0	67644	PASS
199	198	5	9	6.3	4257	PASS
275	198	10	60	24.2	16392	PASS
365	198	1	100	2.8	1868	PASS
441	442	0.01	24	16.5	9137	PASS
442	198	50	100	82.0	55471	PASS
443	442	15	24	18.4	10205	PASS