


Data Path : Z:\HPCHEM1\BNA F\DATA\BF121616\
 Data File : BF091698.D
 Acq On : 17 Dec 2016 3:57
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF120916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 16 00:35:41 2016

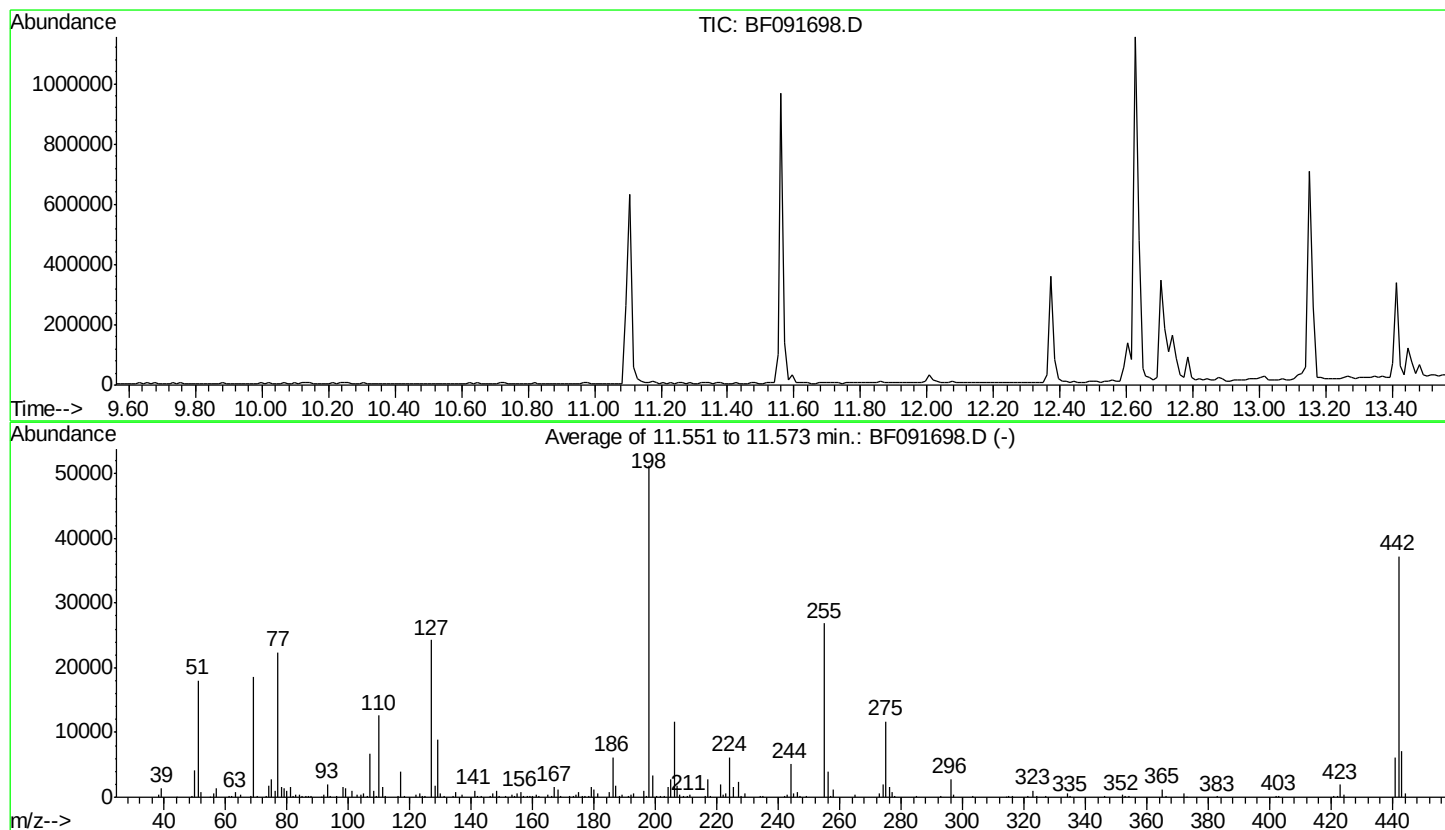

AutoFind: Scans 828, 829, 830; Background Corrected with Scan 825

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.1	17997	PASS
68	69	0.00	2	1.1	210	PASS
69	198	0.00	100	36.4	18666	PASS
70	69	0.00	2	0.6	108	PASS
127	198	10	80	47.4	24260	PASS
197	198	0.00	2	0.4	202	PASS
198	198	100	100	100.0	51213	PASS
199	198	5	9	6.5	3312	PASS
275	198	10	60	22.9	11750	PASS
365	198	1	100	2.5	1264	PASS
441	442	0.01	24	16.8	6230	PASS
442	198	50	100	72.6	37186	PASS
443	442	15	24	19.3	7188	PASS