
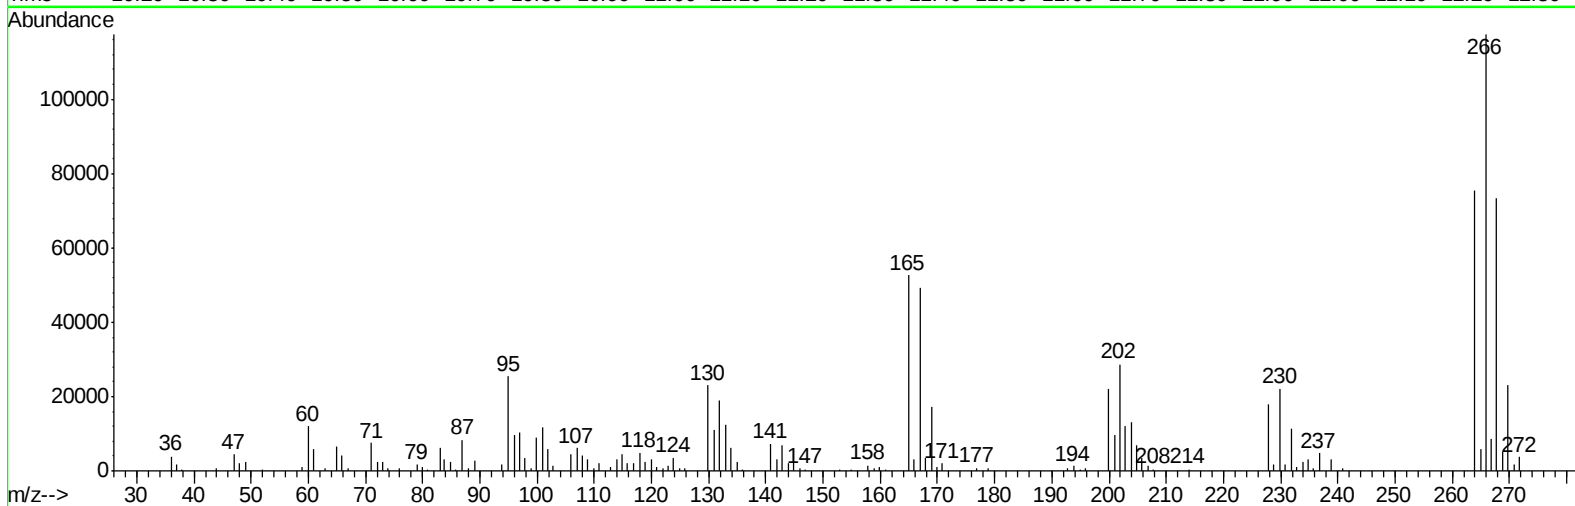


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF121619\
Data File : BF118199.D
Acq On : 16 Dec 2019 15:55
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 17 08:42:56 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF120619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 17:34:43 2019
Response via : Initial Calibration

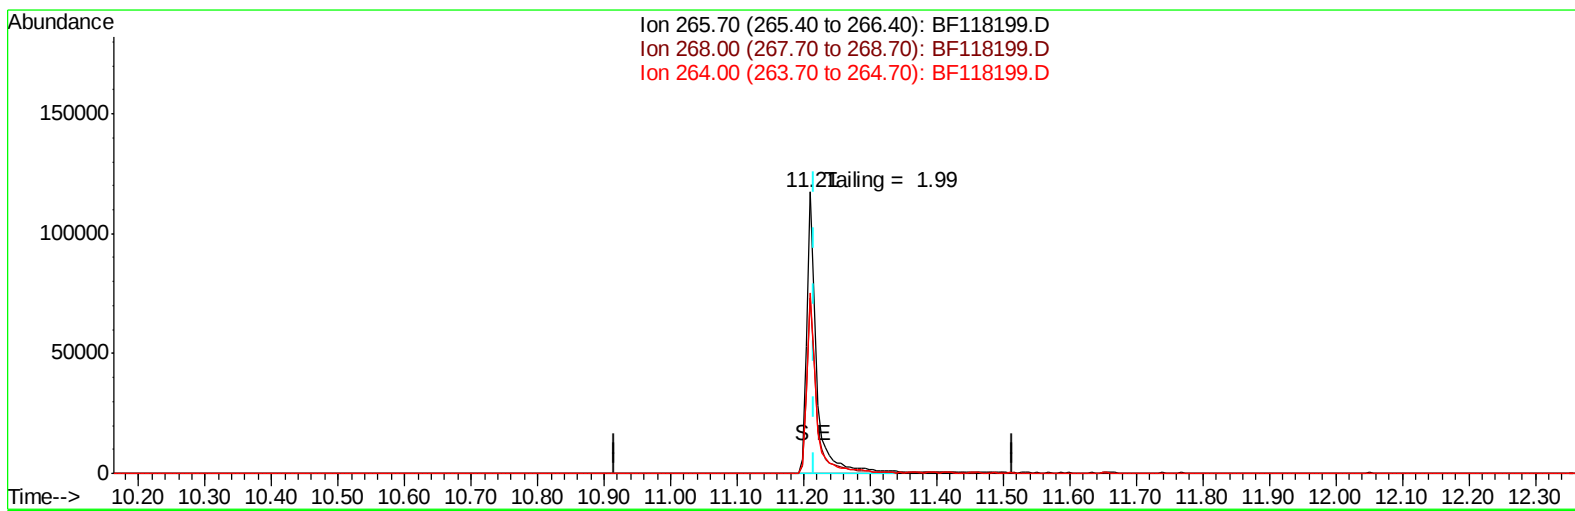

TIC: BF118199.D

(70) Pentachlorophenol (C)



11.210min (-0.006) 48738.70ng

response 123799

Ion	Exp%	Act%
265.70	100	100
268.00	63.40	62.51
264.00	60.90	64.31
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF121619\
Data File : BF118199.D
Acq On : 16 Dec 2019 15:55
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 17 08:42:56 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF120619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 17:34:43 2019
Response via : Initial Calibration

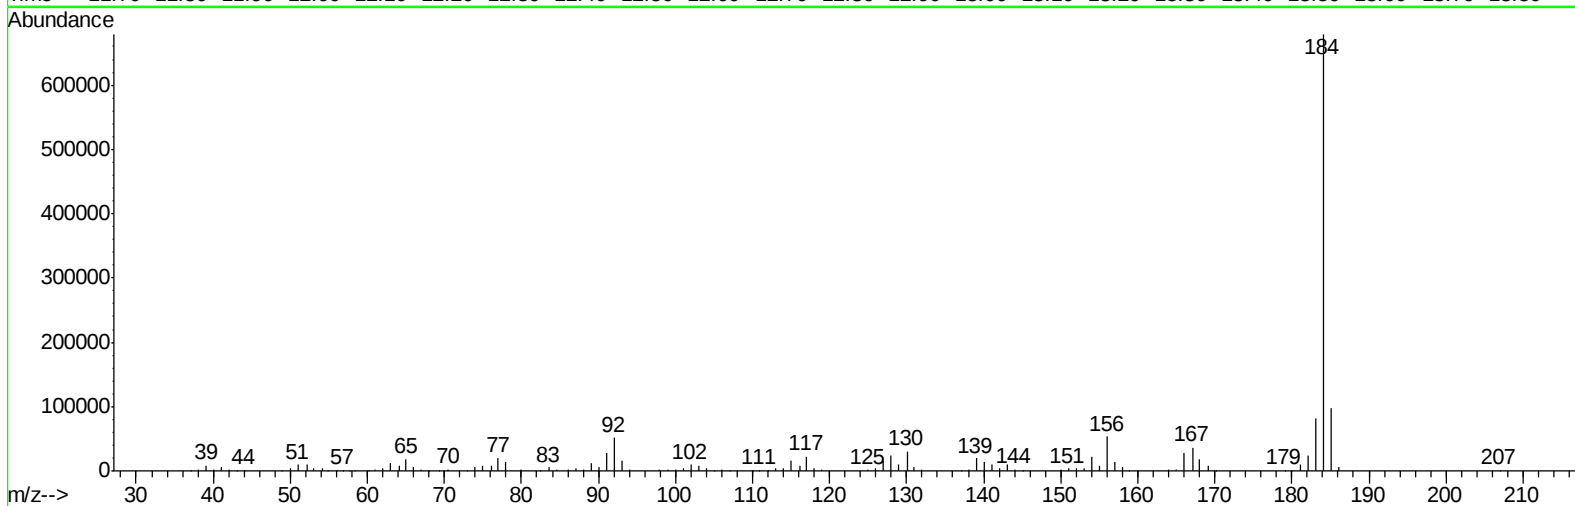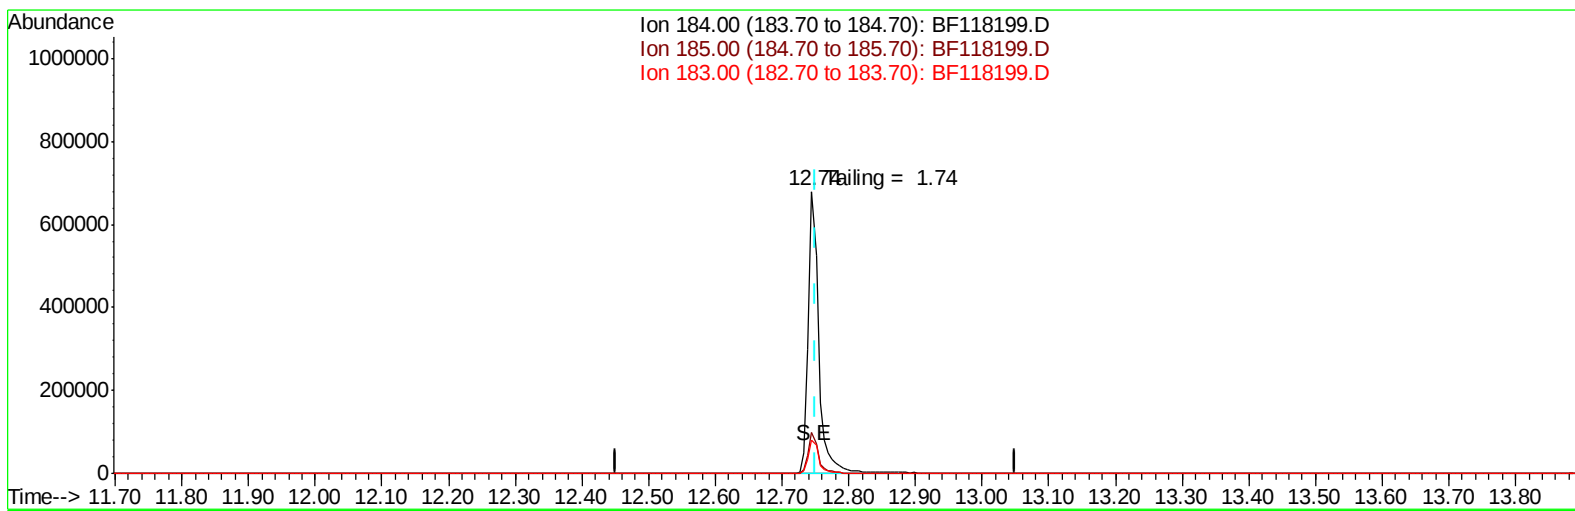

TIC: BF118199.D

(77) Benzidine

12.745min (-0.006) 0.00ng

response 708750

Ion	Exp%	Act%
184.00	100	100
185.00	15.40	14.35
183.00	12.40	12.06
0.00	0.00	0.00