


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF121619\
 Data File : BF118199.D
 Acq On : 16 Dec 2019 15:55
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 06 17:34:43 2019

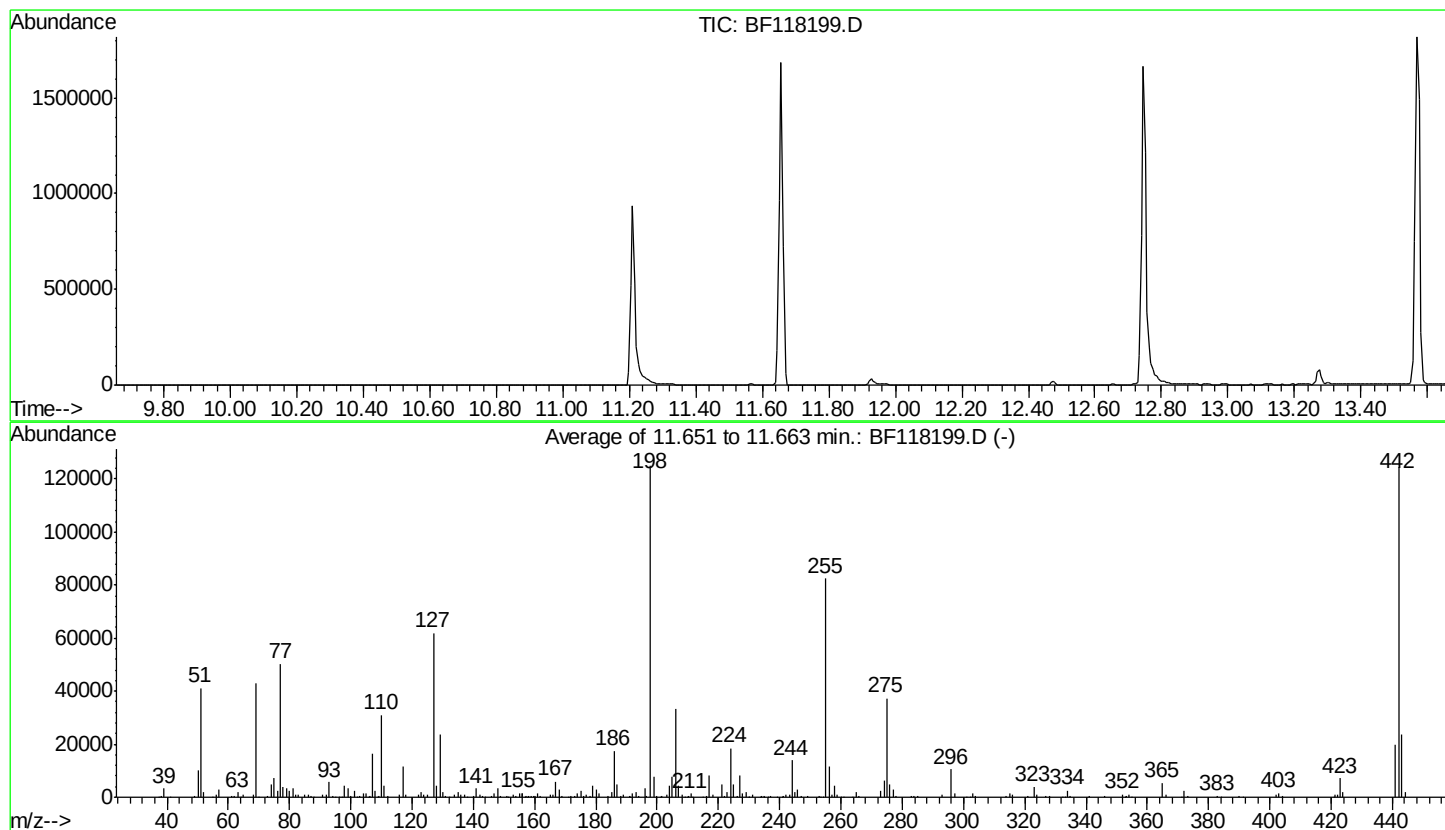

AutoFind: Scans 1626, 1627, 1628; Background Corrected with Scan 1621

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.0	41279	PASS
68	69	0.00	2	1.9	819	PASS
69	198	0.00	100	34.2	42824	PASS
70	69	0.00	2	0.5	223	PASS
127	198	10	80	49.5	61933	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	125058	PASS
199	198	5	9	6.3	7824	PASS
275	198	10	60	29.9	37416	PASS
365	198	1	100	4.3	5360	PASS
441	198	0.01	100	15.7	19670	PASS
442	198	50	100	99.7	124701	PASS
443	442	15	24	18.9	23577	PASS