
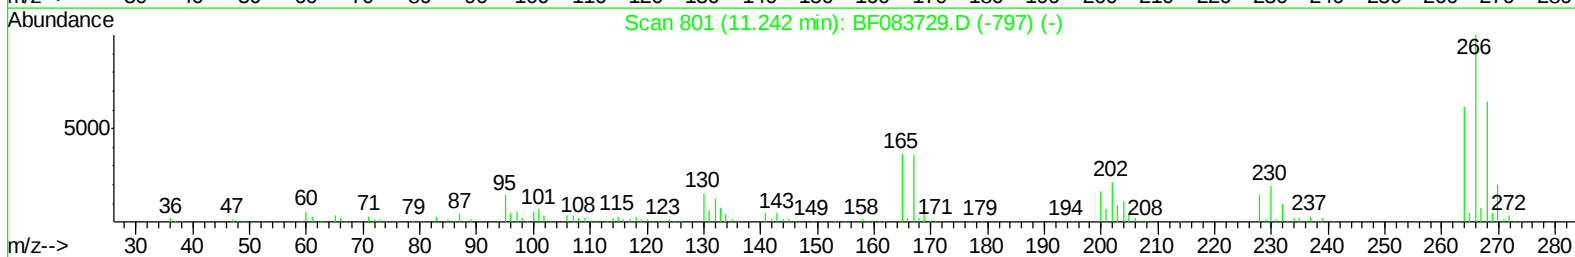
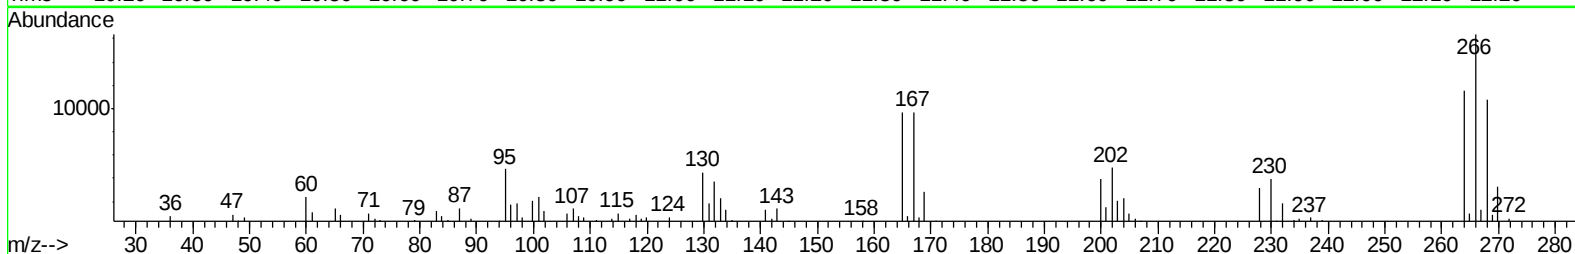


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF121715\
Data File : BF083864.D
Acq On : 17 Dec 2015 3:24
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 17 06:16:07 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 14 01:30:12 2015
Response via : Initial Calibration

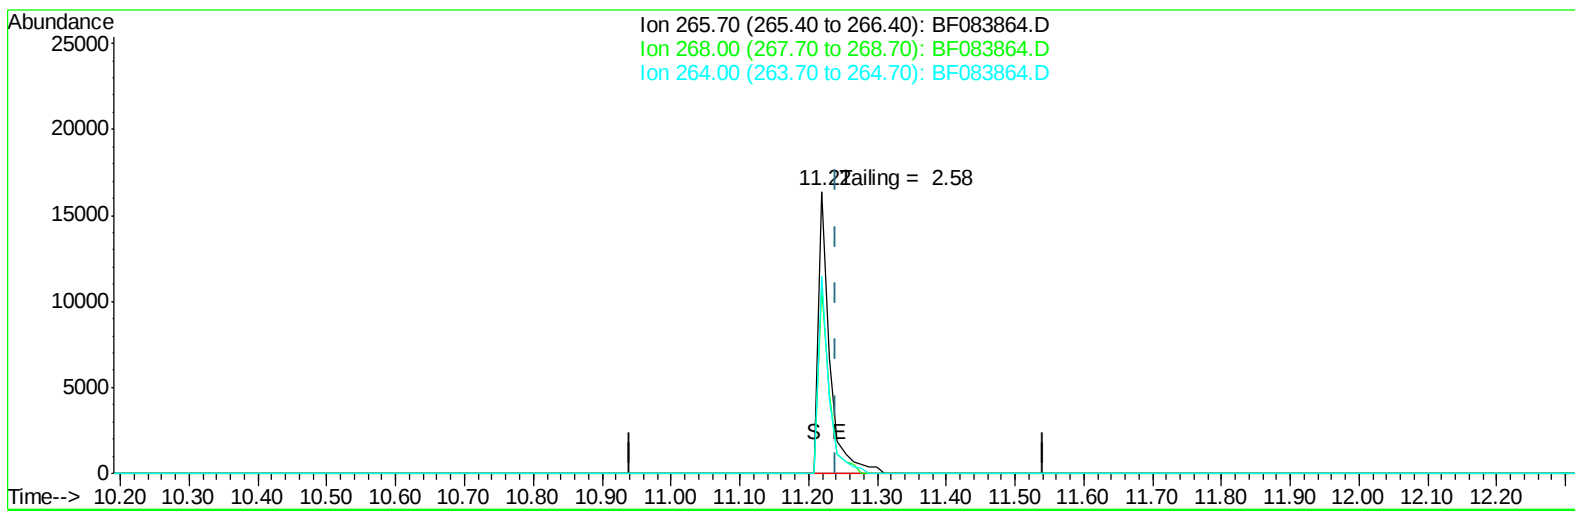

TIC: BF083864.D

(69) Pentachlorophenol (C)




11.219min (-0.022) 0.00ng

response 19191

Ion	Exp%	Act%
265.70	100	100
268.00	62.70	65.95
264.00	64.30	70.20
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF121715\
Data File : BF083864.D
Acq On : 17 Dec 2015 3:24
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 17 06:16:07 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 14 01:30:12 2015
Response via : Initial Calibration

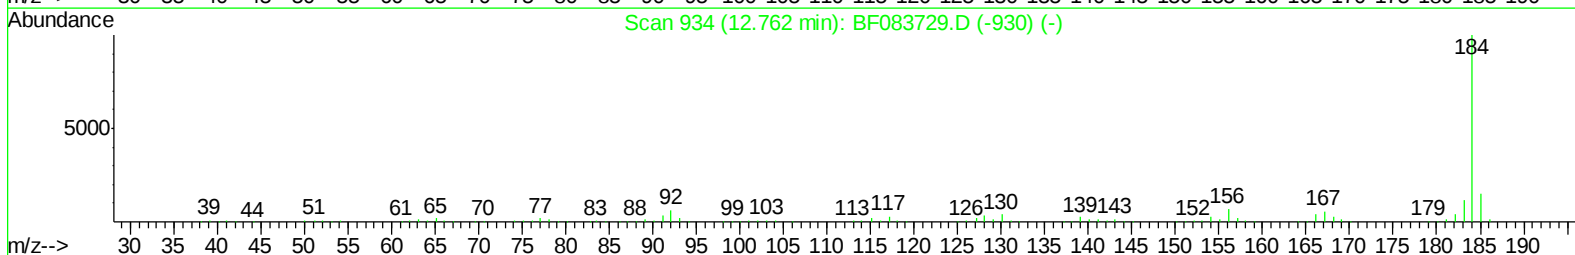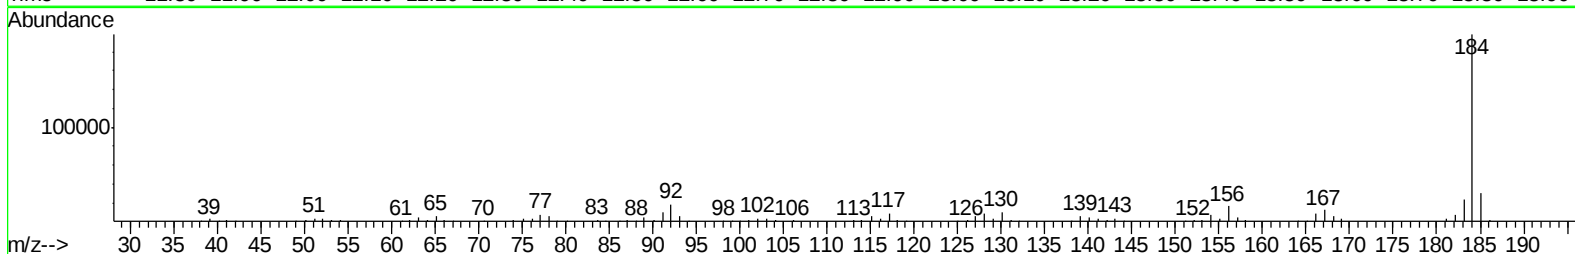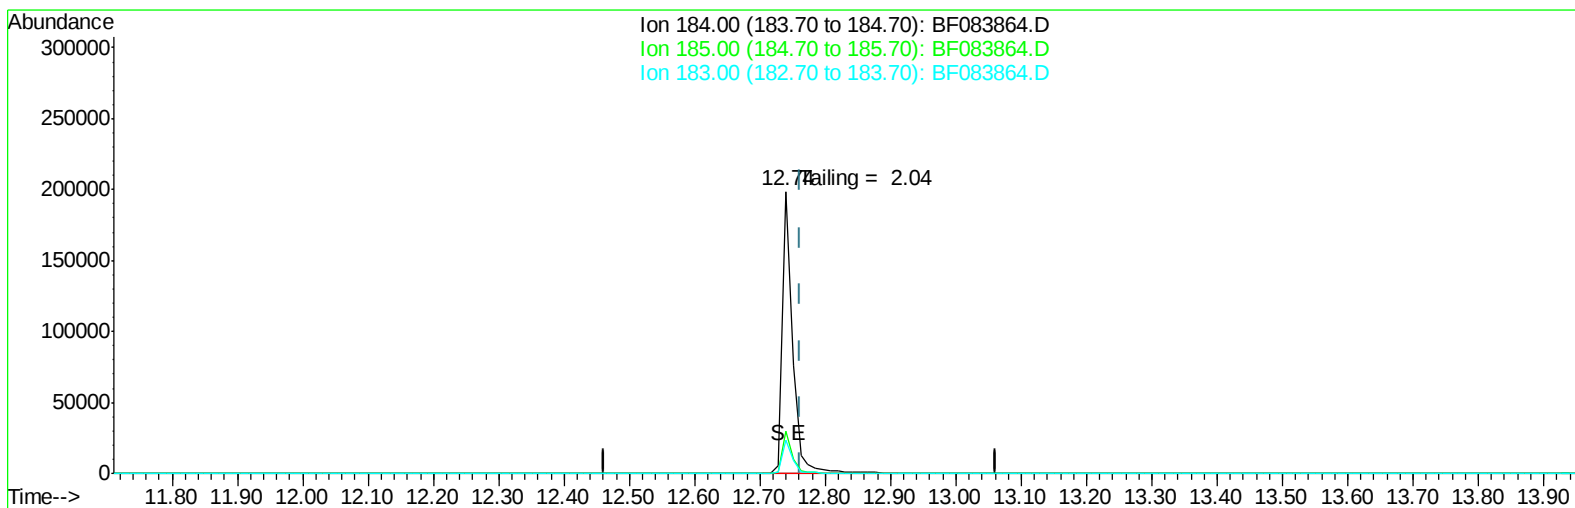

TIC: BF083864.D

(76) Benzidine

12.739min (-0.023) 0.00ng

response 215015

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	14.88
183.00	11.20	11.77
0.00	0.00	0.00