


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF121715\
 Data File : BF083864.D
 Acq On : 17 Dec 2015 3:24
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 14 01:30:12 2015

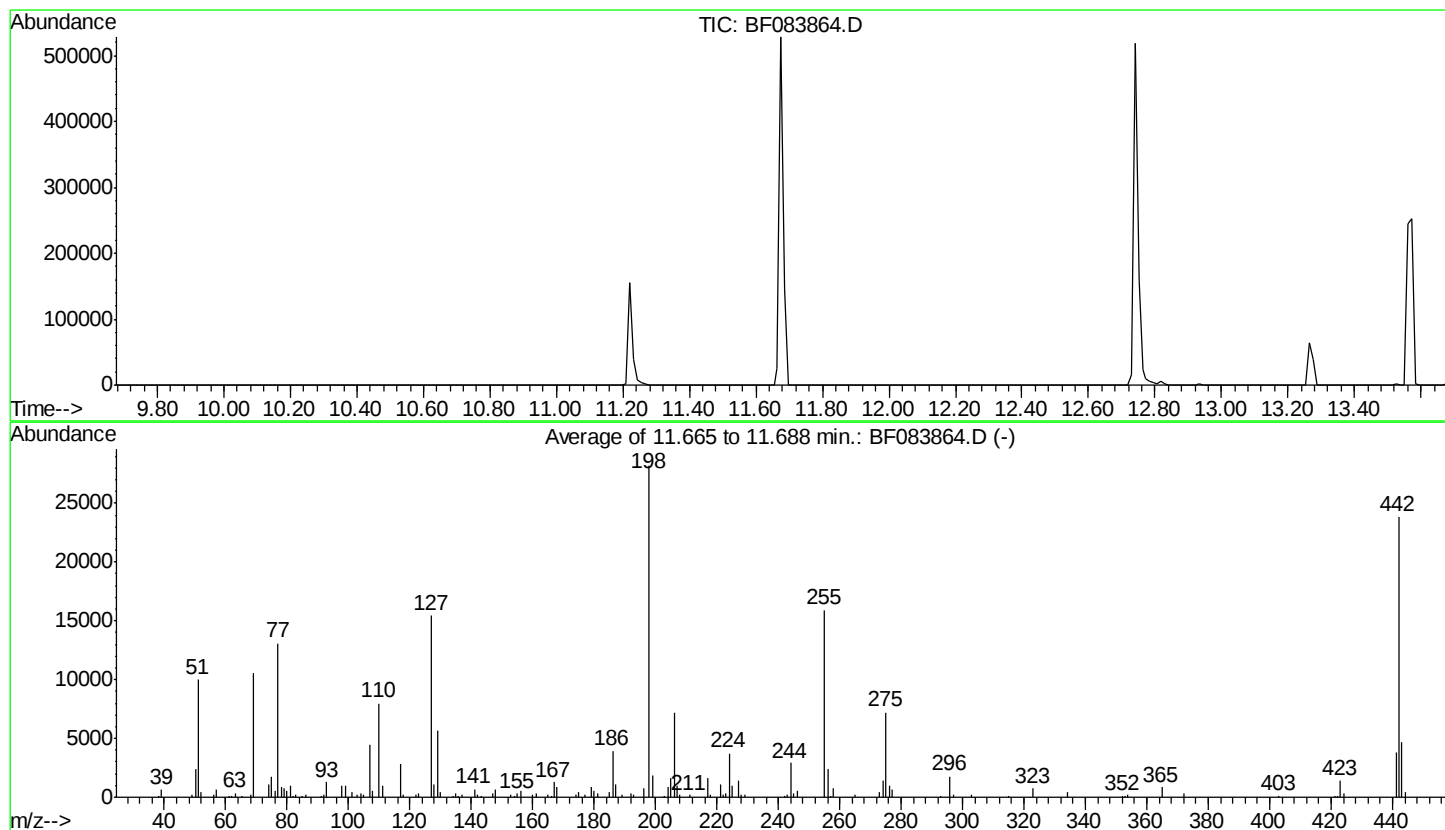

AutoFind: Scans 838, 839, 840; Background Corrected with Scan 835

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.4	9988	PASS
68	69	0.00	2	1.6	169	PASS
69	198	0.00	100	37.4	10552	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.6	15411	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	28200	PASS
199	198	5	9	6.5	1819	PASS
275	198	10	60	25.5	7193	PASS
365	198	1	100	3.1	861	PASS
441	442	0.01	24	16.2	3860	PASS
442	198	50	100	84.7	23888	PASS
443	442	15	24	19.7	4715	PASS