
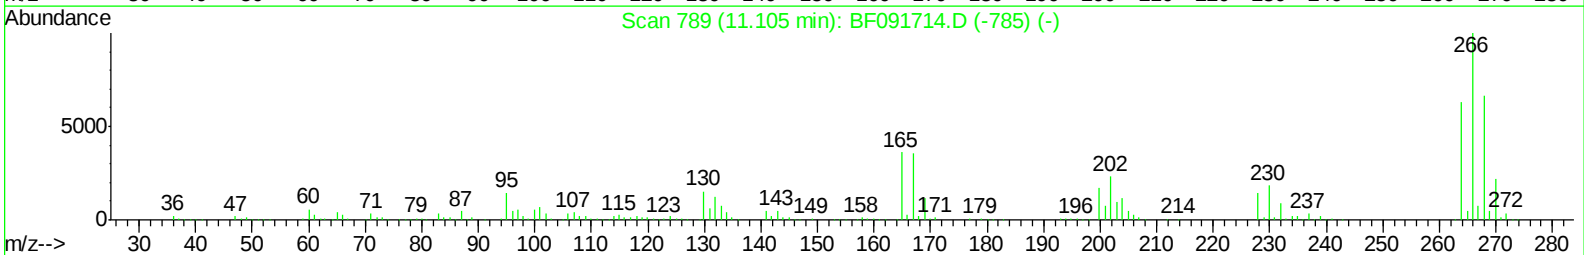
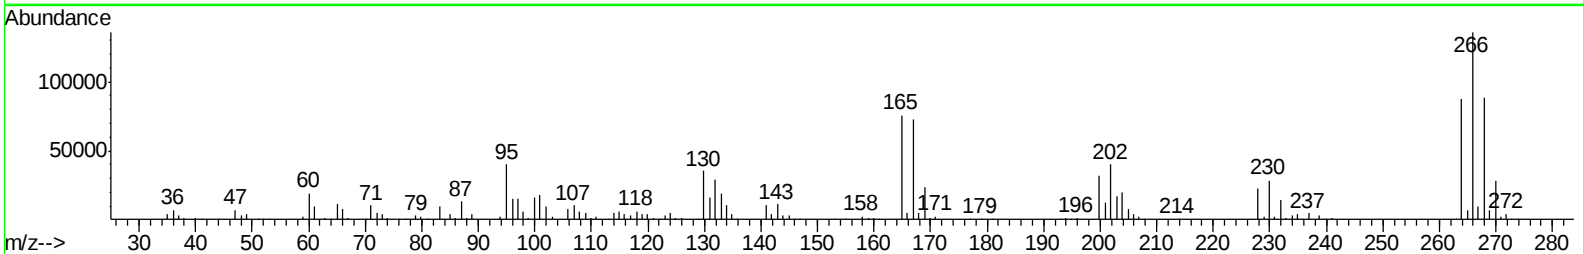


```
Data Path : Z:\HPCHEM1\BNA_F\Data\BF121716\  
Data File : BF091709.D  
Acq On    : 17 Dec 2016  12:23  
Operator  : UM/SJ  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1      Sample Multiplier: 1
```

Quant Time: Dec 19 05:59:36 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 17 22:53:54 2016
Response via : Initial Calibration

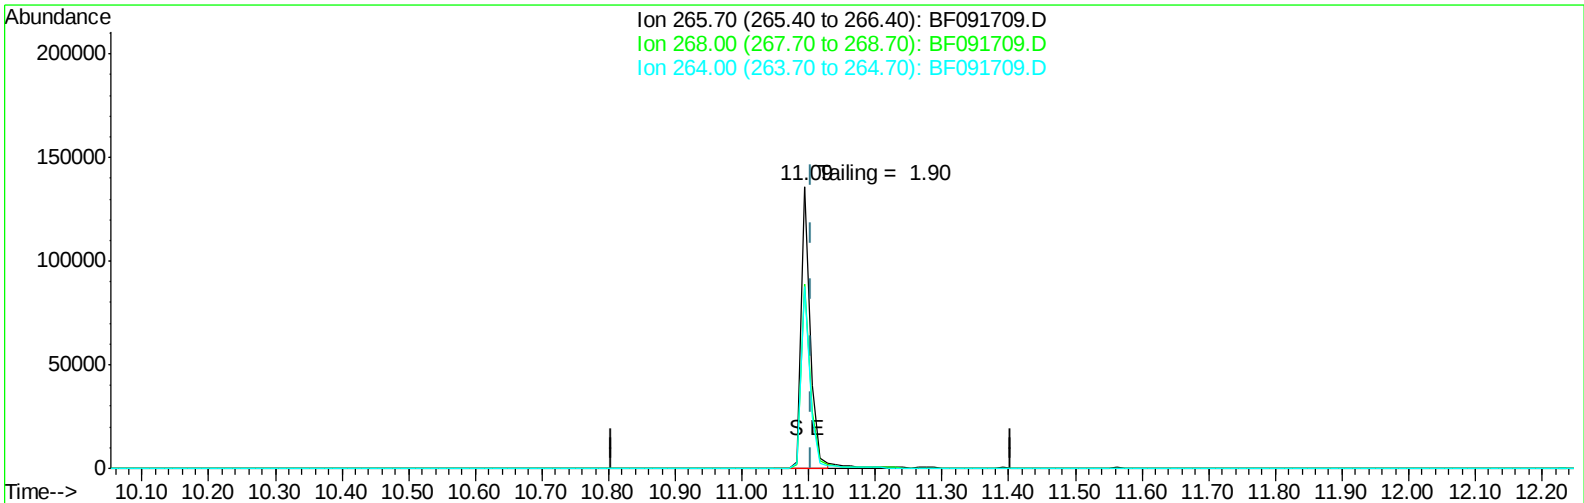

TIC: BF091709.D

(69) Pentachlorophenol (C)




11.093min (-0.011) 11123.38ng

```
response 133360
```

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	65.44
264.00	62.90	64.51
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF121716\
Data File : BF091709.D
Acq On : 17 Dec 2016 12:23
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 19 05:59:36 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 17 22:53:54 2016
Response via : Initial Calibration

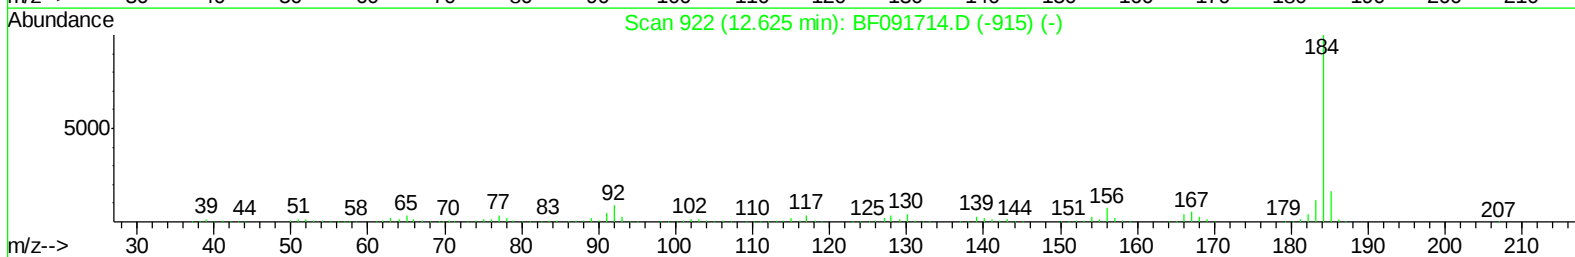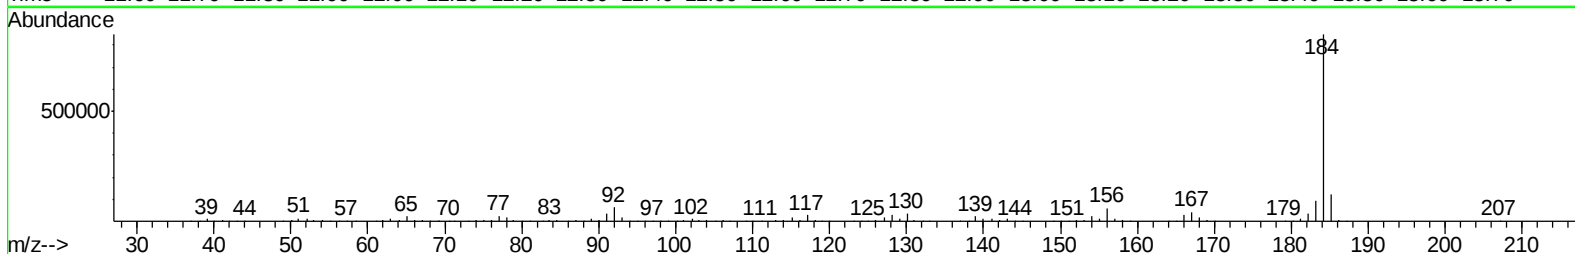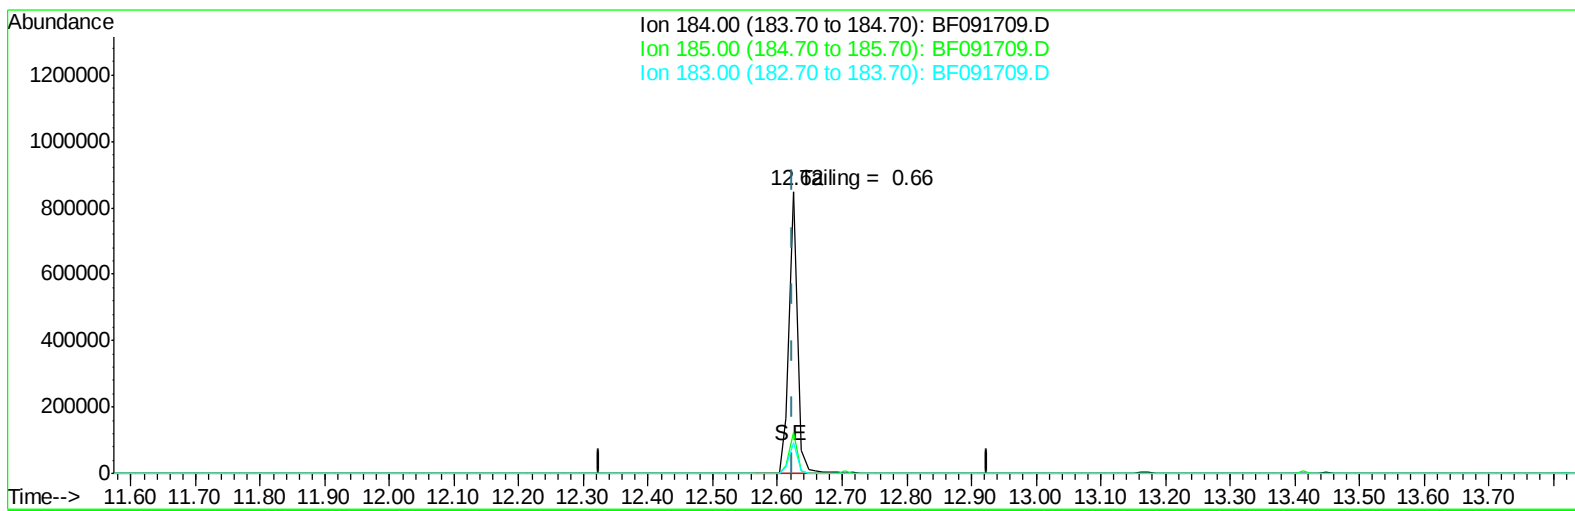

TIC: BF091709.D

(76) Benzidine

12.625min (+0.000) 2605.21ng

response 774814

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.44
183.00	11.50	11.12
0.00	0.00	0.00