

```
Data Path : Z:\HPCHEM1\BNA_F\Data\BF121716\  
Data File : BF091719.D  
Acq On    : 17 Dec 2016   23:21  
Operator  : UM/SJ  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1      Sample Multiplier: 1
```

Data File : BF091719.D

Acq On : 17 Dec 2016 23:21

Operator : UM/SJ

Sample : DFTPP

Misc :

ALS Vial : 1 Sample Multiplier: 1


Quant Time: Dec 19 06:00:31 2016

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121716.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Sat Dec 17 22:53:54 2016

Response via : Initial Calibration

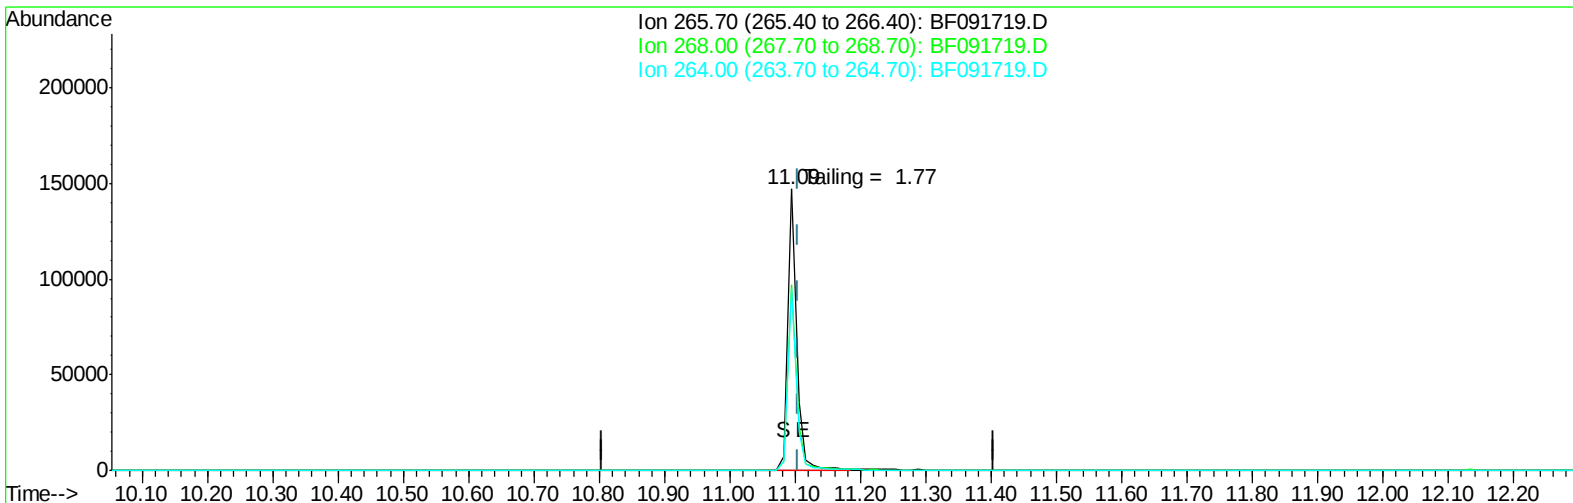

Ion 265.70 (265.40 to 266.40): BF091719.D

Ion 268.00 (267.70 to 268.70): BF091719.D


Ion 264.00 (263.70 to 264.70): BF091719.D

11.09ailing = 1.77


11.09ailing = 1.77

\$14

Time--> 10.10 10.20 10.30 10.40 10.50 10.60 10.70 10.80 10.90 11.00 11.10 11.20 11.30 11.40 11.50 11.60 11.70 11.80 11.90 12.00 12.10 12.20

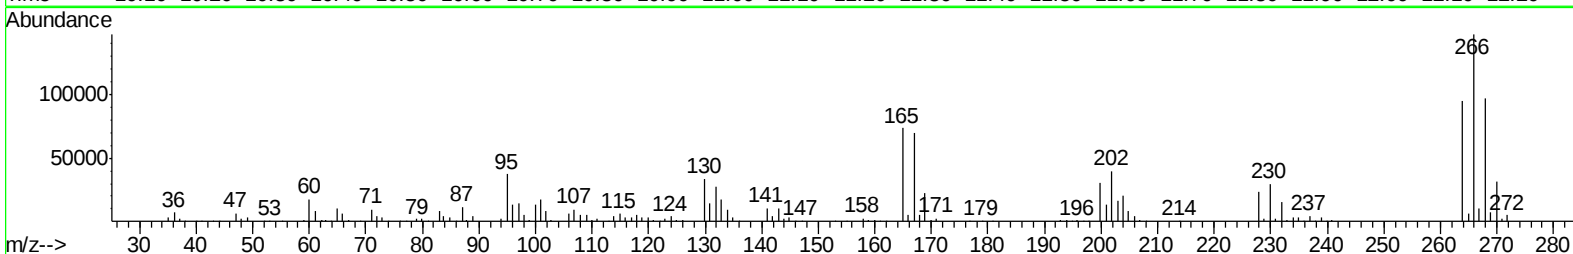

m/z--> 30 40 50 60 70 80 90 100 110 120 130 140 150 160 170 180 190 200 210 220 230 240 250 260 270 280

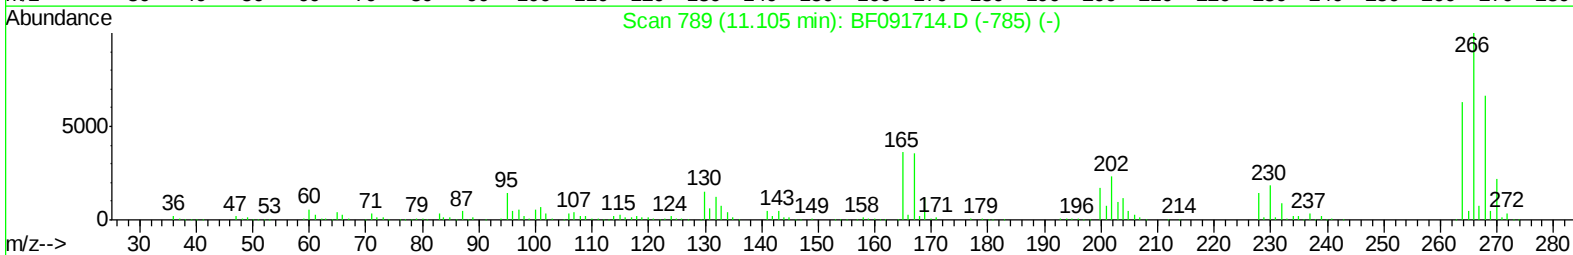

Scan 789 (11.105 min): BF091714.D (-785) (-)

m/z--> 30 40 50 60 70 80 90 100 110 120 130 140 150 160 170 180 190 200 210 220 230 240 250 260 270 280

TIC: BF091719.D

(69) Pentachlorophenol (C)

11.094min (-0.011) 6067.77ng

response 141969

Ion	Exp%	Act%
-----	------	------

265.70	100	100
--------	-----	-----




268.00 66.60 66.01

264.00	62.90	64.52
--------	-------	-------

0.00 0.00 0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF121716\
Data File : BF091719.D
Acq On : 17 Dec 2016 23:21
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 19 06:00:31 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 17 22:53:54 2016
Response via : Initial Calibration

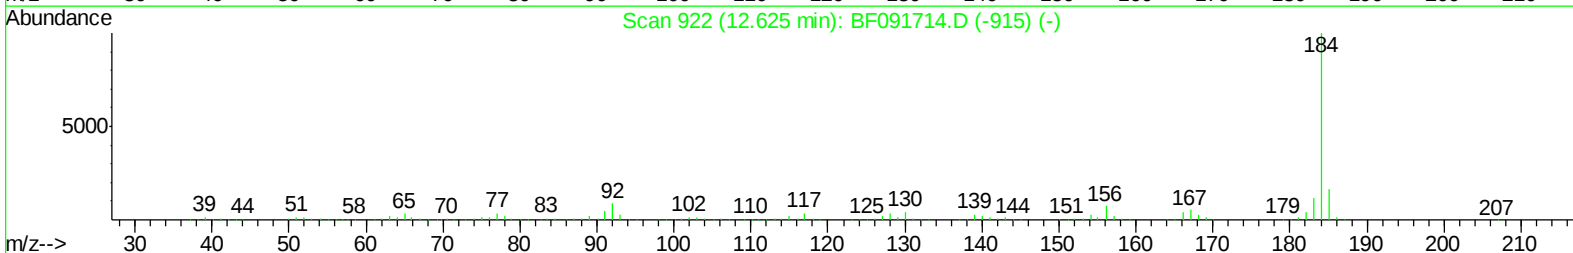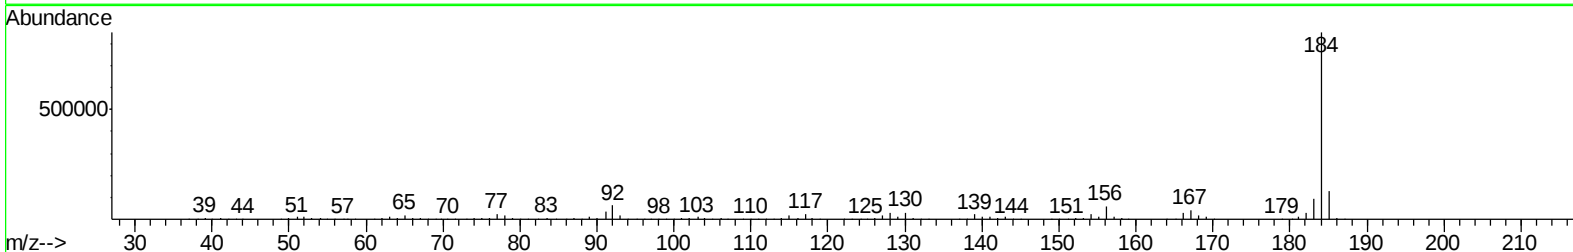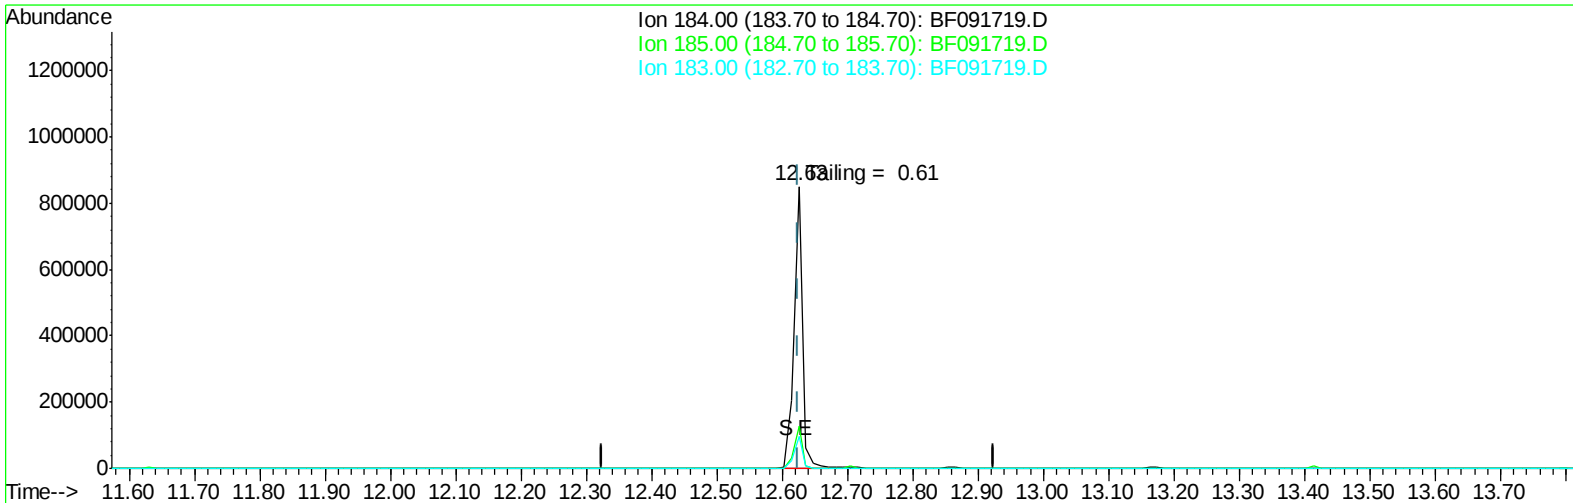

TIC: BF091719.D

(76) Benzidine

12.625min (+0.000) 480.62ng

response 801049

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	15.01
183.00	11.50	11.23
0.00	0.00	0.00