


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF121716\
 Data File : BF091709.D
 Acq On : 17 Dec 2016 12:23
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Dec 17 22:53:54 2016

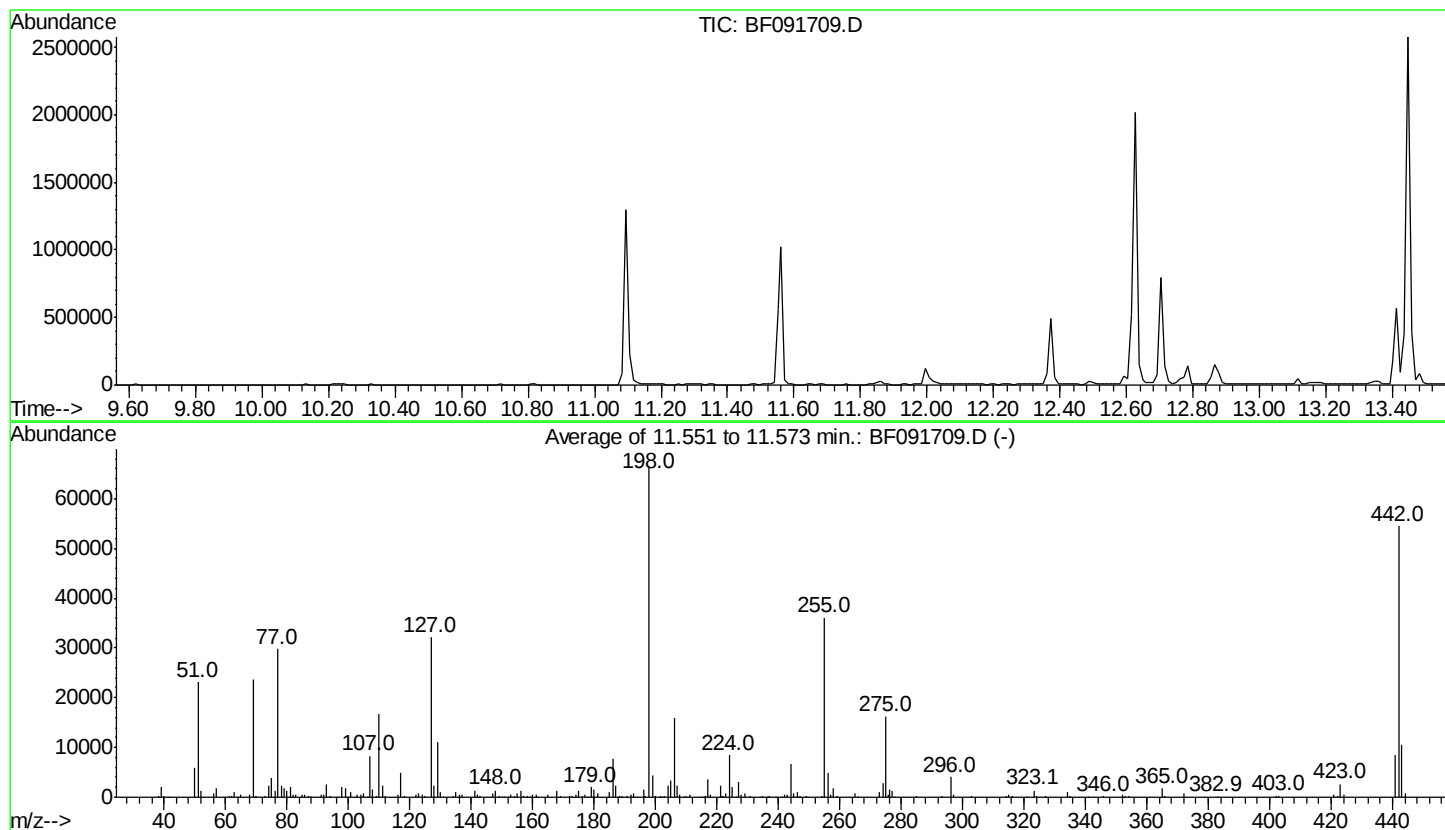

AutoFind: Scans 828, 829, 830; Background Corrected with Scan 824

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.6	23044	PASS
68	69	0.00	2	1.7	413	PASS
69	198	0.00	100	35.7	23780	PASS
70	69	0.00	2	1.1	269	PASS
127	198	10	80	48.2	32086	PASS
197	198	0.00	2	0.4	279	PASS
198	198	100	100	100.0	66629	PASS
199	198	5	9	6.5	4304	PASS
275	198	10	60	24.2	16153	PASS
365	198	1	100	2.6	1719	PASS
441	442	0.01	24	15.7	8582	PASS
442	198	50	100	81.8	54516	PASS
443	442	15	24	19.2	10447	PASS