
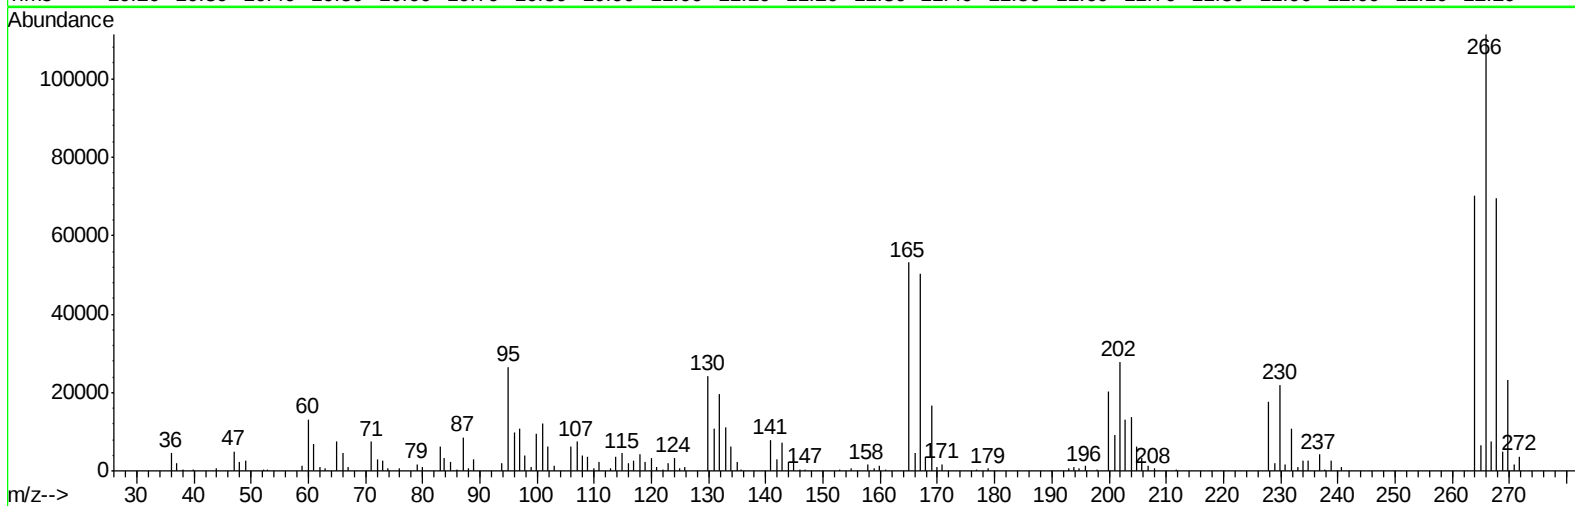


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF121719\
 Data File : BF118224.D
 Acq On : 17 Dec 2019 13:58
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 18 08:46:46 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF120619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 06 17:34:43 2019
 Response via : Initial Calibration

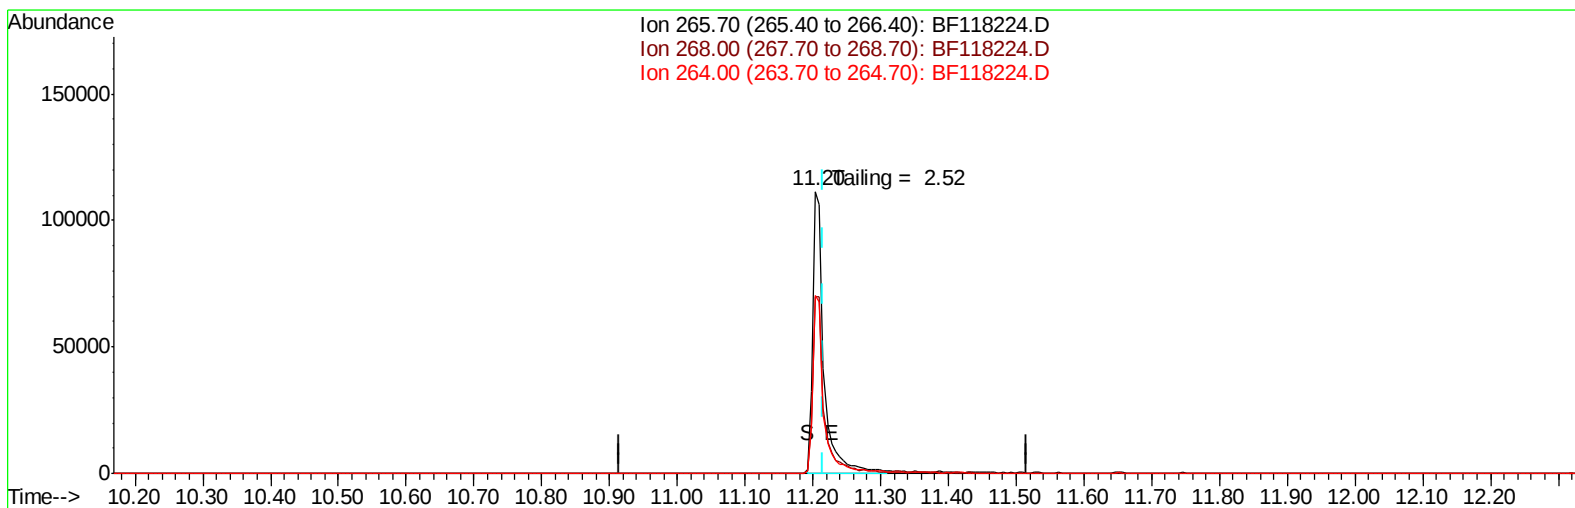

TIC: BF118224.D

(70) Pentachlorophenol (C)

11.204min (-0.012) 34421.55ng

response 130279

Ion	Exp%	Act%
265.70	100	100
268.00	63.40	62.58
264.00	60.90	63.04
0.00	0.00	0.00