
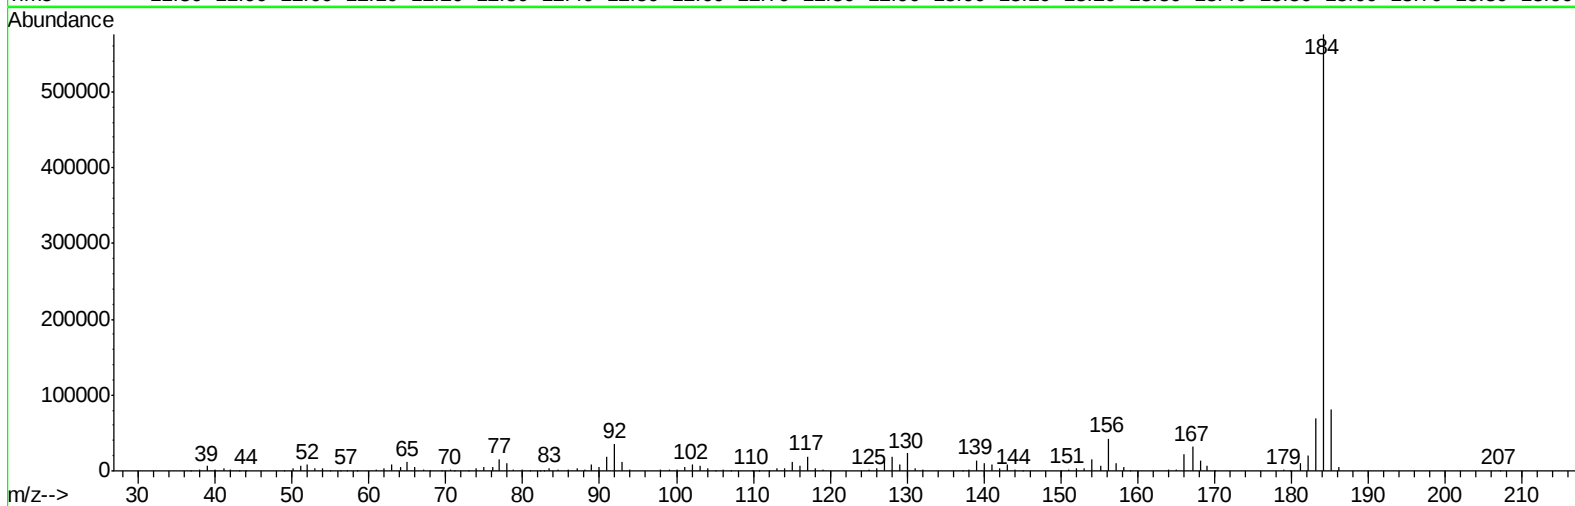


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF121719\
Data File : BF118224.D
Acq On : 17 Dec 2019 13:58
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 18 08:46:46 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF120619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 17:34:43 2019
Response via : Initial Calibration

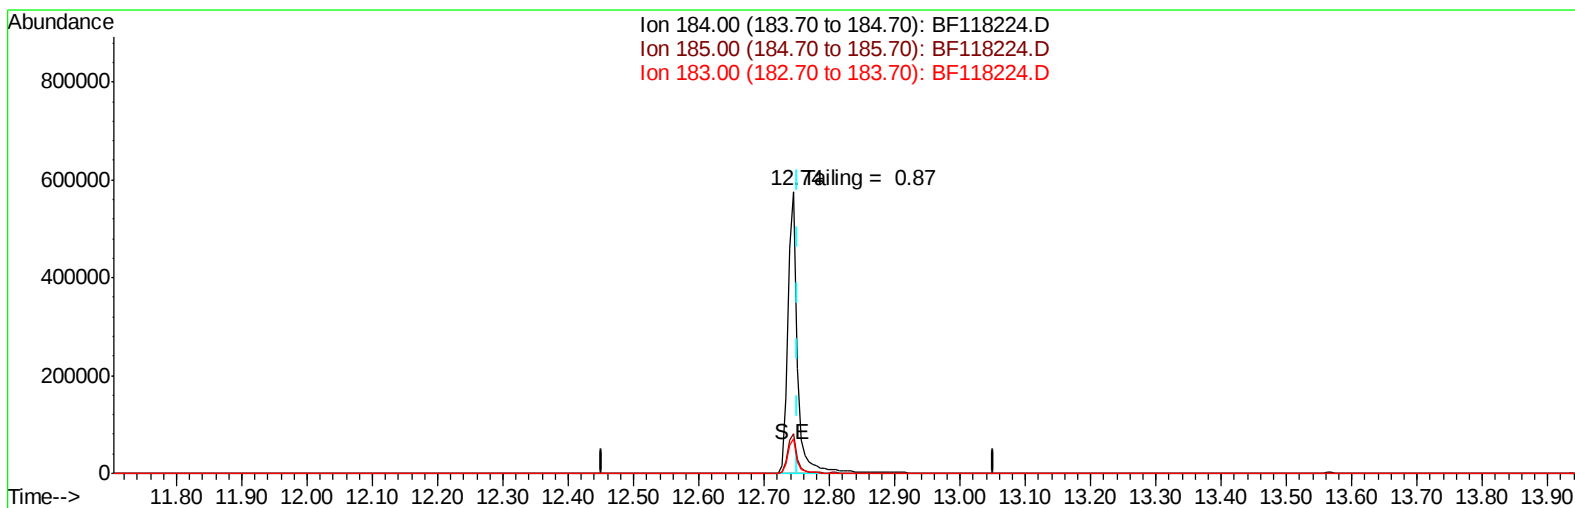

TIC: BF118224.D

(77) Benzidine

12.745min (-0.006) 0.00ng m

response 586154

Ion	Exp%	Act%
184.00	100	100
185.00	15.40	13.97
183.00	12.40	12.13
0.00	0.00	0.00