
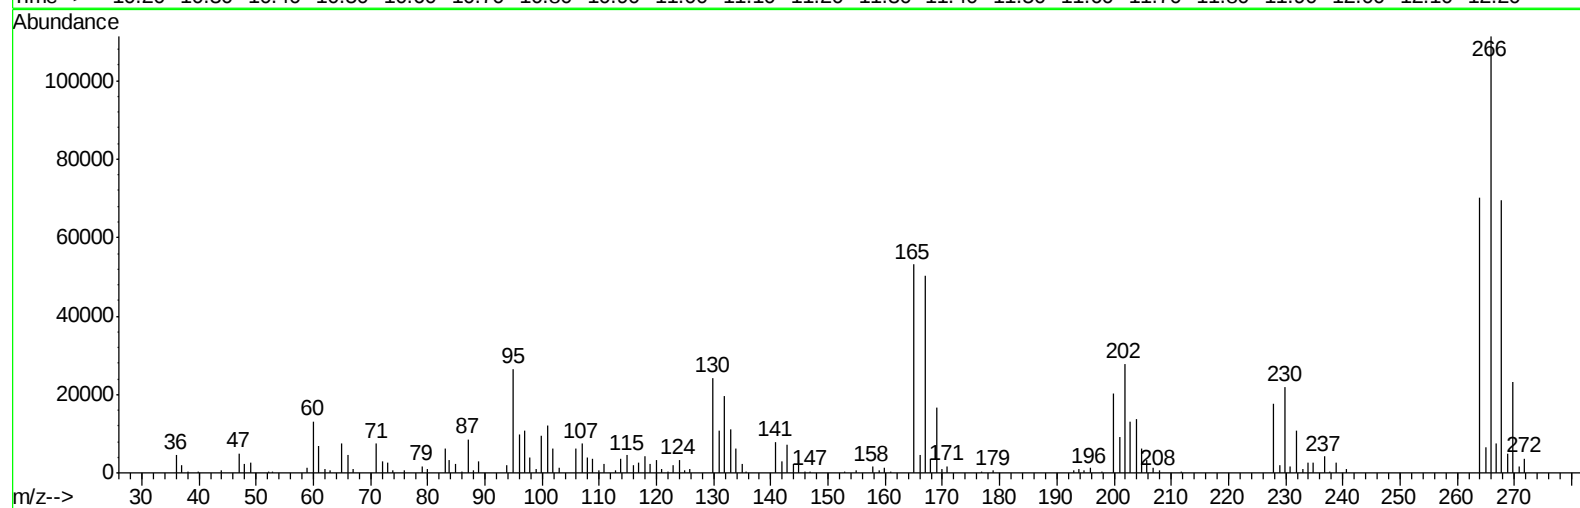


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF121719\  
Data File : BF118224.D  
Acq On : 17 Dec 2019 13:58  
Operator : JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 18 08:46:46 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF120619.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Dec 06 17:34:43 2019  
Response via : Initial Calibration

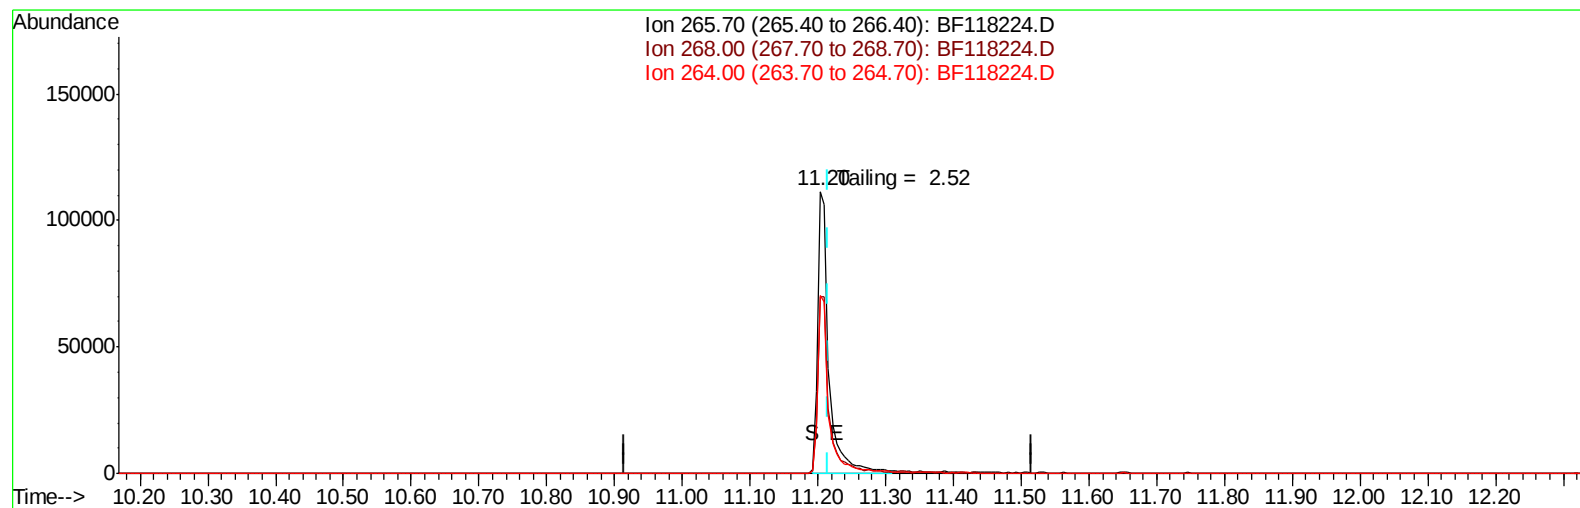

TIC: BF118224.D

(70) Pentachlorophenol (C)



11.204min (-0.012) 34421.55ng

response 130279

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.40 | 62.58 |
| 264.00 | 60.90 | 63.04 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF121719\  
Data File : BF118224.D  
Acq On : 17 Dec 2019 13:58  
Operator : JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 18 08:46:46 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF120619.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Dec 06 17:34:43 2019  
Response via : Initial Calibration

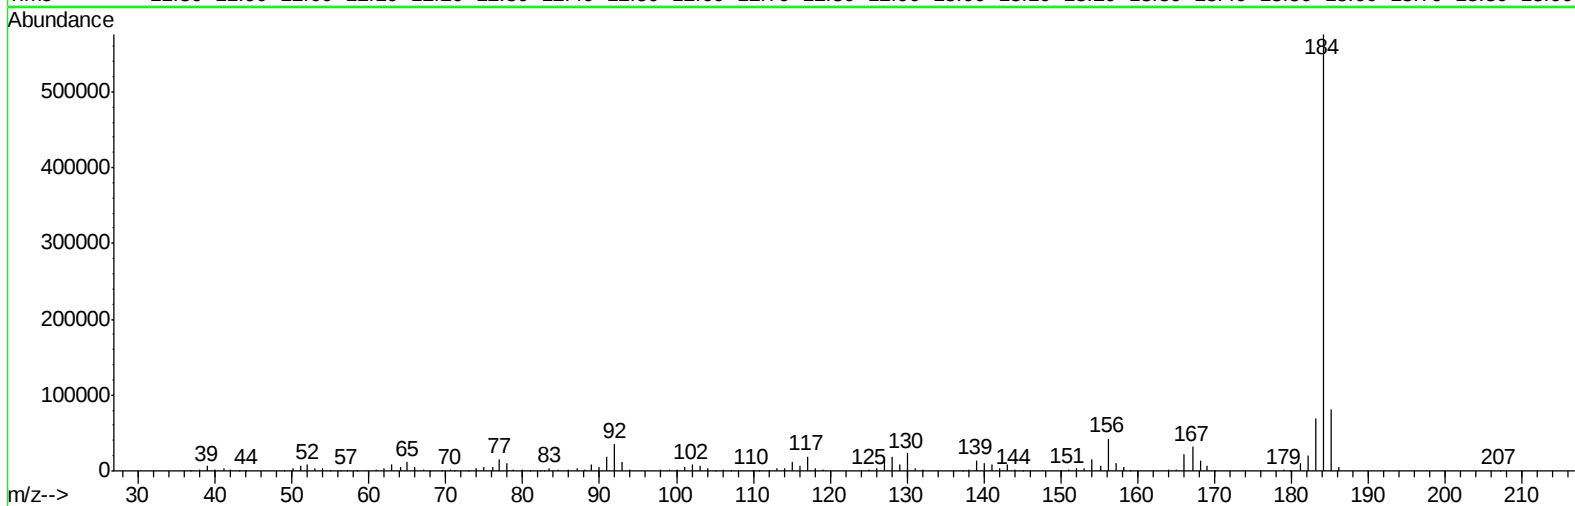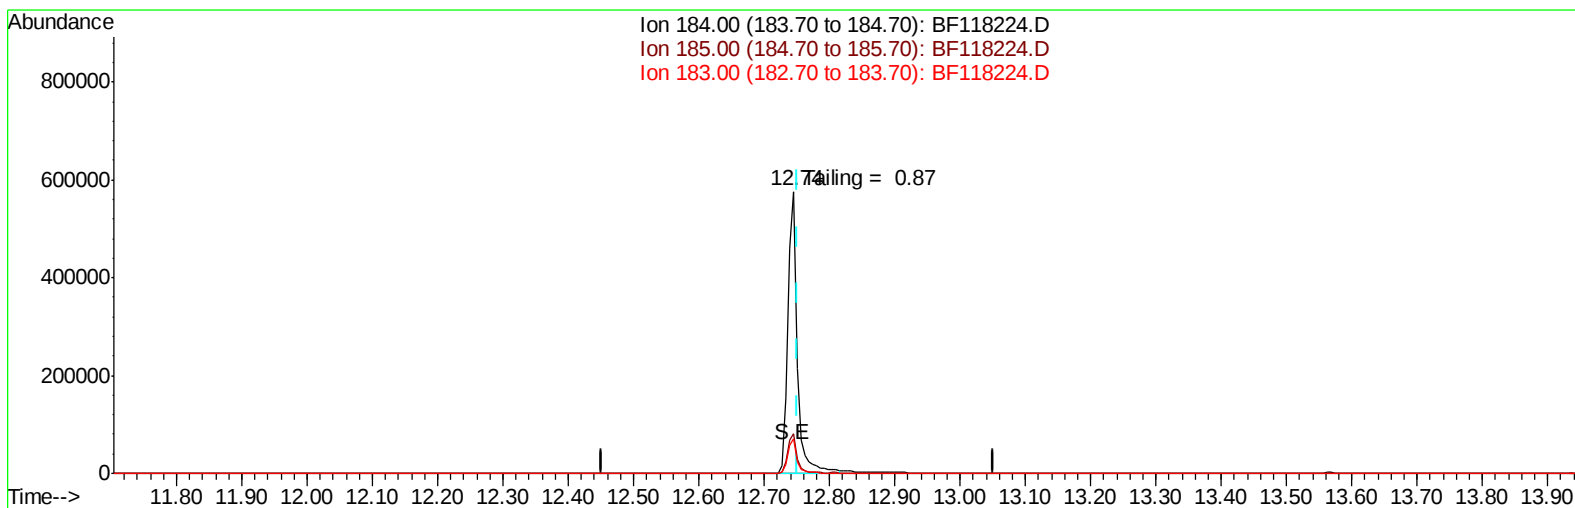

TIC: BF118224.D

(77) Benzidine

12.745min (-0.006) 0.00ng m

response 586154

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 15.40 | 13.97 |
| 183.00 | 12.40 | 12.13 |
| 0.00   | 0.00  | 0.00  |