


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF121719\
 Data File : BF118224.D
 Acq On : 17 Dec 2019 13:58
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 06 17:34:43 2019

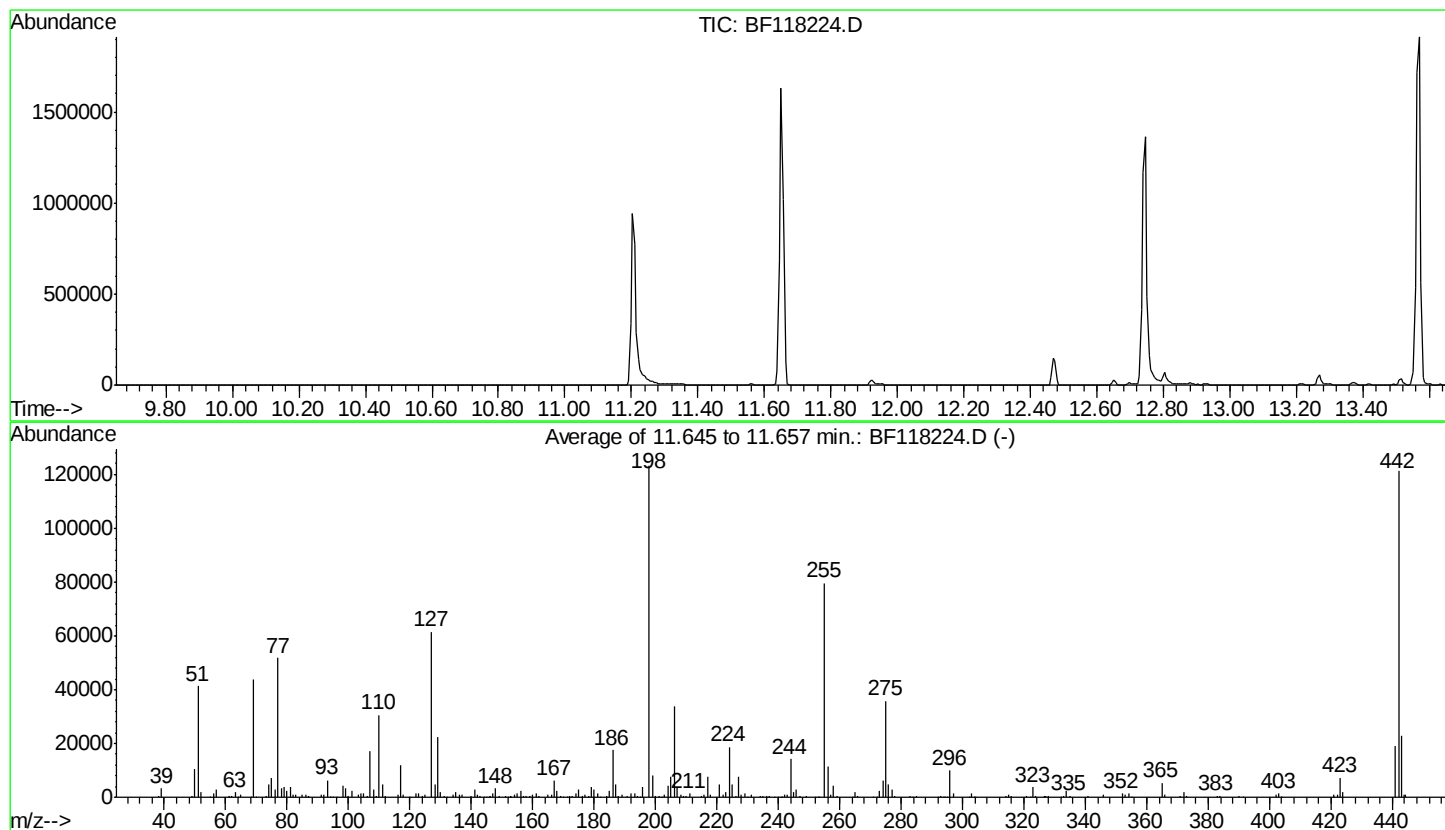

AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.6	41378	PASS
68	69	0.00	2	0.6	241	PASS
69	198	0.00	100	35.6	43816	PASS
70	69	0.00	2	0.3	126	PASS
127	198	10	80	50.0	61581	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	123242	PASS
199	198	5	9	6.8	8321	PASS
275	198	10	60	29.0	35797	PASS
365	198	1	100	4.3	5332	PASS
441	198	0.01	100	15.4	19031	PASS
442	198	50	100	98.3	121160	PASS
443	442	15	24	19.0	22988	PASS