
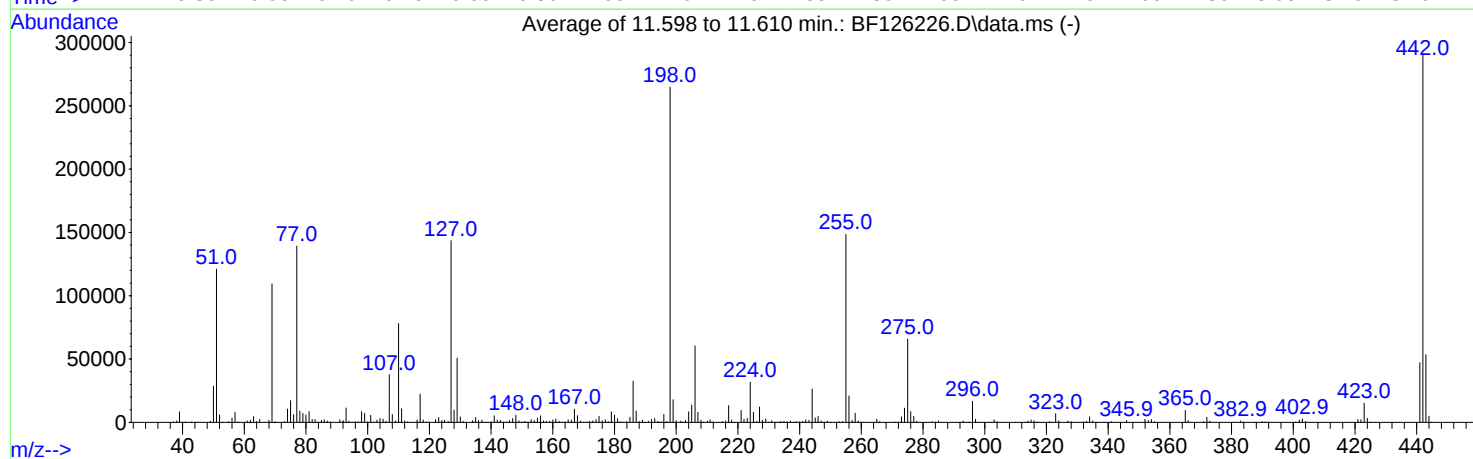


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121721\
 Data File : BF126226.D
 Acq On : 17 Dec 2021 9:31
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 16 12:22:48 2021



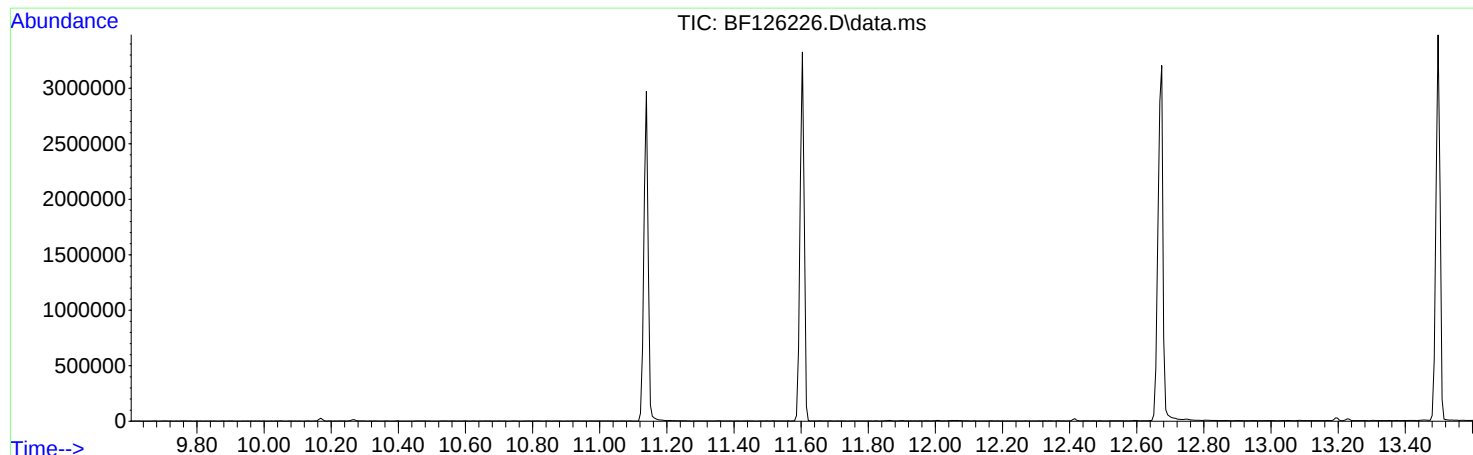


AutoFind: Scans 1617, 1618, 1619; Background Corrected with Scan 1612

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.7	120976	PASS
68	69	0.00	2	1.5	1614	PASS
69	198	0.00	100	41.3	109376	PASS
70	69	0.00	2	0.4	424	PASS
127	198	10	80	54.2	143600	PASS
197	198	0.00	2	0.2	590	PASS
198	198	100	100	100.0	264768	PASS
199	198	5	9	6.8	17935	PASS
275	198	10	60	24.9	65845	PASS
365	198	1	100	3.6	9542	PASS
441	198	0.01	100	17.8	47096	PASS
442	442	50	100	100.0	290517	PASS
443	442	15	24	18.4	53507	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121721\
 Data File : BF126226.D
 Acq On : 17 Dec 2021 9:31
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 17 12:26:12 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 16 12:22:48 2021
 Response via : Initial Calibration

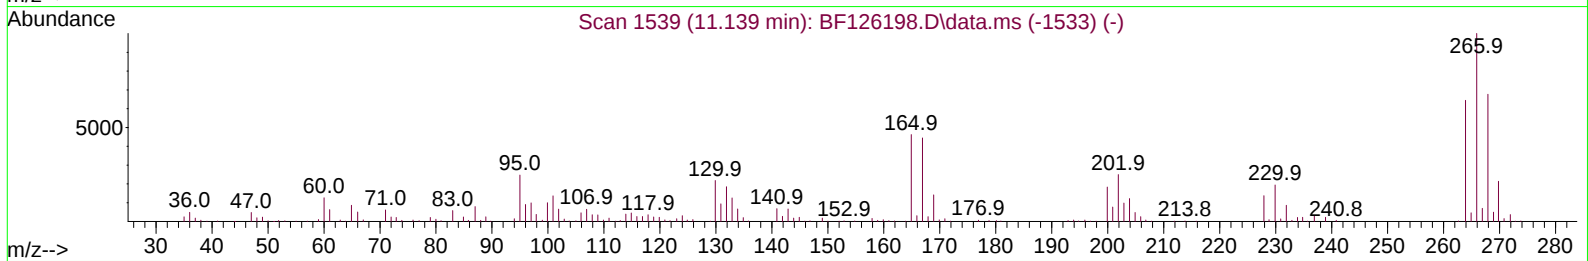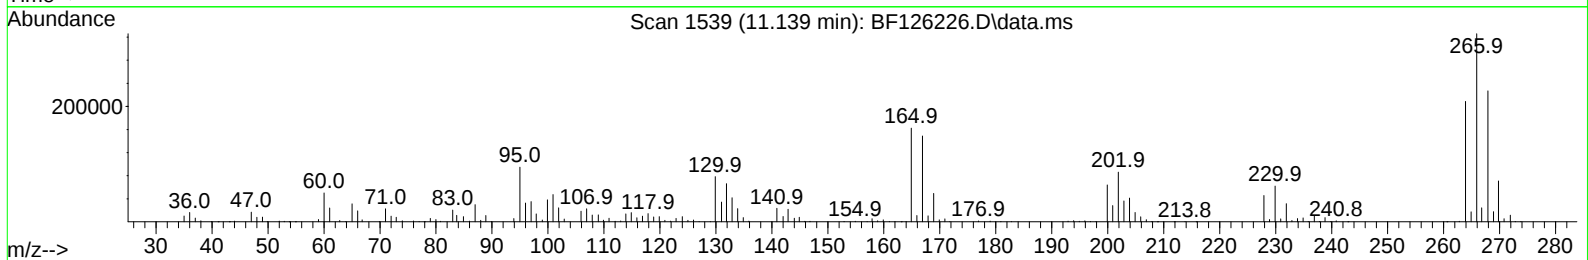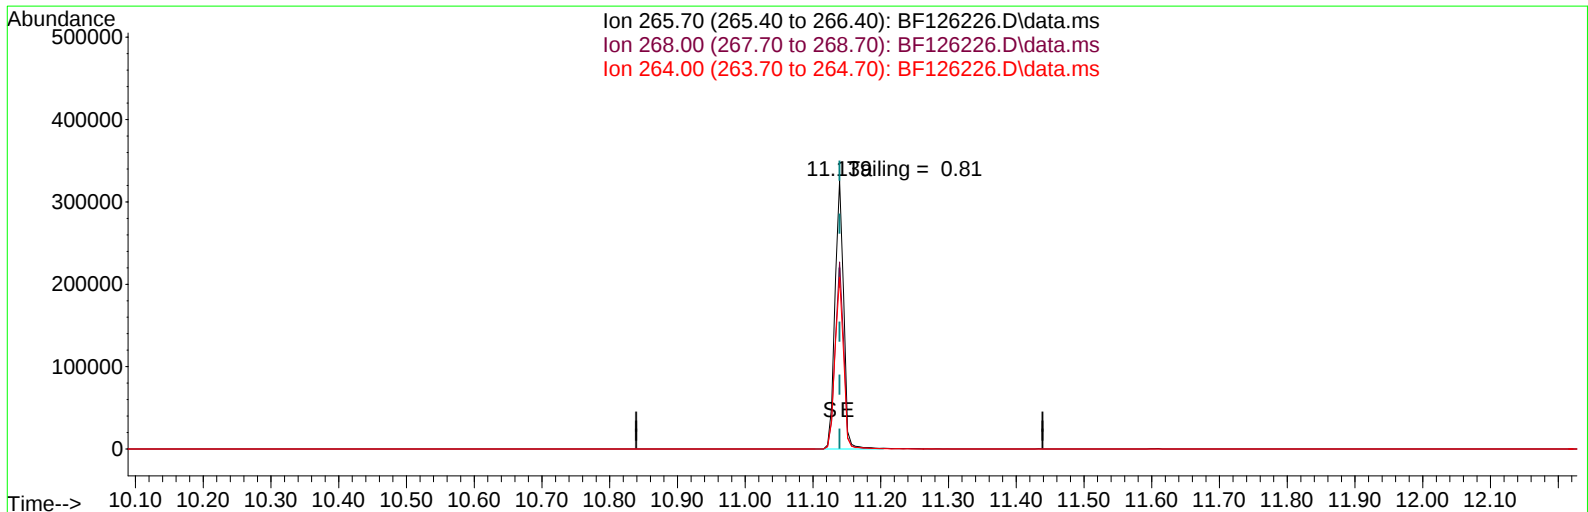

TIC: BF126226.D\data.ms

(70) Pentachlorophenol (C)




11.139min (+ 0.000) 312151.14 ng

response 289733

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	69.67
264.00	69.90	64.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121721\
Data File : BF126226.D
Acq On : 17 Dec 2021 9:31
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 17 12:26:12 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 16 12:22:48 2021
Response via : Initial Calibration

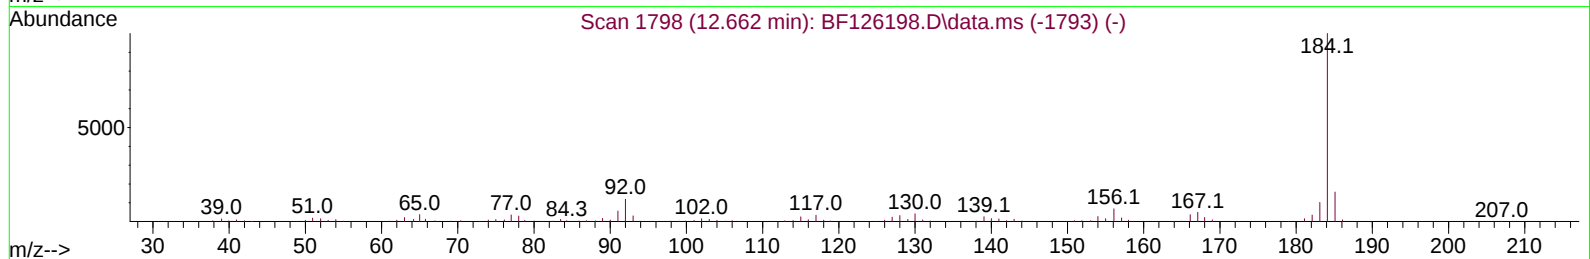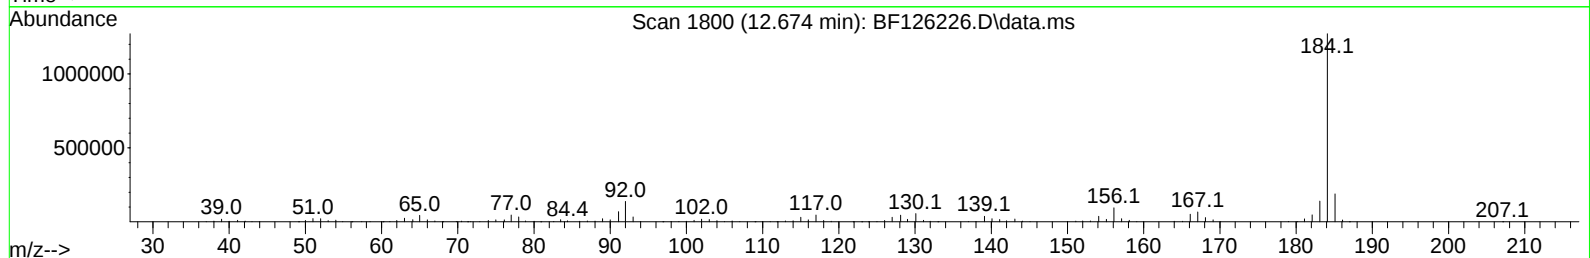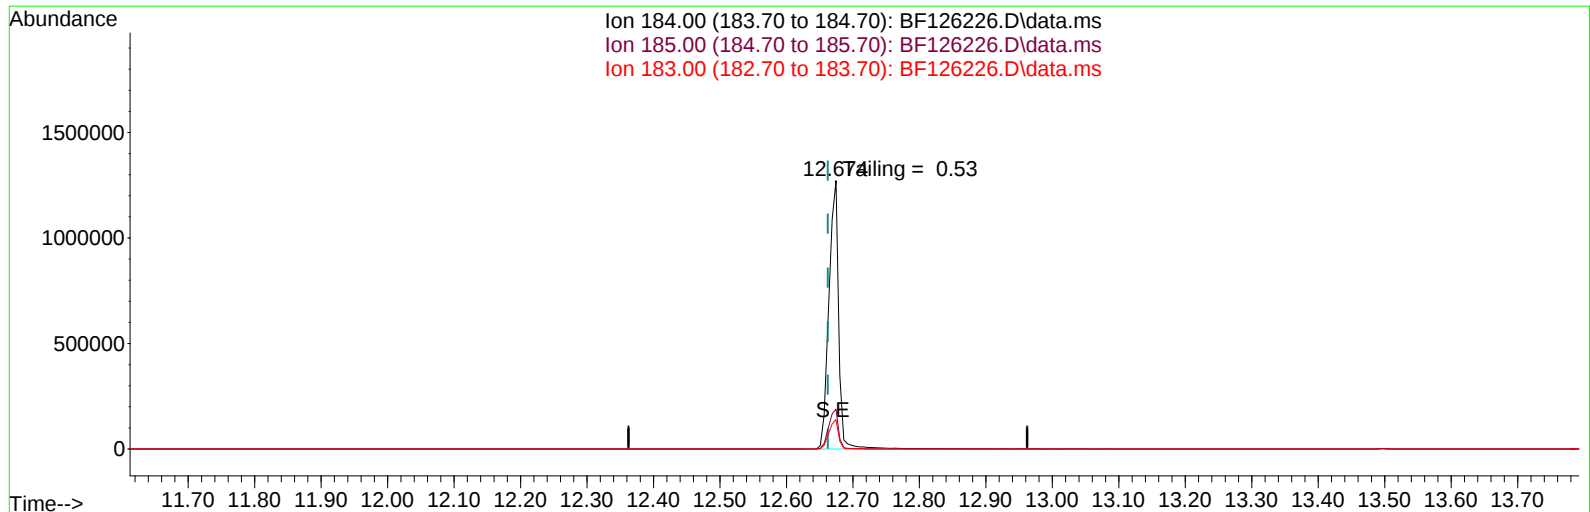

TIC: BF126226.D\data.ms

(77) Benzidine

12.674min (+ 0.012) 0.00 ng

response 1300782

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.88
183.00	10.10	10.99
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/17/2021	BNA_F	<u>BF126226.D</u>
Compound Name	Response	Retention Time
DDT	560252	13.49
DDD	4311	13.19
DDE	301	12.86
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4612	564864	0.82