

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121724\
 Data File : BF140890.D
 Acq On : 17 Dec 2024 17:22
 Operator : RC/JU
 Sample : P5279-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 ROCKAWAY-PARK

Quant Time: Dec 18 00:13:07 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 16 16:59:50 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.851	152	57445	20.000	ng	0.00
21) Naphthalene-d8	8.128	136	220060	20.000	ng	0.00
39) Acenaphthene-d10	9.881	164	113565	20.000	ng	0.00
64) Phenanthrene-d10	11.369	188	201340	20.000	ng	0.00
76) Chrysene-d12	14.022	240	178498	20.000	ng	-0.01
86) Perylene-d12	15.516	264	185951	20.000	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.493	112	214285	61.407	ng	0.00
7) Phenol-d6	6.498	99	291981	63.172	ng	0.00
23) Nitrobenzene-d5	7.410	82	212736	48.366	ng	0.00
42) 2,4,6-Tribromophenol	10.675	330	76347	56.842	ng	0.00
45) 2-Fluorobiphenyl	9.198	172	408390	49.441	ng	0.00
79) Terphenyl-d14	12.957	244	459185	40.565	ng	0.00
Target Compounds					Qvalue	
3) Pyridine	3.393	79	7087	2.036	ng	# 32
18) Hexachloroethane	7.345	117	5039	3.075	ng	# 9
19) n-Nitroso-di-n-propyla...	7.410	70	28693	10.349	ng	# 77
25) Isophorone	7.410	82	210161	28.516	ng	# 65
31) Naphthalene	8.151	128	39945	3.304	ng	98
49) Acenaphthylene	9.745	152	63054	6.211	ng	99
51) 2,6-Dinitrotoluene	9.881	165	16085	8.788	ng	# 28
52) Acenaphthene	9.916	154	23804	3.671	ng	99
54) 2,4-Dinitrophenol	9.816	184	114	6.658	ng	# 1
56) 4-Nitrophenol	10.039	139	323	4.754	ng	# 1
58) Fluorene	10.434	166	21092	2.544	ng	96
63) Azobenzene	10.592	77	17475	2.239	ng	# 1
67) 4-Bromophenyl-phenylether	10.675	248	4833	2.146	ng	# 1
71) Phenanthrene	11.398	178	219520	21.202	ng	99
72) Anthracene	11.451	178	46899	4.600	ng	98
75) Fluoranthene	12.592	202	342571	28.729	ng	99
78) Pyrene	12.822	202	446351	28.120	ng	99
81) Benzo(a)anthracene	14.016	228	248523	19.645	ng	97
83) Chrysene	14.051	228	178387	15.507	ng	98
87) Indeno(1,2,3-cd)pyrene	17.015	276	109571	9.442	ng	# 93
88) Benzo(b)fluoranthene	15.086	252	336911	26.101	ng	99
89) Benzo(k)fluoranthene	15.086	252	336911	30.428	ng	98
90) Benzo(a)pyrene	15.457	252	181398	17.947	ng	97
91) Dibenzo(a,h)anthracene	17.021	278	29335	3.051	ng	# 89
92) Benzo(g,h,i)perylene	17.474	276	105031	10.735	ng	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121724\
Data File : BF140890.D
Acq On : 17 Dec 2024 17:22
Operator : RC/JU
Sample : P5279-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
ROCKAWAY-PARK

Quant Time: Dec 18 00:13:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 16 16:59:50 2024
Response via : Initial Calibration




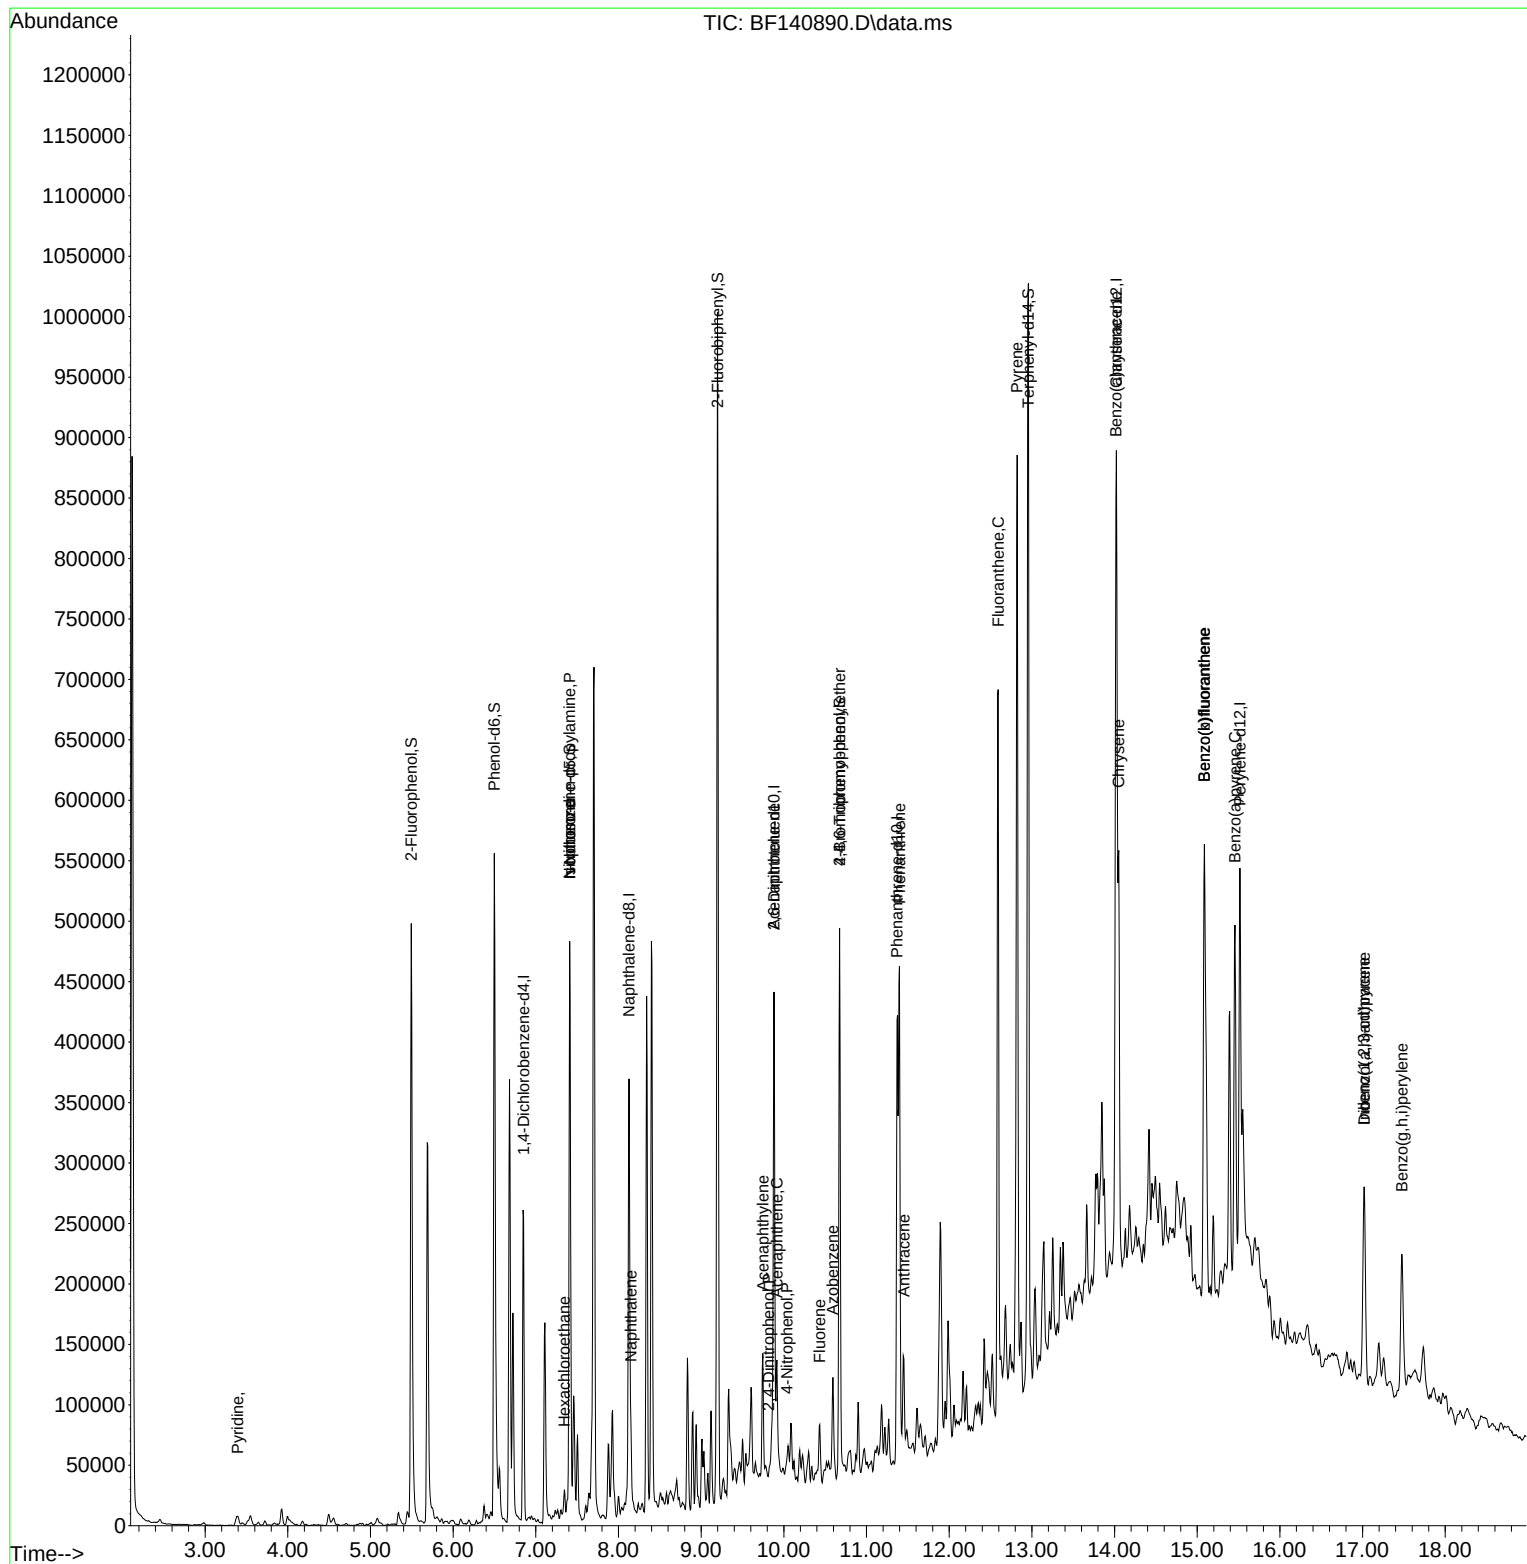




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.851 min Scan# 809
Delta R.T. 0.000 min
Lab File: BF140890.D
Acq: 17 Dec 2024 17:22




Instrument :
BNA_F
ClientSampleId :
ROCKAWAY-PARK


Tgt Ion:152 Resp: 57445
Ion Ratio Lower Upper
152 100
150 151.3 127.9 191.9
115 59.7 48.0 72.0

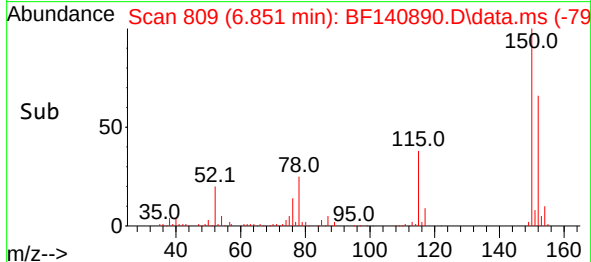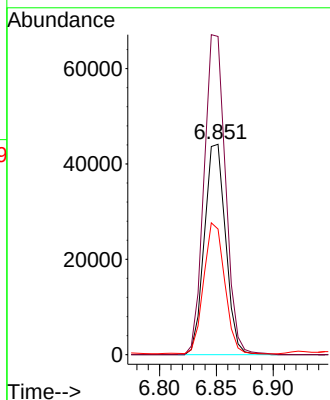

#3
Pyridine
Concen: 2.036 ng
RT: 3.393 min Scan# 221
Delta R.T. -0.012 min
Lab File: BF140890.D
Acq: 17 Dec 2024 17:22

Tgt Ion: 79 Resp: 7087
Ion Ratio Lower Upper
79 100
52 0.0 51.7 77.5#
51 11.0 28.2 42.4#


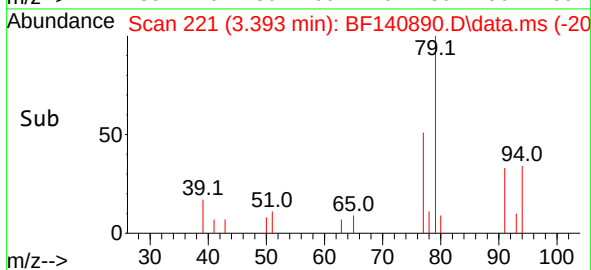
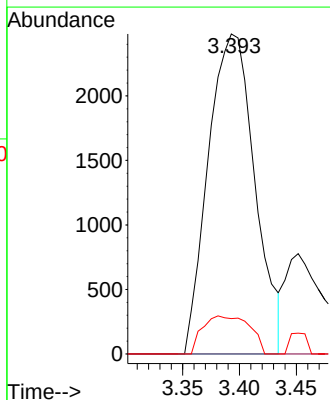





#5
2-Fluorophenol
Concen: 61.407 ng
RT: 5.493 min Scan# 51
Delta R.T. 0.006 min
Lab File: BF140890.D
Acq: 17 Dec 2024 17:22




Instrument :
BNA_F
ClientSampleId :
ROCKAWAY-PARK


Tgt Ion:112 Resp: 214285
Ion Ratio Lower Upper
112 100
64 58.9 46.1 69.1
63 31.5 24.9 37.3

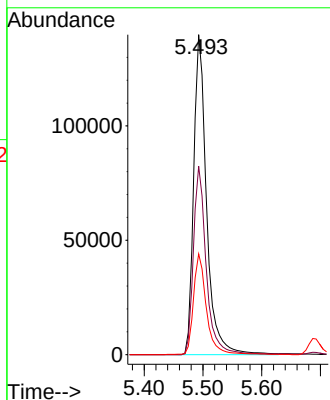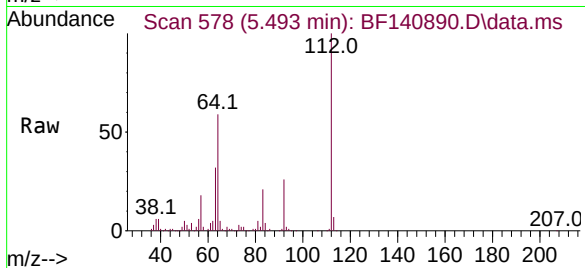

#7
Phenol-d6
Concen: 63.172 ng
RT: 6.498 min Scan# 749
Delta R.T. 0.000 min
Lab File: BF140890.D
Acq: 17 Dec 2024 17:22

Tgt Ion: 99 Resp: 291981
Ion Ratio Lower Upper
99 100
42 17.5 14.3 21.5
71 36.7 29.9 44.9


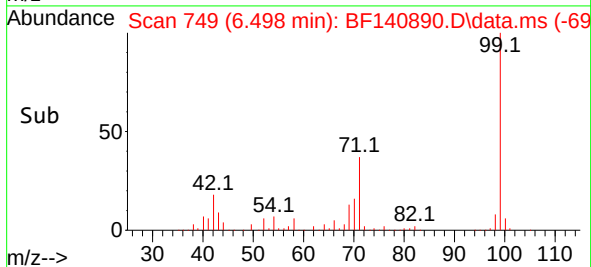
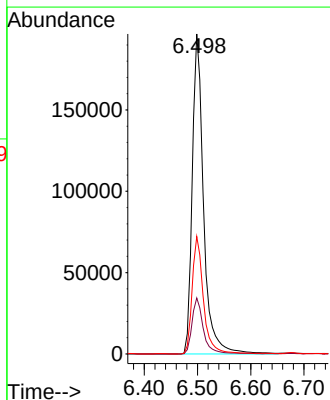
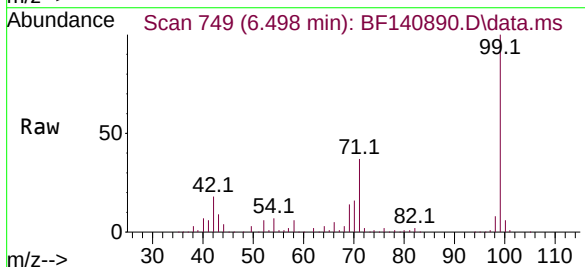




#18
Hexachloroethane
Concen: 3.075 ng
RT: 7.345 min Scan# 89
Delta R.T. -0.012 min
Lab File: BF140890.D
Acq: 17 Dec 2024 17:22




Instrument :
BNA_F
ClientSampleId :
ROCKAWAY-PARK


Tgt Ion:117 Resp: 5039
Ion Ratio Lower Upper
117 100
119 18.6 77.4 116.0#
201 0.0 83.4 125.0#

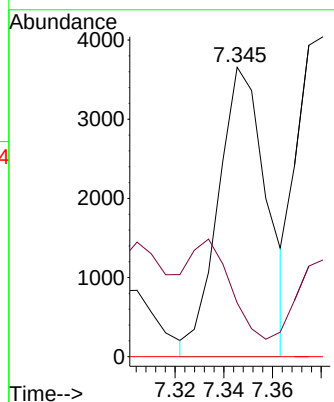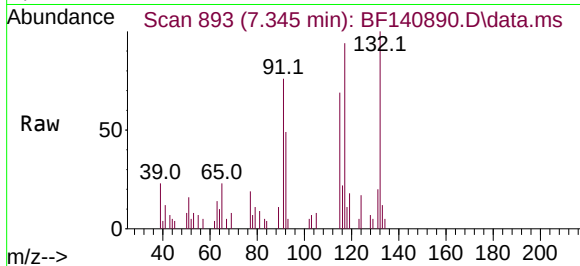

#19
n-Nitroso-di-n-propylamine
Concen: 10.349 ng
RT: 7.410 min Scan# 904
Delta R.T. 0.147 min
Lab File: BF140890.D
Acq: 17 Dec 2024 17:22

Tgt Ion: 70 Resp: 28693
Ion Ratio Lower Upper
70 100
42 44.7 45.3 67.9#
101 0.0 8.0 12.0#
130 2.6 16.9 25.3#


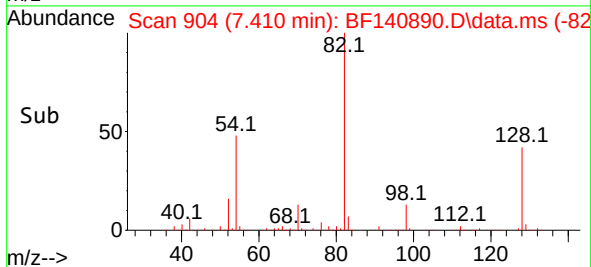
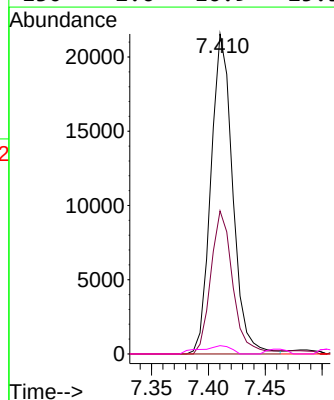
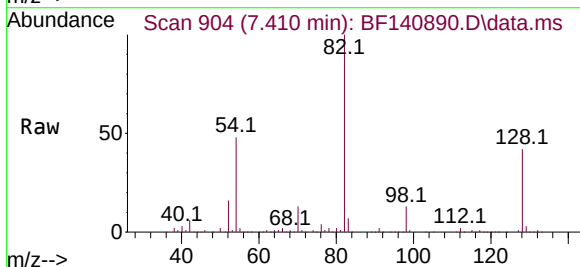




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.128 min Scan# 10
Delta R.T. 0.000 min
Lab File: BF140890.D
Acq: 17 Dec 2024 17:22




Instrument :
BNA_F
ClientSampleId :
ROCKAWAY-PARK


Tgt Ion:	136	Resp:	220060
Ion	Ratio	Lower	Upper
136	100		
137	10.9	9.0	13.4
54	6.4	5.6	8.4
68	5.1	4.2	6.2



#23
Nitrobenzene-d5
Concen: 48.366 ng
RT: 7.410 min Scan# 904
Delta R.T. -0.006 min
Lab File: BF140890.D
Acq: 17 Dec 2024 17:22

Tgt Ion:	82	Resp:	212736
Ion	Ratio	Lower	Upper
82	100		
128	41.7	34.4	51.6
54	47.6	38.8	58.2


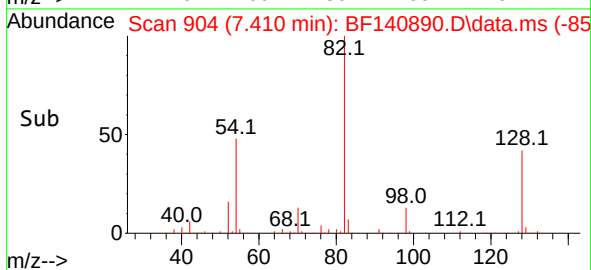






#25
Isophorone
Concen: 28.516 ng
RT: 7.410 min Scan# 90
Delta R.T. -0.265 min
Lab File: BF140890.D
Acq: 17 Dec 2024 17:22




Instrument :
BNA_F
ClientSampleId :
ROCKAWAY-PARK


Tgt Ion: 82 Resp: 210161
Ion Ratio Lower Upper
82 100
95 0.1 6.3 9.5#
138 0.0 14.1 21.1#

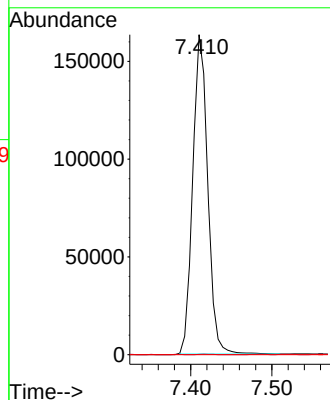

#31
Naphthalene
Concen: 3.304 ng
RT: 8.151 min Scan# 1030
Delta R.T. 0.000 min
Lab File: BF140890.D
Acq: 17 Dec 2024 17:22

Tgt Ion: 128 Resp: 39945
Ion Ratio Lower Upper
128 100
129 12.6 8.9 13.3
127 13.3 10.6 16.0


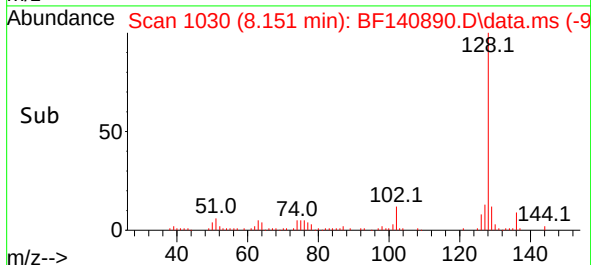
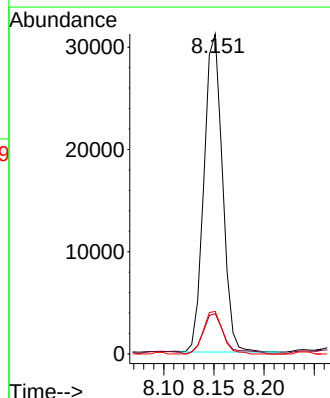
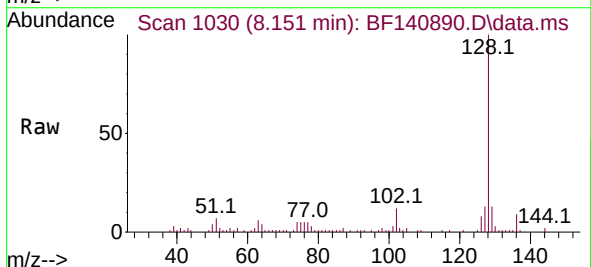




#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.881 min Scan# 11
Delta R.T. -0.006 min
Lab File: BF140890.D
Acq: 17 Dec 2024 17:22




Instrument :
BNA_F
ClientSampleId :
ROCKAWAY-PARK


Tgt Ion:164 Resp: 113565
Ion Ratio Lower Upper
164 100
162 101.4 79.9 119.9
160 44.2 35.2 52.8



#42
2,4,6-Tribromophenol
Concen: 56.842 ng
RT: 10.675 min Scan# 1459
Delta R.T. -0.006 min
Lab File: BF140890.D
Acq: 17 Dec 2024 17:22

Tgt Ion:330 Resp: 76347
Ion Ratio Lower Upper
330 100
332 97.4 76.2 114.4
141 34.1 24.9 37.3


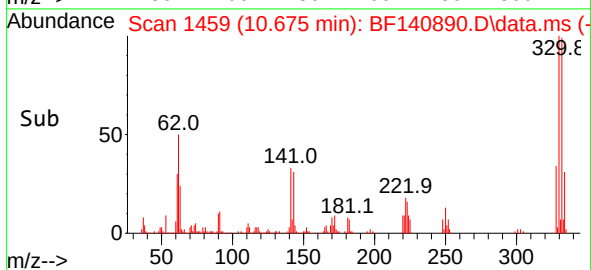

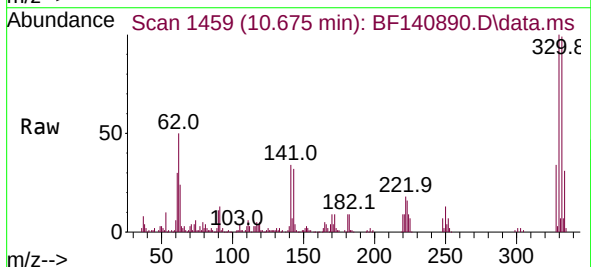




#45
2-Fluorobiphenyl
Concen: 49.441 ng
RT: 9.198 min Scan# 11
Delta R.T. -0.006 min
Lab File: BF140890.D
Acq: 17 Dec 2024 17:22




Instrument :
BNA_F
ClientSampleId :
ROCKAWAY-PARK


Tgt Ion:172 Resp: 408390
Ion Ratio Lower Upper
172 100
171 35.0 28.4 42.6
170 23.2 18.6 28.0

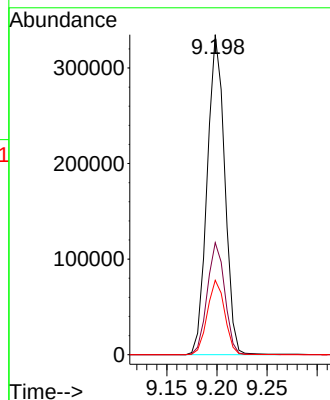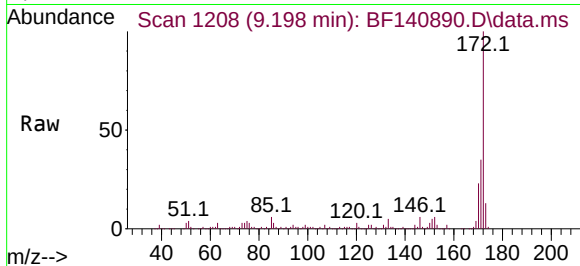

#49
Acenaphthylene
Concen: 6.211 ng
RT: 9.745 min Scan# 1301
Delta R.T. 0.000 min
Lab File: BF140890.D
Acq: 17 Dec 2024 17:22

Tgt Ion:152 Resp: 63054
Ion Ratio Lower Upper
152 100
151 19.7 16.0 24.0
153 13.0 10.6 16.0


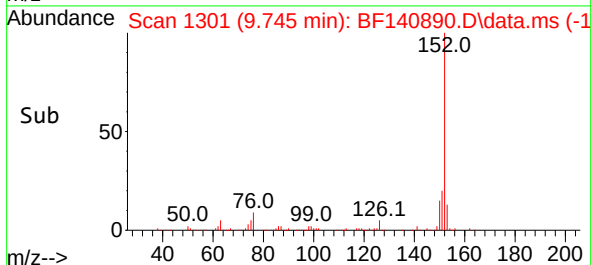
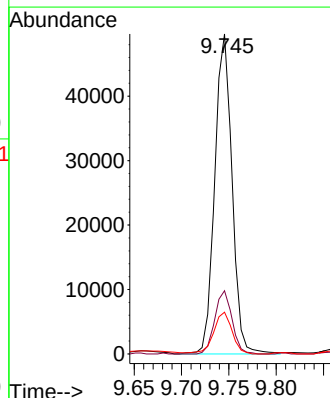
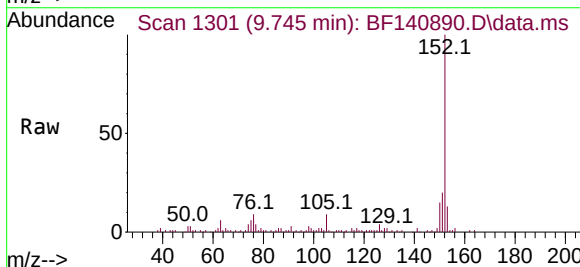




#51
2,6-Dinitrotoluene
Concen: 8.788 ng
RT: 9.881 min Scan# 11
Delta R.T. 0.206 min
Lab File: BF140890.D
Acq: 17 Dec 2024 17:22




Instrument :
BNA_F
ClientSampleId :
ROCKAWAY-PARK


Tgt Ion:165 Resp: 16085
Ion Ratio Lower Upper
165 100
63 6.2 49.7 74.5#
89 5.8 48.2 72.4#

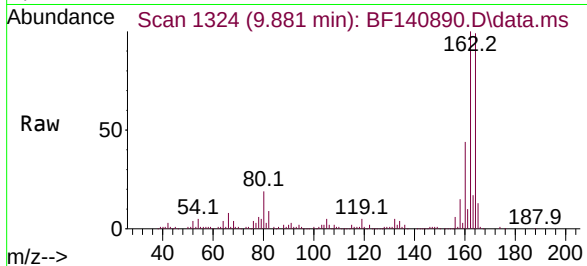

#52
Acenaphthene
Concen: 3.671 ng
RT: 9.916 min Scan# 1330
Delta R.T. 0.000 min
Lab File: BF140890.D
Acq: 17 Dec 2024 17:22

Tgt Ion:154 Resp: 23804
Ion Ratio Lower Upper
154 100
153 111.7 89.9 134.9
152 54.5 42.6 63.8


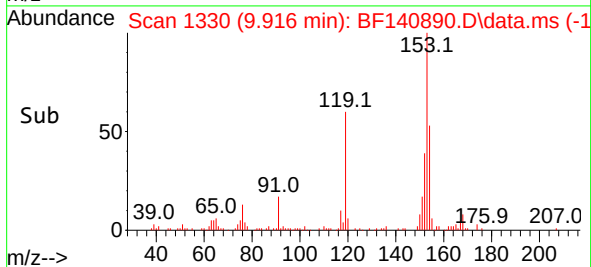

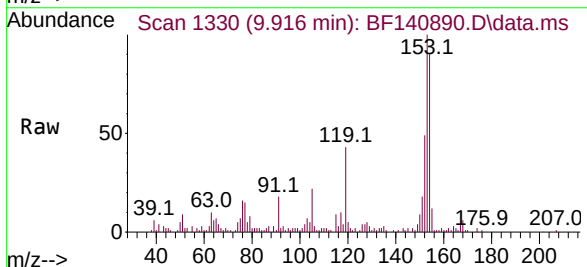




#54
2,4-Dinitrophenol
Concen: 6.658 ng
RT: 9.816 min Scan# 1114
Delta R.T. -0.153 min
Lab File: BF140890.D
Acq: 17 Dec 2024 17:22




Instrument :
BNA_F
ClientSampleId :
ROCKAWAY-PARK


Tgt Ion:184 Resp: 114
Ion Ratio Lower Upper
184 100
63 300.6 51.6 77.4#
154 0.0 56.1 84.1#

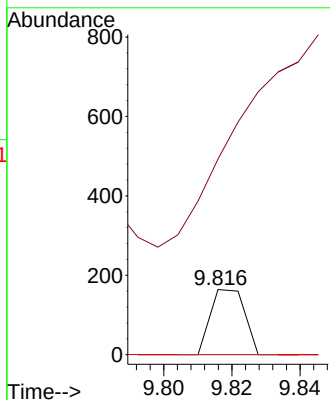

#56
4-Nitrophenol
Concen: 4.754 ng
RT: 10.039 min Scan# 1351
Delta R.T. 0.005 min
Lab File: BF140890.D
Acq: 17 Dec 2024 17:22

Tgt Ion:139 Resp: 323
Ion Ratio Lower Upper
139 100
109 82.9 56.7 96.7
65 463.5 78.1 118.1#

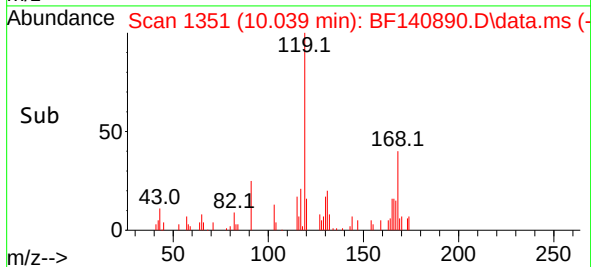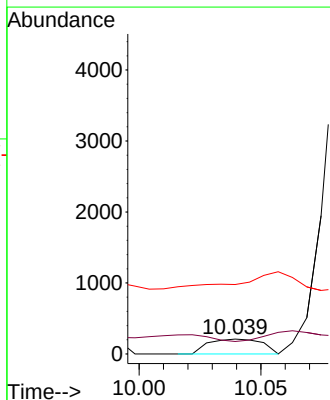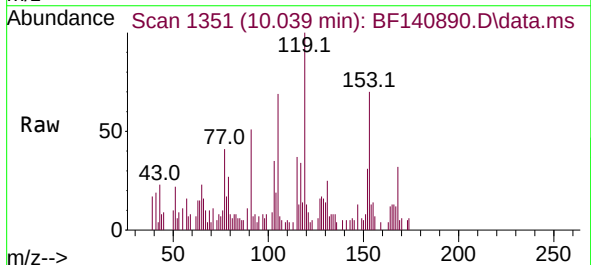



#58

Fluorene

Concen: 2.544 ng

RT: 10.434 min Scan# 1418

Delta R.T. 0.000 min

Lab File: BF140890.D

Acq: 17 Dec 2024 17:22

Instrument :

BNA_F

ClientSampleId :

ROCKAWAY-PARK





Tgt Ion:166 Resp: 21092

Ion Ratio Lower Upper

166 100

165 98.4 75.1 112.7

167 14.2 11.1 16.7

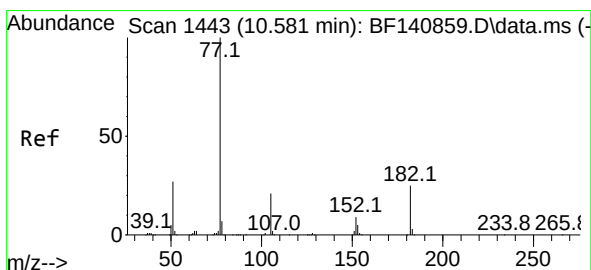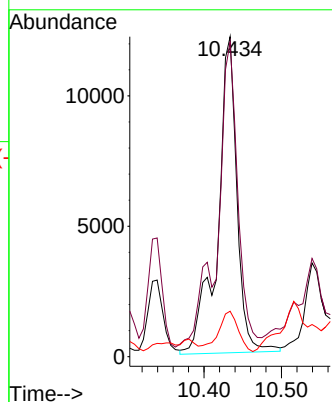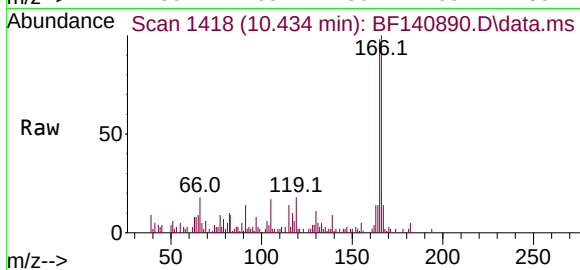

#63

Azobenzene

Concen: 2.239 ng

RT: 10.592 min Scan# 1445

Delta R.T. 0.012 min

Lab File: BF140890.D

Acq: 17 Dec 2024 17:22

Tgt Ion: 77 Resp: 17475




Ion Ratio Lower Upper


77 100

182 105.4 4.5 44.5#

105 153.8 0.9 40.9#

51 38.5 8.6 48.6

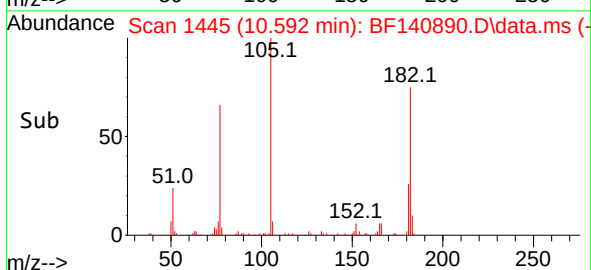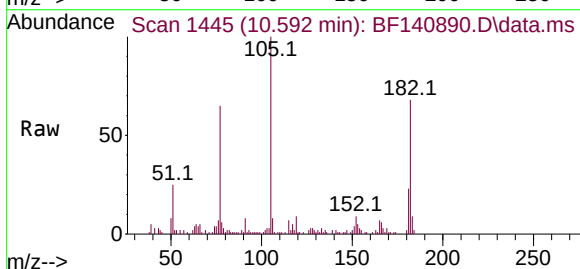



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.369 min Scan# 1

Delta R.T. -0.006 min

Lab File: BF140890.D

Acq: 17 Dec 2024 17:22

Instrument :

BNA_F

ClientSampleId :

ROCKAWAY-PARK





Tgt Ion:188 Resp: 201340

Ion Ratio Lower Upper

188 100

94 8.6 6.4 9.6

80 9.1 6.8 10.2



#67

4-Bromophenyl-phenylether

Concen: 2.146 ng

RT: 10.675 min Scan# 1459

Delta R.T. -0.235 min

Lab File: BF140890.D

Acq: 17 Dec 2024 17:22




Tgt Ion:248 Resp: 4833


Ion Ratio Lower Upper

248 100

250 185.5 77.4 116.2#

141 496.1 62.9 94.3#

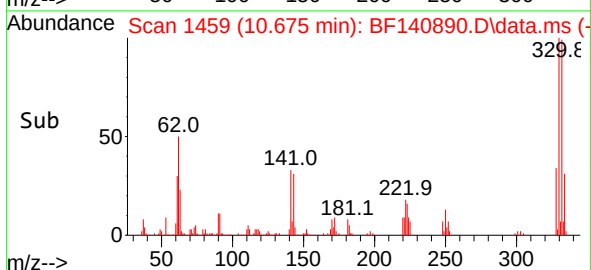

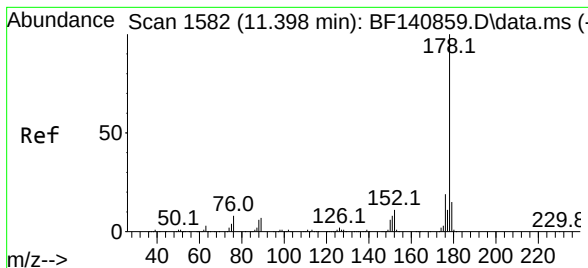

#71

Phenanthrene

Concen: 21.202 ng

RT: 11.398 min Scan# 1582

Delta R.T. 0.000 min

Lab File: BF140890.D

Acq: 17 Dec 2024 17:22

Instrument :

BNA_F

ClientSampleId :

ROCKAWAY-PARK





Tgt Ion:178 Resp: 219520

Ion Ratio Lower Upper

178 100

176 19.2 15.4 23.2

179 15.6 12.1 18.1

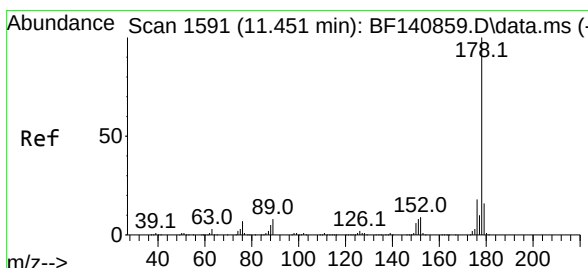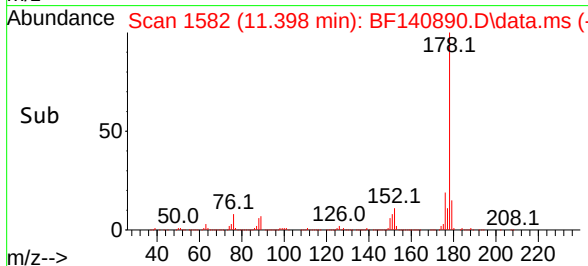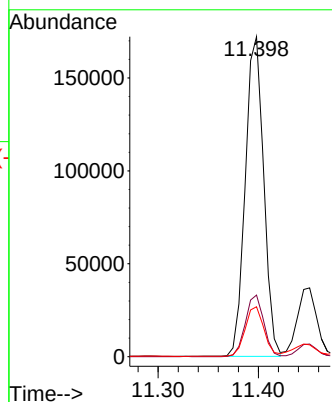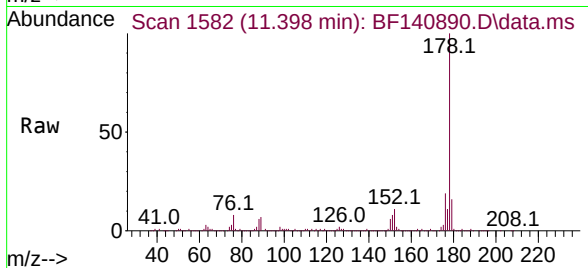

#72

Anthracene

Concen: 4.600 ng

RT: 11.451 min Scan# 1591

Delta R.T. 0.000 min

Lab File: BF140890.D

Acq: 17 Dec 2024 17:22




Tgt Ion:178 Resp: 46899


Ion Ratio Lower Upper

178 100

176 18.4 14.6 22.0

179 17.3 12.6 18.8


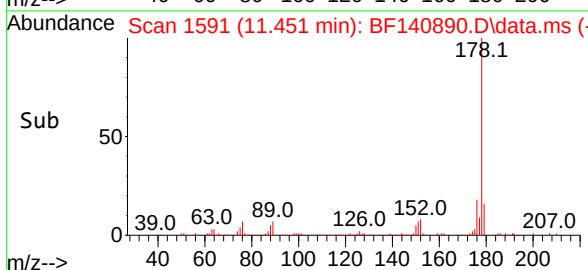

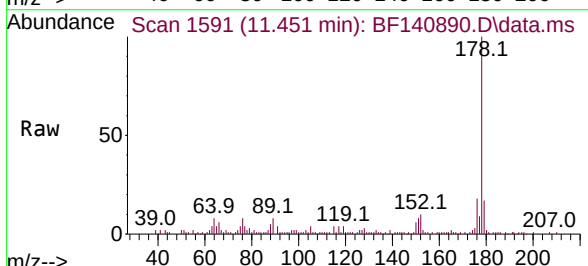




#75
Fluoranthene
Concen: 28.729 ng
RT: 12.592 min Scan# 11
Delta R.T. 0.000 min
Lab File: BF140890.D
Acq: 17 Dec 2024 17:22




Instrument :
BNA_F
ClientSampleId :
ROCKAWAY-PARK


Tgt Ion:202 Resp: 342571
Ion Ratio Lower Upper
202 100
101 8.6 0.0 29.3
203 17.3 0.0 37.4

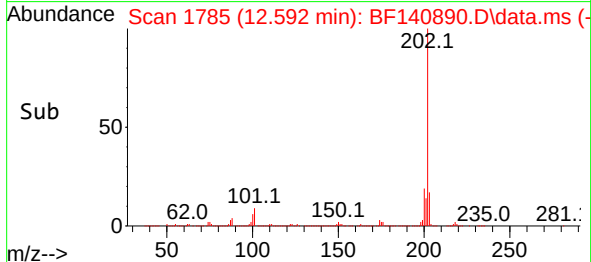

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.022 min Scan# 2028
Delta R.T. -0.012 min
Lab File: BF140890.D
Acq: 17 Dec 2024 17:22

Tgt Ion:240 Resp: 178498
Ion Ratio Lower Upper
240 100
120 10.1 7.6 11.4
236 25.4 20.5 30.7


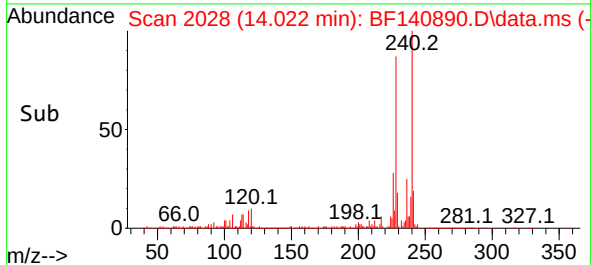

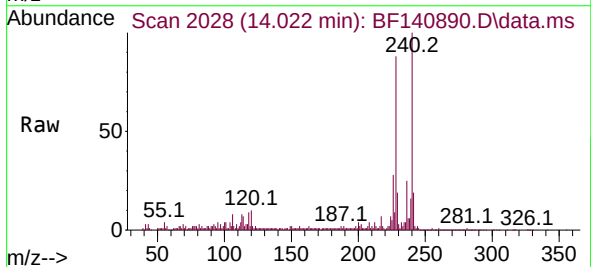




#78
Pyrene
Concen: 28.120 ng
RT: 12.822 min Scan# 1824
Delta R.T. 0.000 min
Lab File: BF140890.D
Acq: 17 Dec 2024 17:22




Instrument :
BNA_F
ClientSampleId :
ROCKAWAY-PARK


Tgt Ion:202 Resp: 446351
Ion Ratio Lower Upper
202 100
200 19.8 16.1 24.1
203 17.6 14.2 21.4

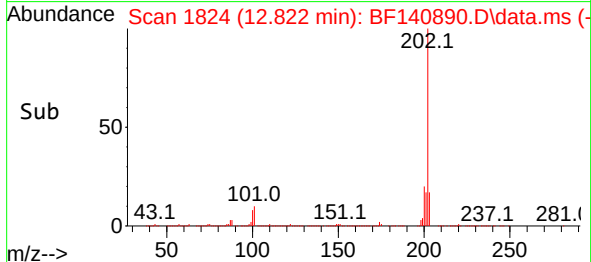

#79
Terphenyl-d14
Concen: 40.565 ng
RT: 12.957 min Scan# 1847
Delta R.T. 0.000 min
Lab File: BF140890.D
Acq: 17 Dec 2024 17:22

Tgt Ion:244 Resp: 459185
Ion Ratio Lower Upper
244 100
212 6.9 5.6 8.4
122 9.3 8.2 12.2

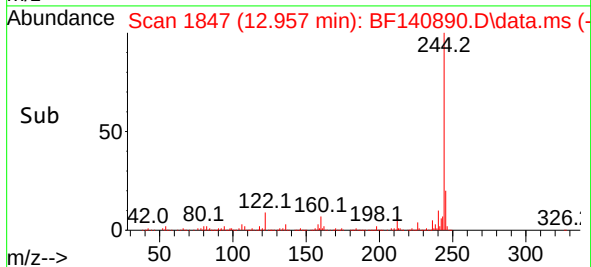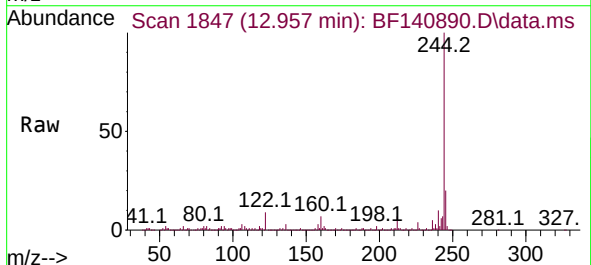



#81

Benzo(a)anthracene

Concen: 19.645 ng

RT: 14.016 min Scan# 2028

Delta R.T. -0.006 min

Lab File: BF140890.D

Acq: 17 Dec 2024 17:22

Instrument :

BNA_F

ClientSampleId :

ROCKAWAY-PARK





Tgt Ion:228 Resp: 248523

Ion Ratio Lower Upper

228 100

226 29.4 21.8 32.8

229 21.0 15.8 23.8

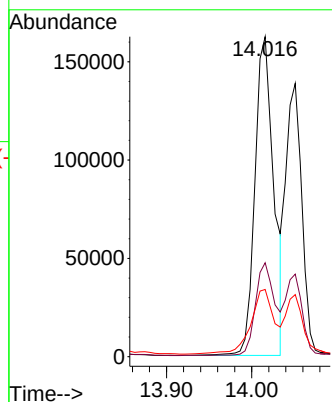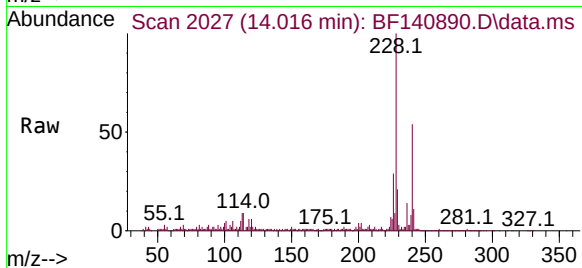

#83

Chrysene

Concen: 15.507 ng

RT: 14.051 min Scan# 2033

Delta R.T. -0.012 min

Lab File: BF140890.D

Acq: 17 Dec 2024 17:22




Tgt Ion:228 Resp: 178387


Ion Ratio Lower Upper

228 100

226 30.2 24.1 36.1

229 22.7 16.0 24.0

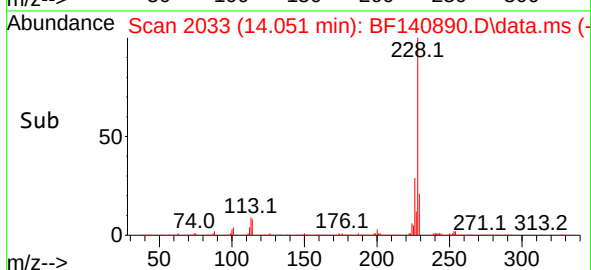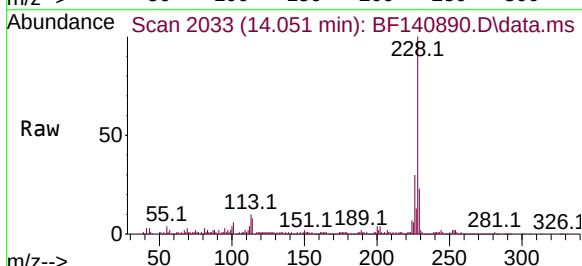



#86

Perylene-d12

Concen: 20.000 ng

RT: 15.516 min Scan# 21

Delta R.T. -0.029 min

Lab File: BF140890.D

Acq: 17 Dec 2024 17:22

Instrument :

BNA_F

ClientSampleId :

ROCKAWAY-PARK





Tgt Ion:264 Resp: 185951

Ion Ratio Lower Upper

264 100

260 24.4 19.1 28.7

265 22.6 17.0 25.4

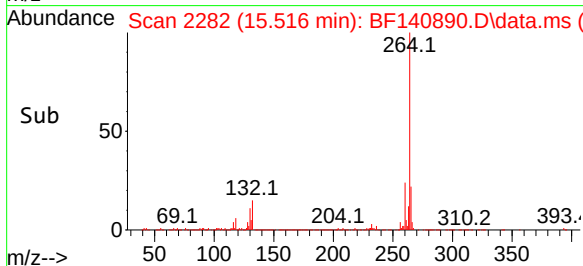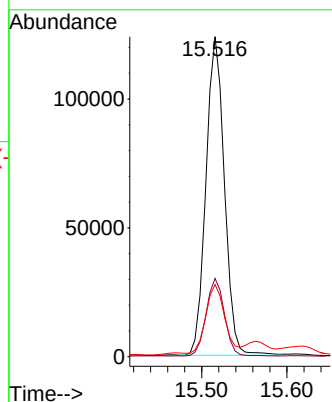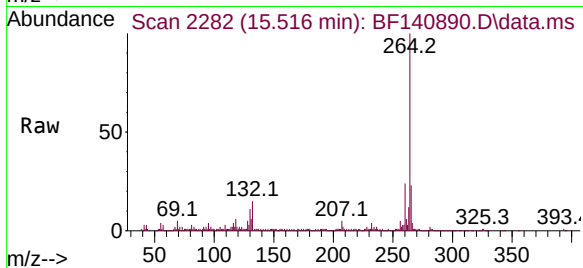

#87

Indeno(1,2,3-cd)pyrene

Concen: 9.442 ng

RT: 17.015 min Scan# 2537

Delta R.T. -0.035 min

Lab File: BF140890.D

Acq: 17 Dec 2024 17:22




Tgt Ion:276 Resp: 109571


Ion Ratio Lower Upper

276 100

138 16.7 16.9 25.3#

277 23.2 20.2 30.4


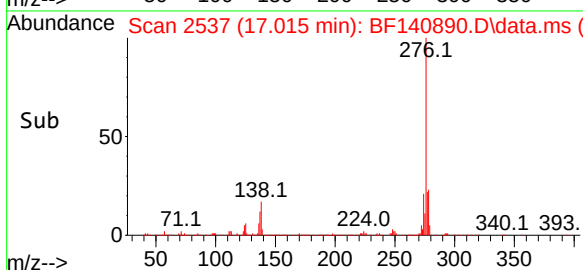

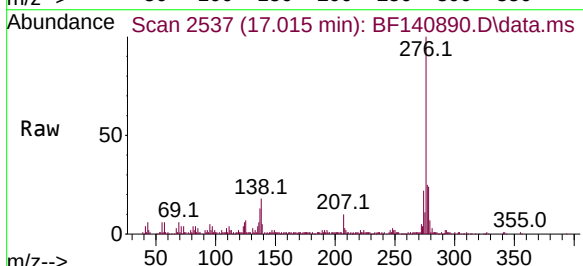




#88
Benzo(b)fluoranthene
Concen: 26.101 ng
RT: 15.086 min Scan# 21
Delta R.T. -0.024 min
Lab File: BF140890.D
Acq: 17 Dec 2024 17:22




Instrument :
BNA_F
ClientSampleId :
ROCKAWAY-PARK


Tgt Ion:252 Resp: 336911
Ion Ratio Lower Upper
252 100
253 22.3 17.8 26.6
125 9.8 7.0 10.4

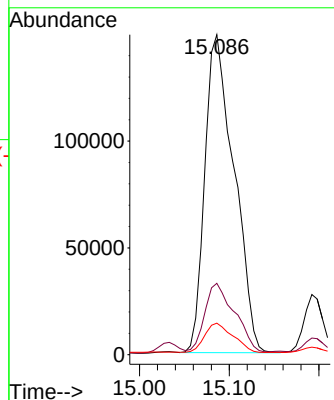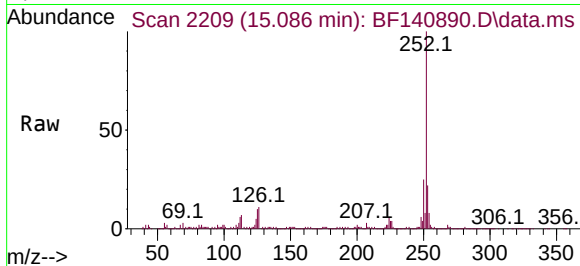

#89
Benzo(k)fluoranthene
Concen: 30.428 ng
RT: 15.086 min Scan# 2209
Delta R.T. -0.053 min
Lab File: BF140890.D
Acq: 17 Dec 2024 17:22

Tgt Ion:252 Resp: 336911
Ion Ratio Lower Upper
252 100
253 22.3 17.5 26.3
125 9.8 6.8 10.2


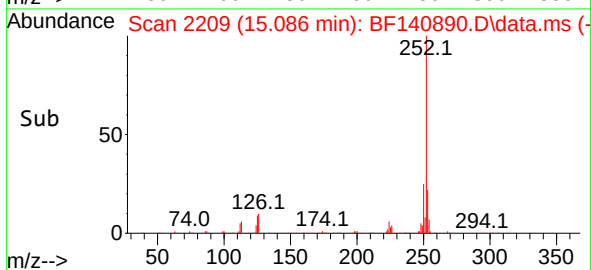
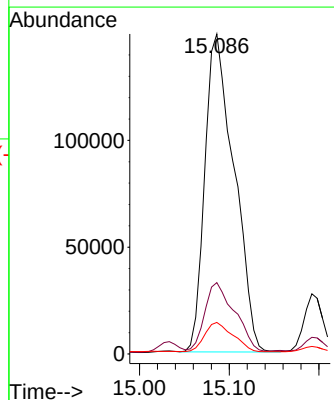
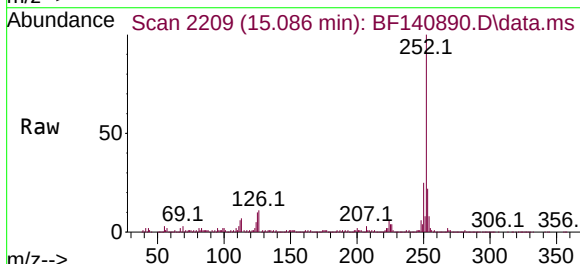




#90
Benzo(a)pyrene
Concen: 17.947 ng
RT: 15.457 min Scan# 21
Delta R.T. -0.023 min
Lab File: BF140890.D
Acq: 17 Dec 2024 17:22




Instrument :
BNA_F
ClientSampleId :
ROCKAWAY-PARK


Tgt Ion:252 Resp: 181398
Ion Ratio Lower Upper
252 100
253 23.5 17.5 26.3
125 9.8 7.5 11.3

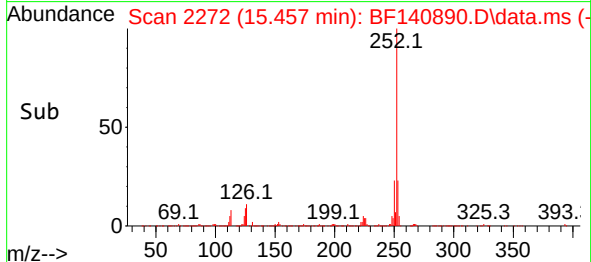

#91
Dibenzo(a,h)anthracene
Concen: 3.051 ng
RT: 17.021 min Scan# 2538
Delta R.T. -0.035 min
Lab File: BF140890.D
Acq: 17 Dec 2024 17:22

Tgt Ion:278 Resp: 29335
Ion Ratio Lower Upper
278 100
139 19.2 10.6 16.0#
279 28.4 19.2 28.8

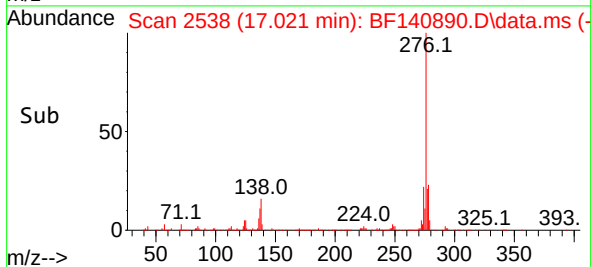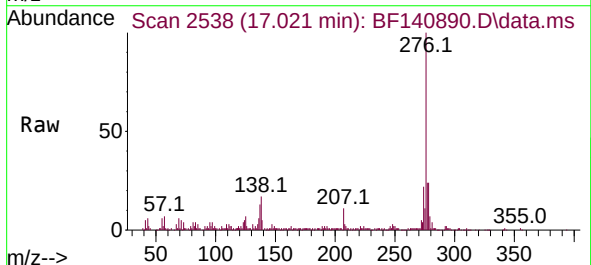



#92
 Benzo(g,h,i)perylene
 Concen: 10.735 ng
 RT: 17.474 min Scan# 20
 Delta R.T. -0.029 min
 Lab File: BF140890.D
 Acq: 17 Dec 2024 17:22

Instrument :
 BNA_F
 ClientSampleId :
 ROCKAWAY-PARK

Tgt Ion:276 Resp: 105031
 Ion Ratio Lower Upper
 276 100
 277 24.8 18.7 28.1
 138 18.8 14.2 21.2

