
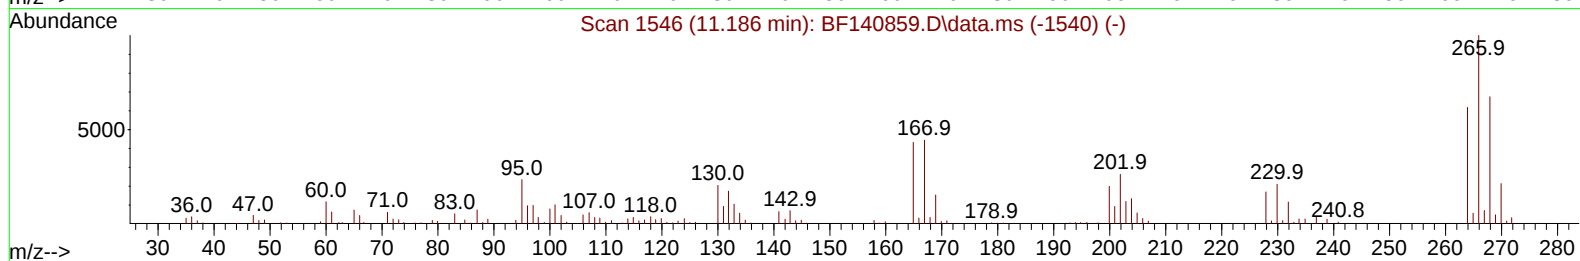
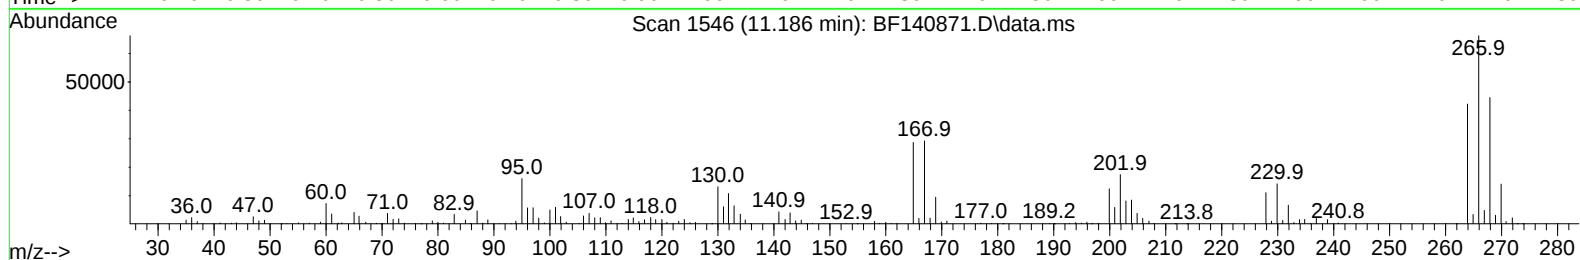


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121724\
Data File : BF140871.D
Acq On : 17 Dec 2024 08:58
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 17 10:34:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 16 16:59:50 2024
Response via : Initial Calibration

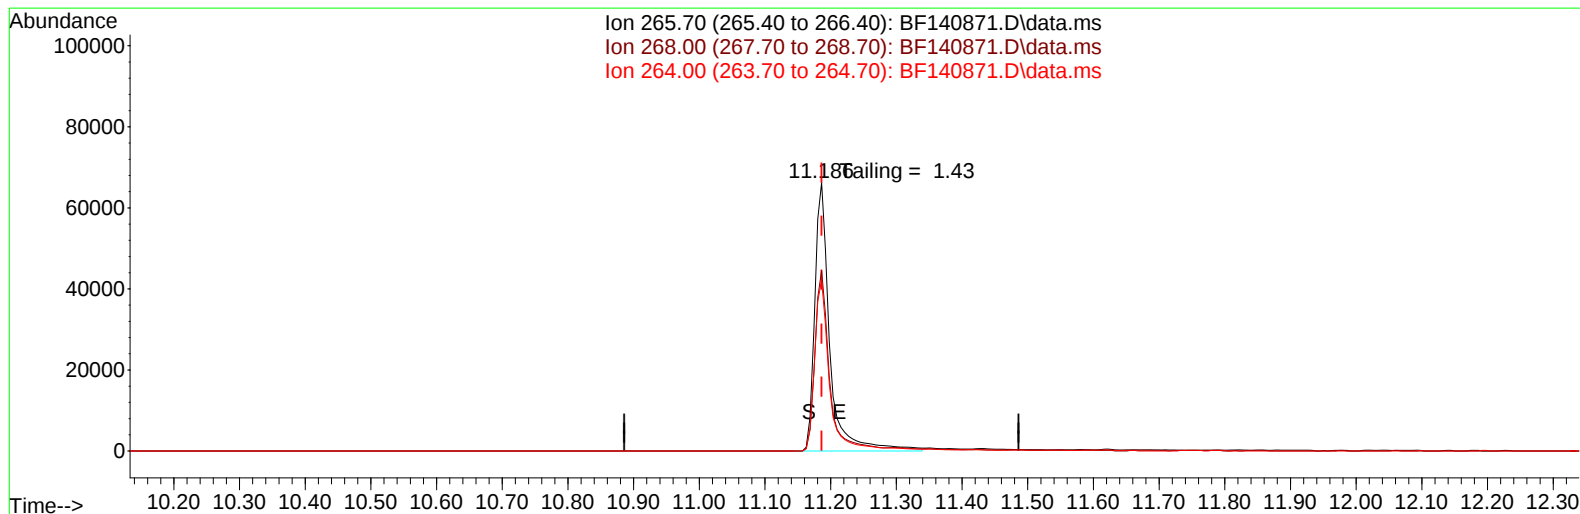

TIC: BF140871.D\data.ms

(70) Pentachlorophenol (C)




11.186min (+ 0.000) 4762.31 ng m

response 106624

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.50	67.21
264.00	61.80	63.75
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121724\
Data File : BF140871.D
Acq On : 17 Dec 2024 08:58
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 17 10:34:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 16 16:59:50 2024
Response via : Initial Calibration

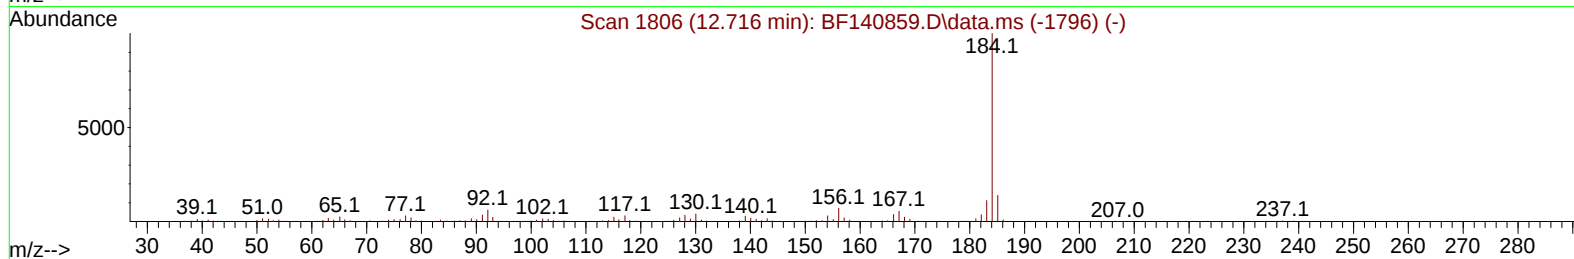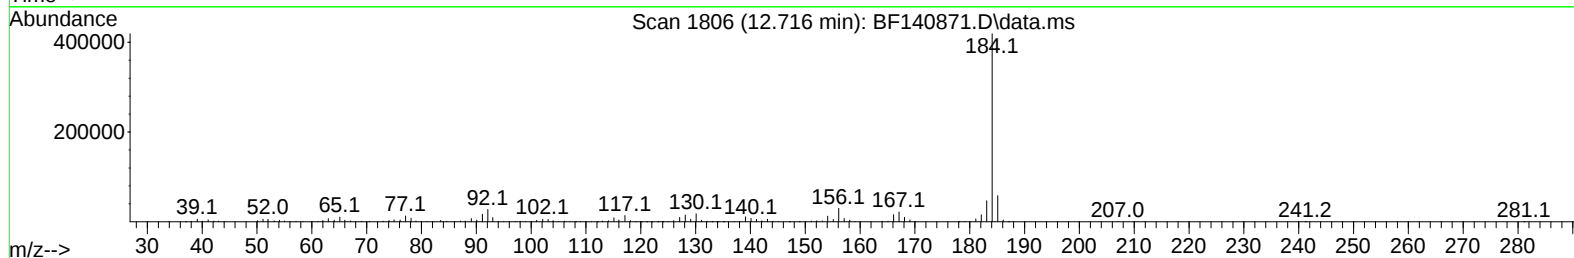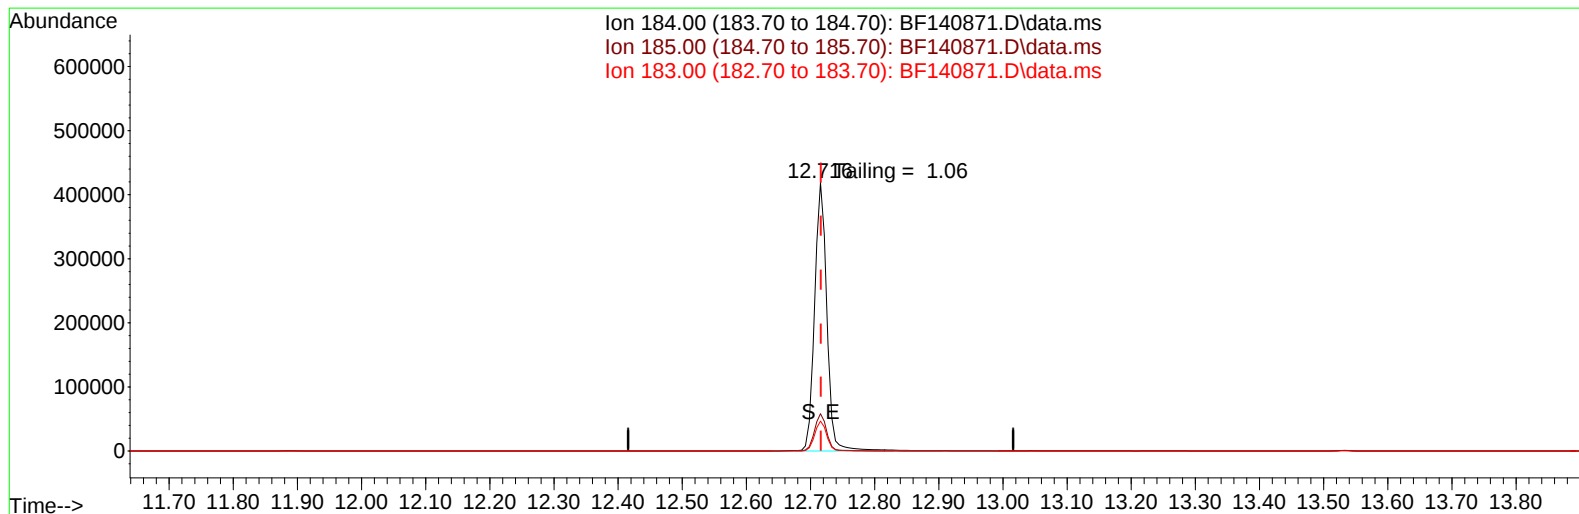

TIC: BF140871.D\data.ms

(77) Benzidine**12.716min (-0.000) 4637.75 ng****response 561870**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.89
183.00	11.20	11.16
0.00	0.00	0.00