




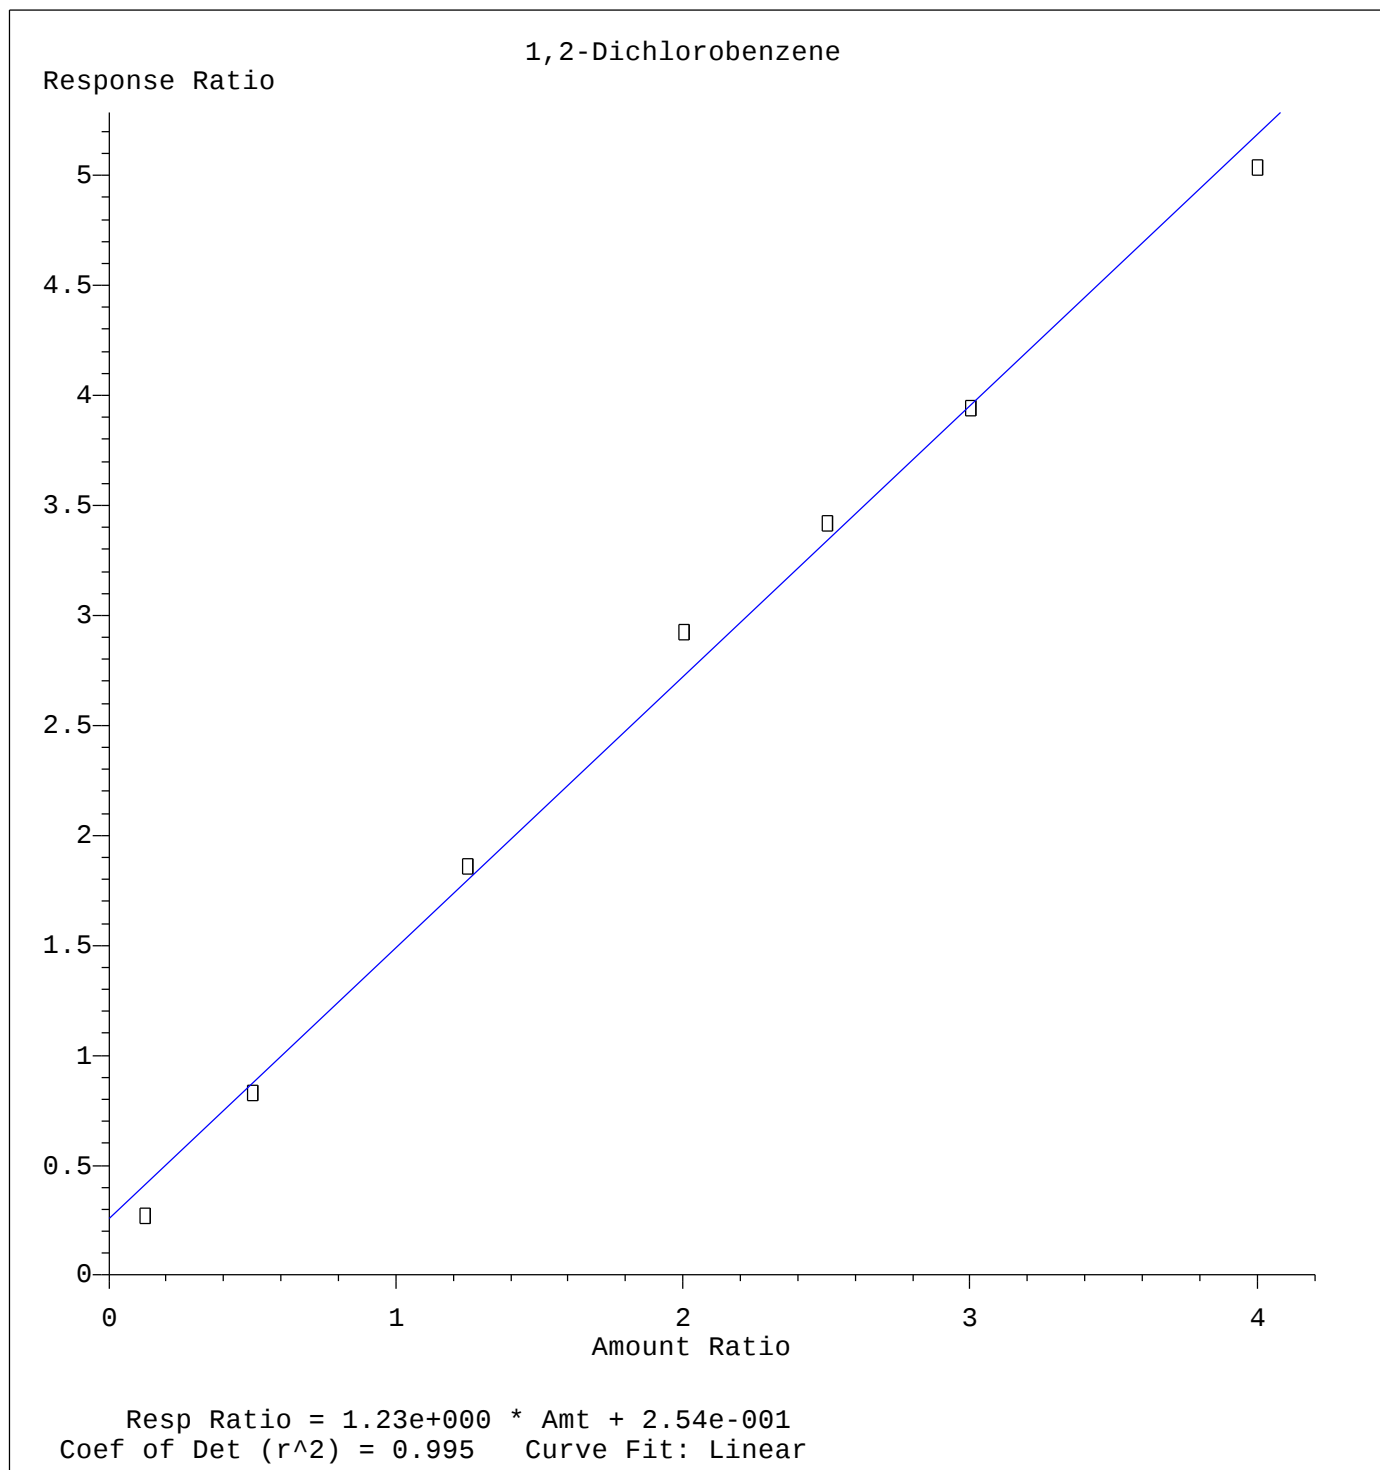

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF121815.M
Calibration Table Last Updated: Fri Dec 18 14:23:22 2015

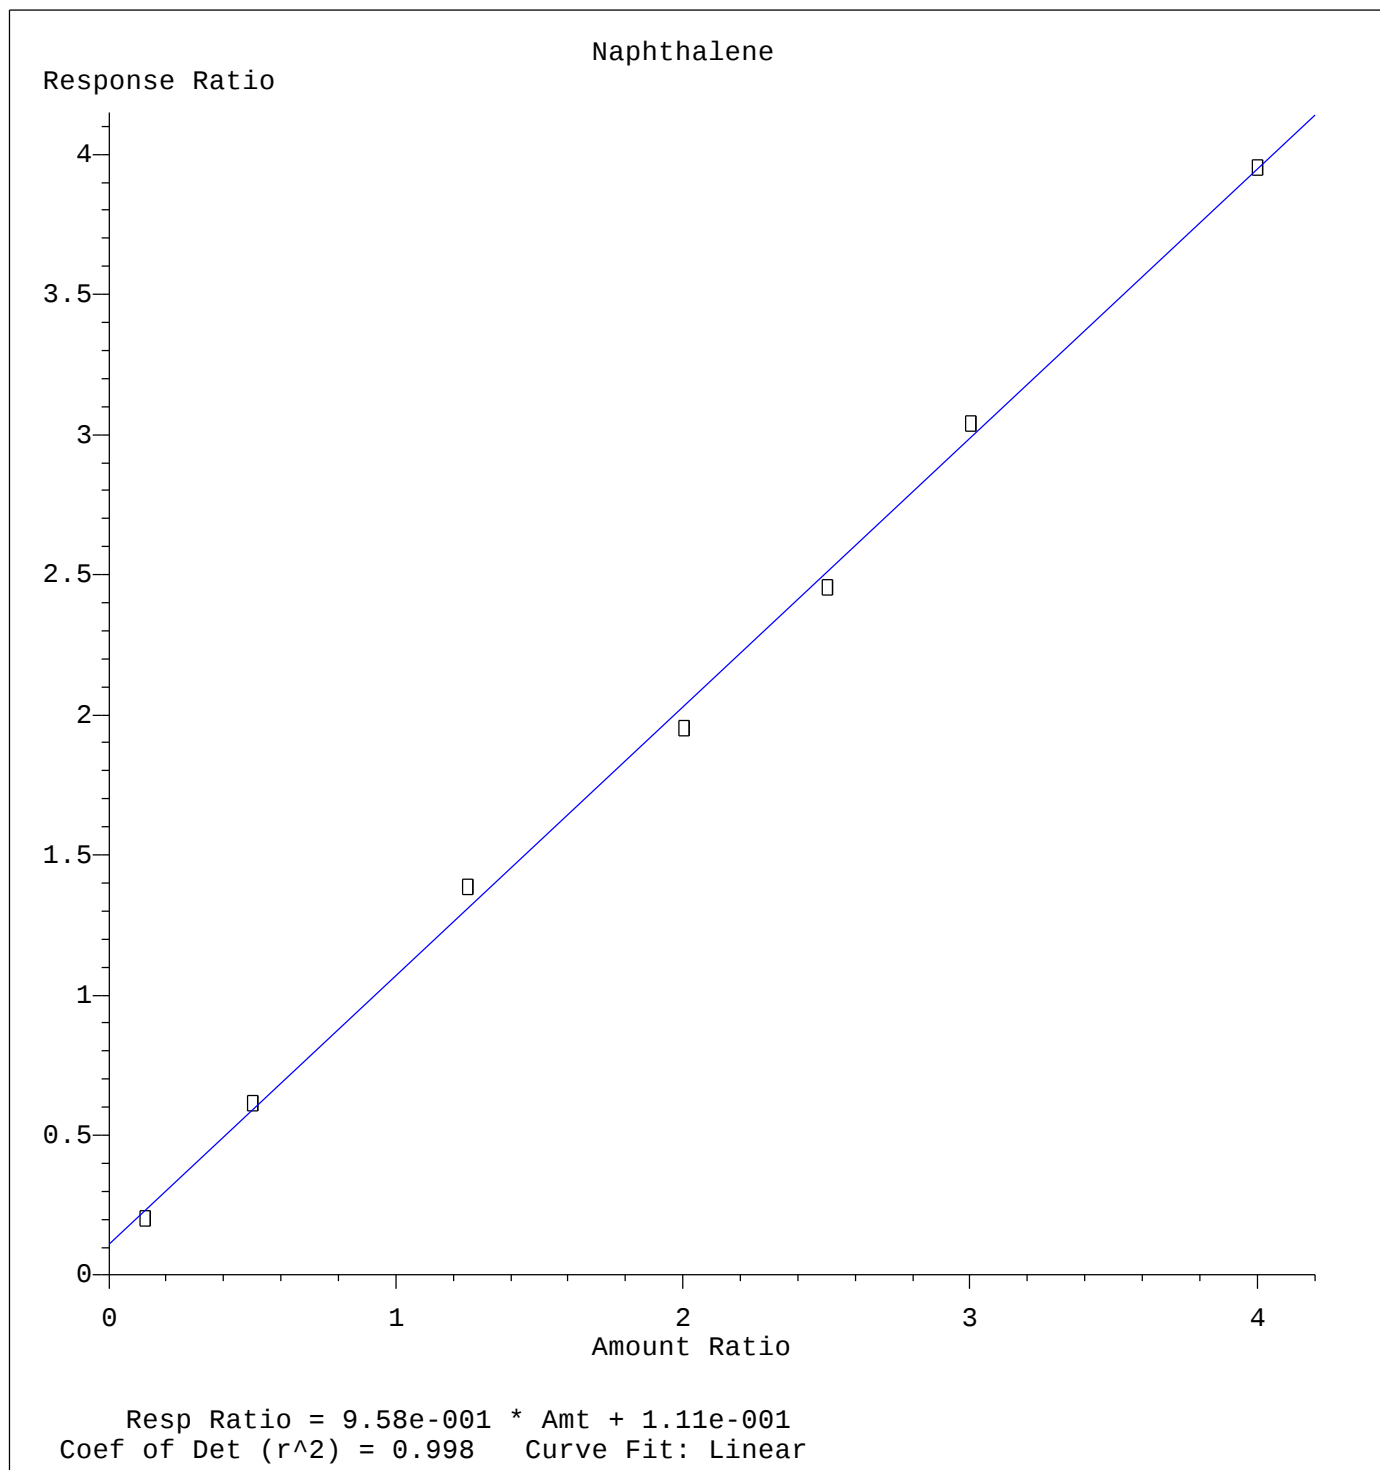


Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF121815.M
Calibration Table Last Updated: Fri Dec 18 14:23:22 2015

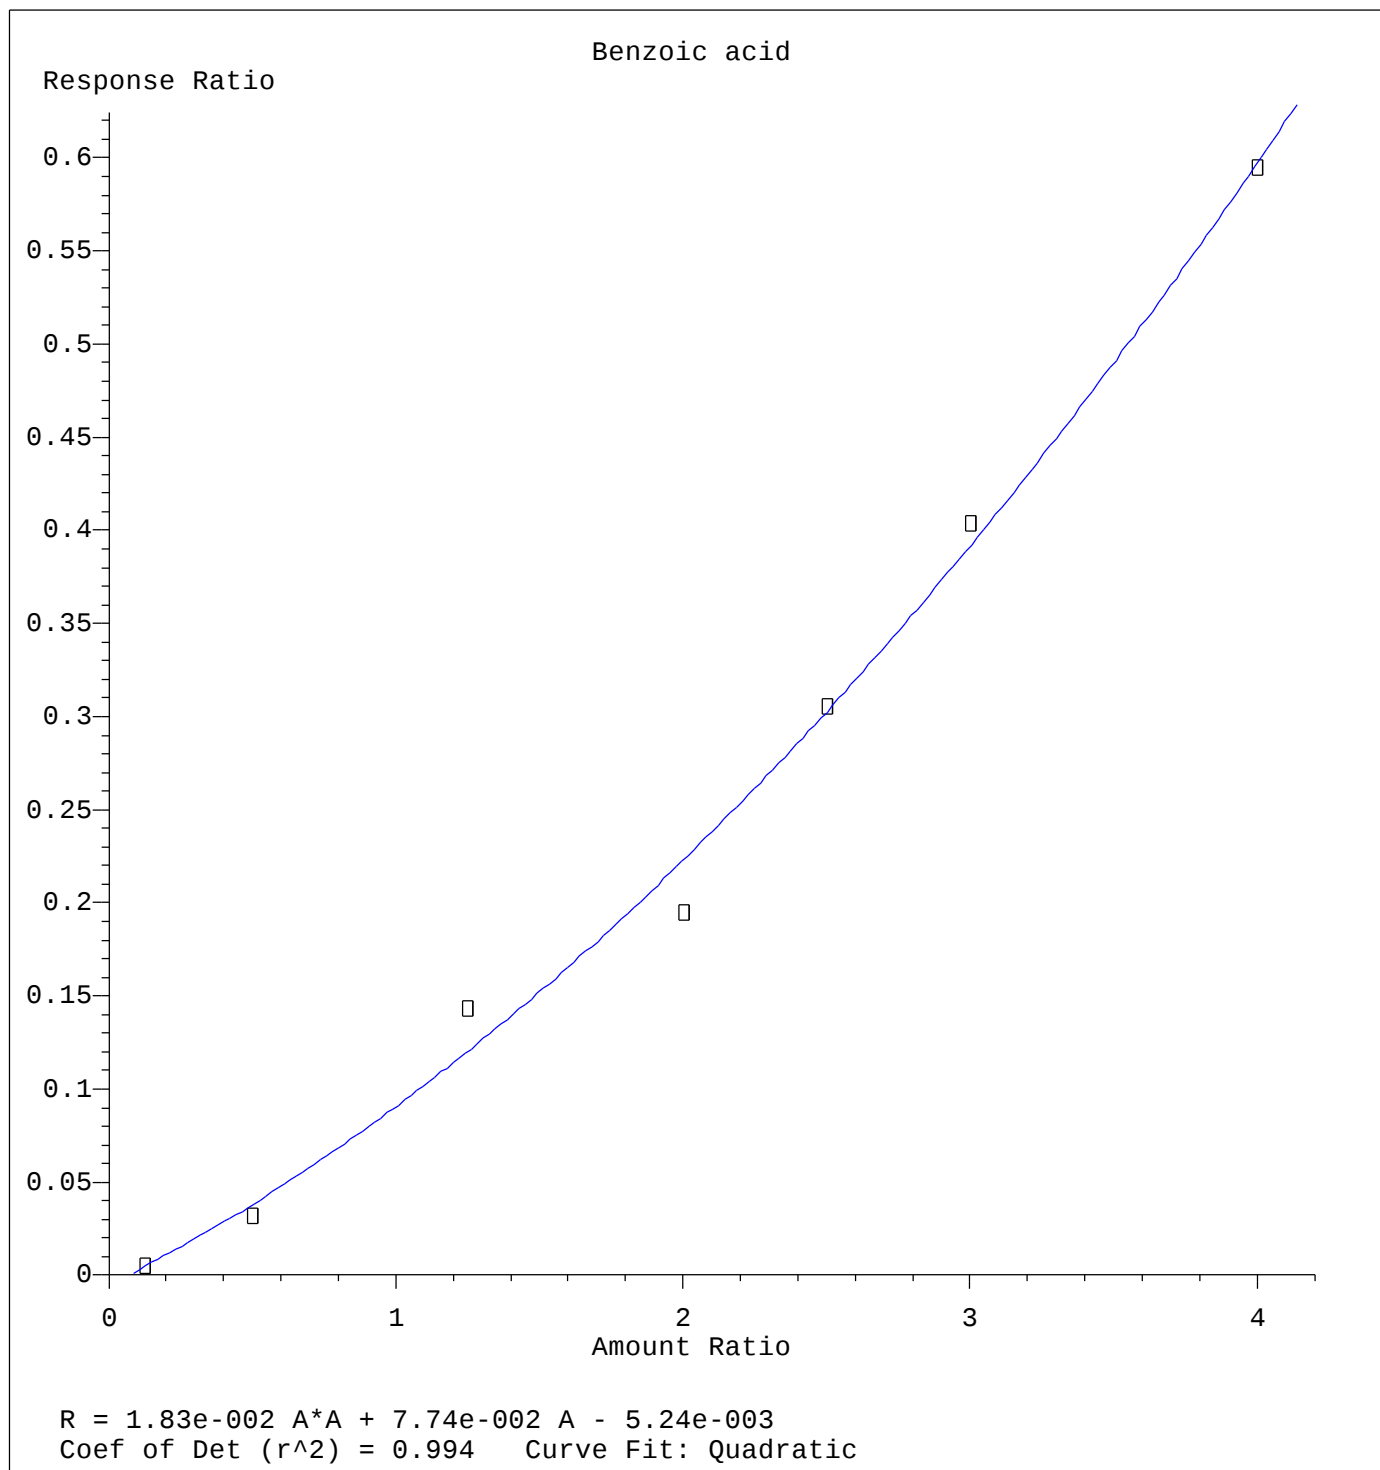

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF121815.M
Calibration Table Last Updated: Fri Dec 18 14:23:22 2015

4-Chloro-3-methylphenol

Response Ratio

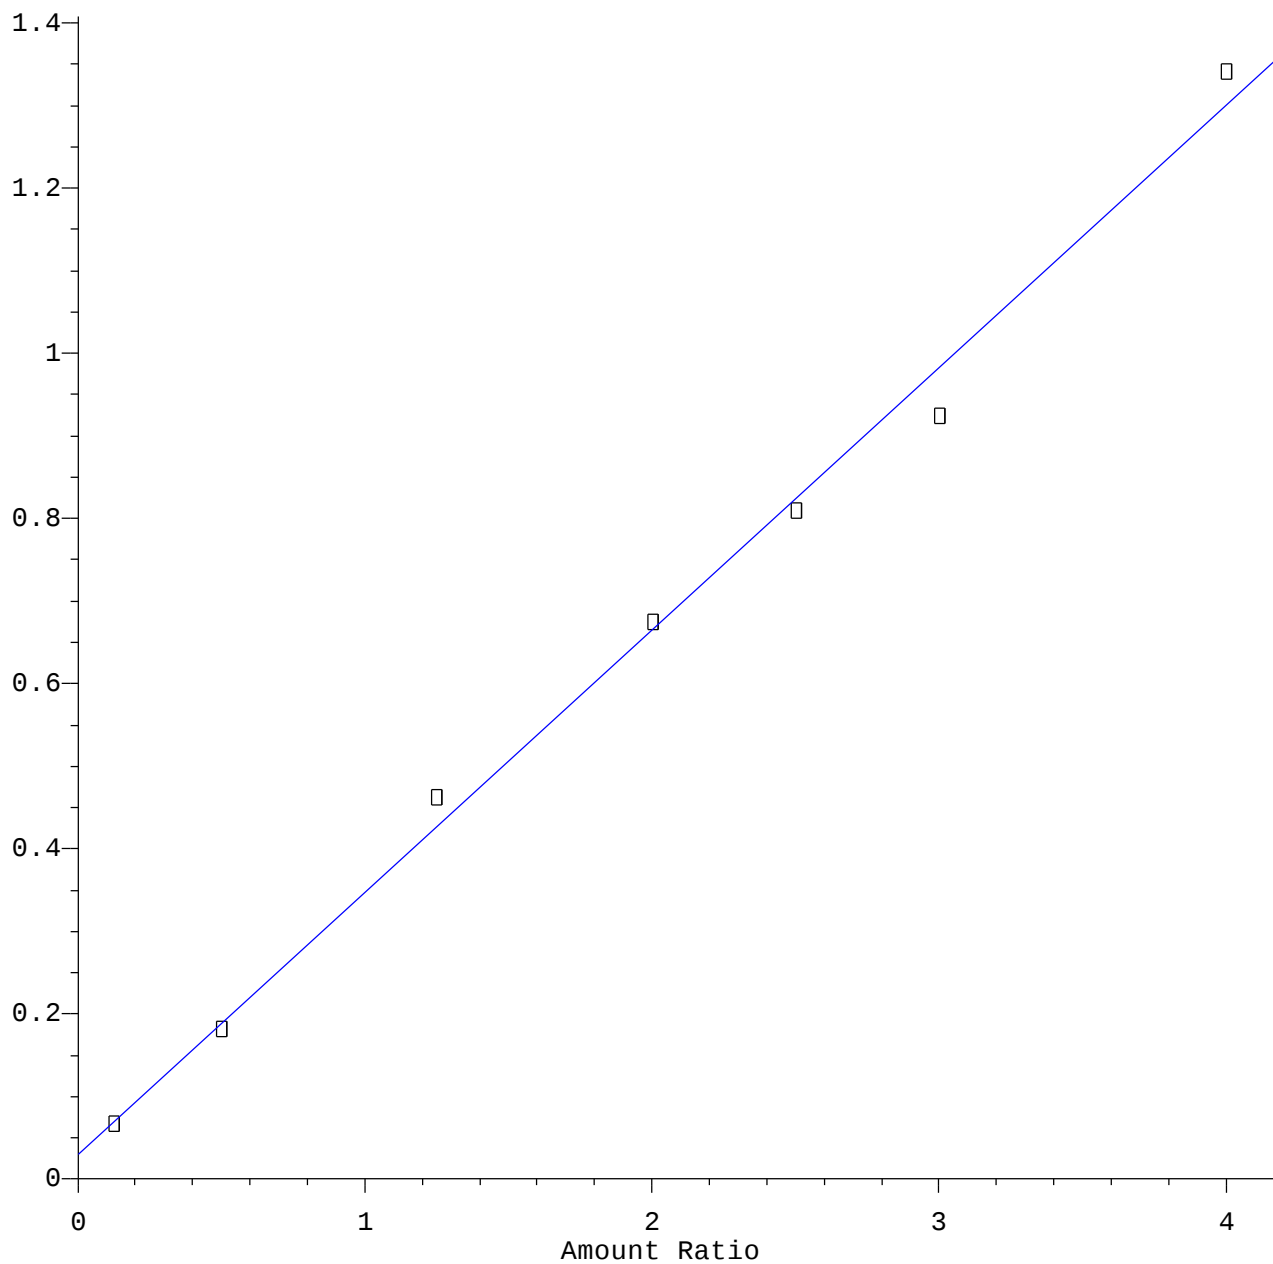


Resp Ratio = $3.18 \times 10^{-1} \times \text{Amt} + 2.92 \times 10^{-2}$
Coef of Det (r^2) = 0.994 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF121815.M
Calibration Table Last Updated: Fri Dec 18 14:23:22 2015

Hexachlorocyclopentadiene

Response Ratio

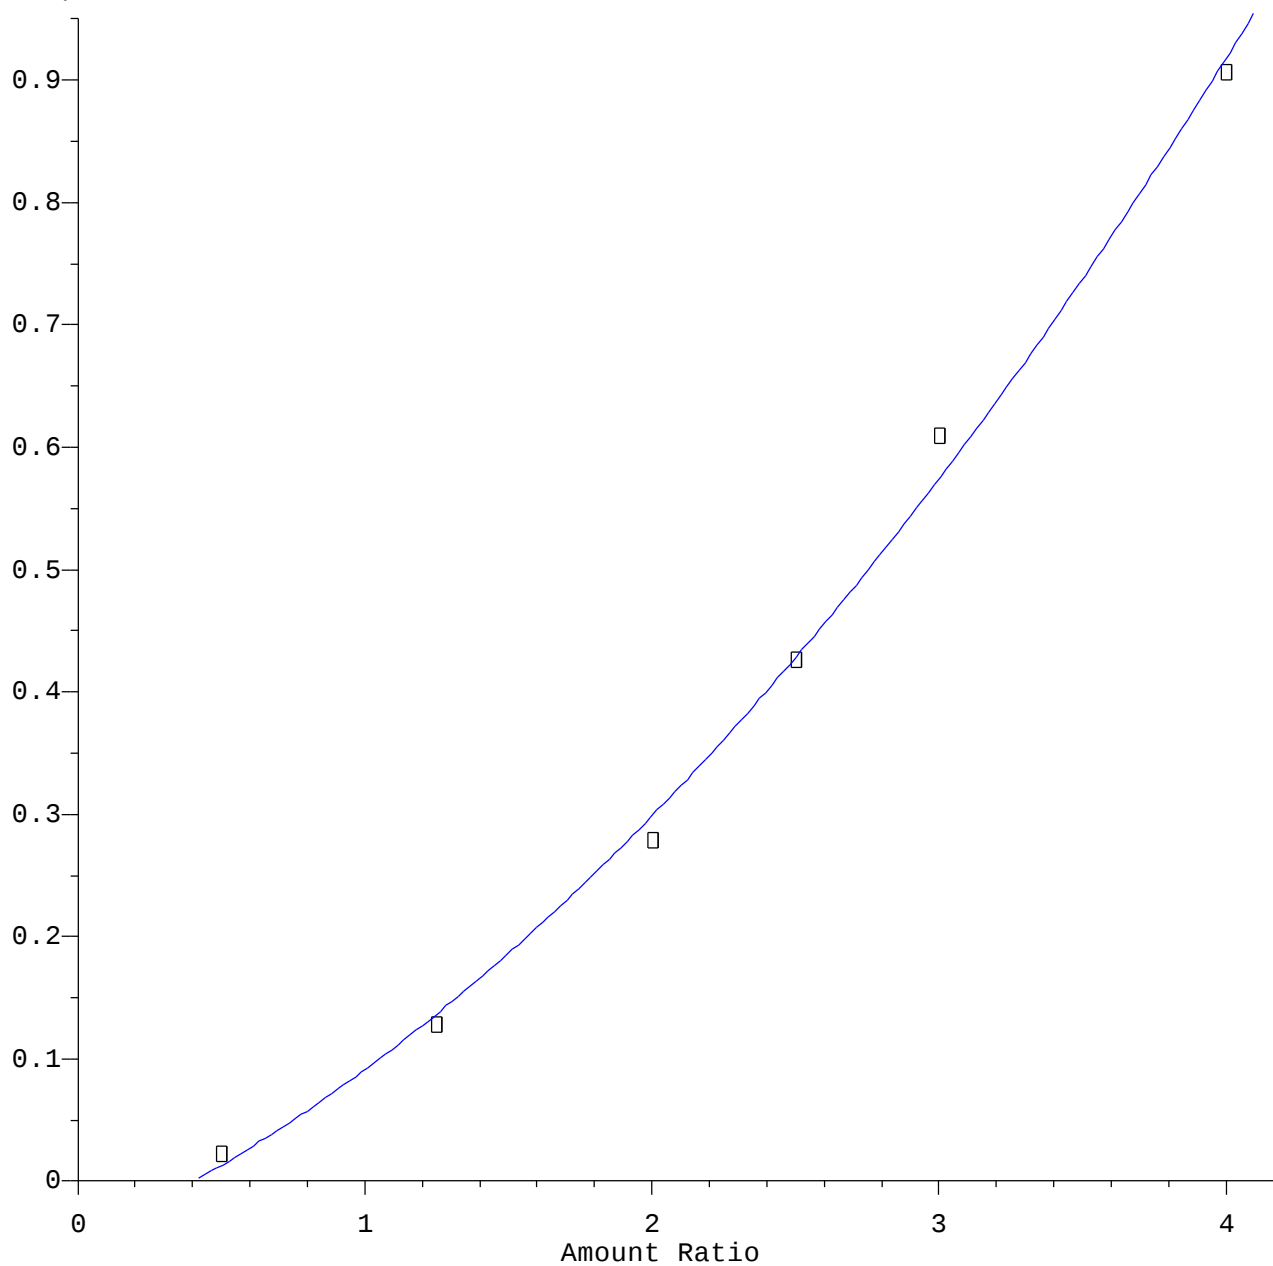


$R = 3.41e-002 A^2 + 1.05e-001 A - 4.84e-002$
Coef of Det (r^2) = 0.996 Curve Fit: Quadratic

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF121815.M
Calibration Table Last Updated: Fri Dec 18 14:23:22 2015

2-Fluorobiphenyl

Response Ratio

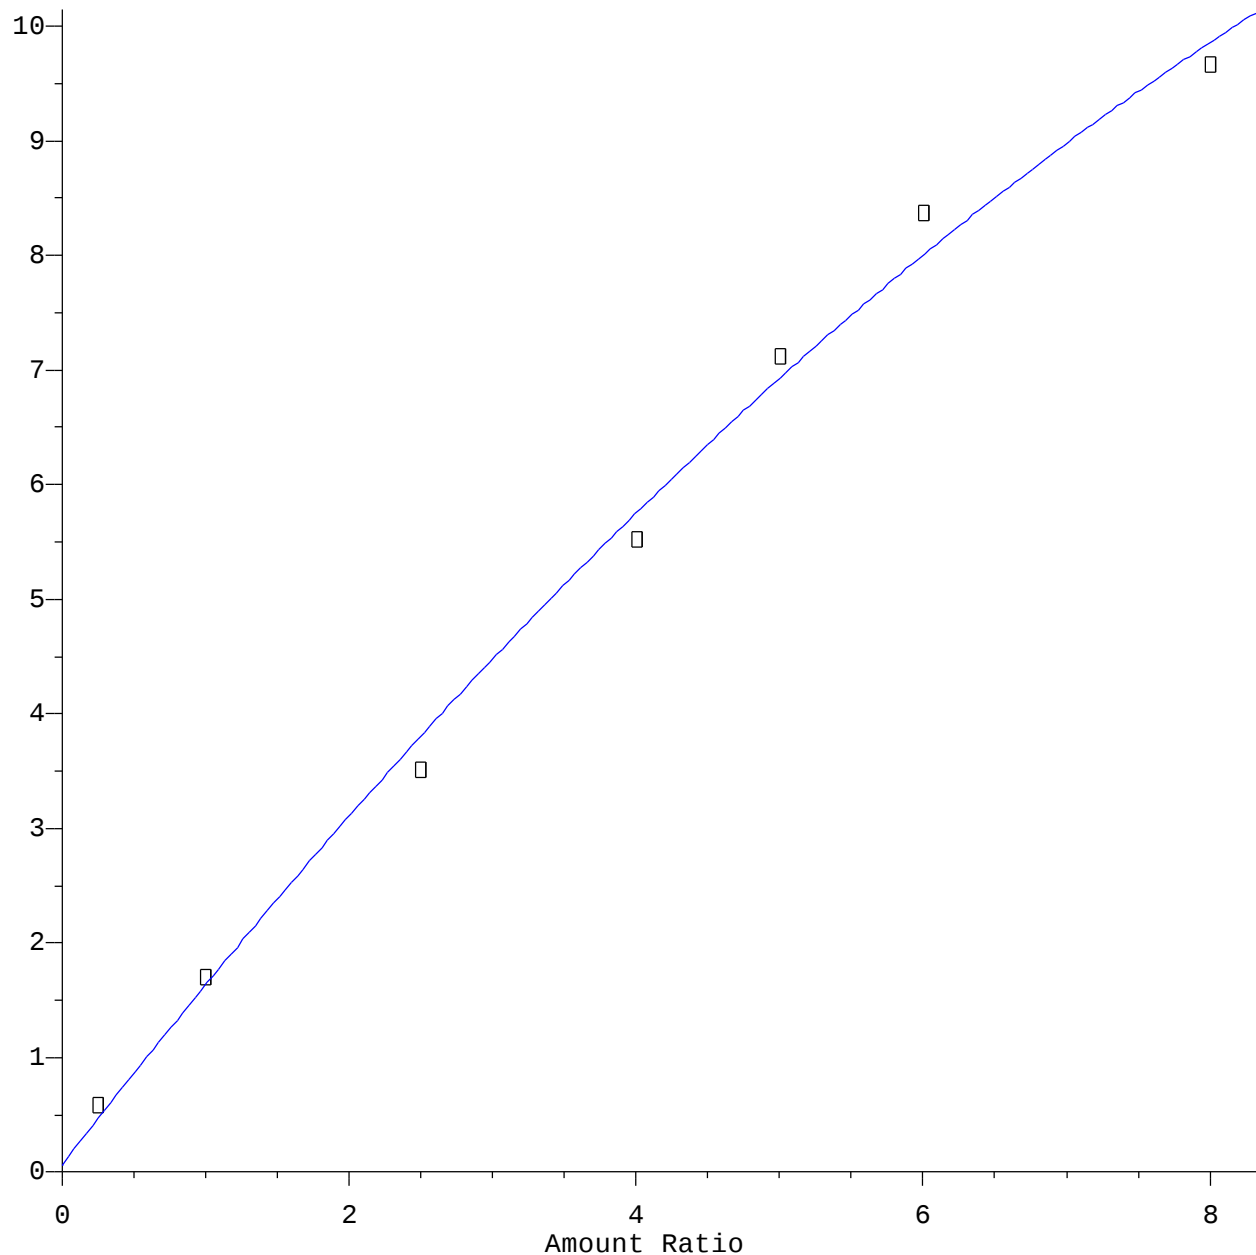


$R = -4.94e-002 A^2 + 1.62e+000 A + 6.38e-002$
Coef of Det (r^2) = 0.995 Curve Fit: Quadratic

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF121815.M
Calibration Table Last Updated: Fri Dec 18 14:23:22 2015

1,1'-Biphenyl

Response Ratio

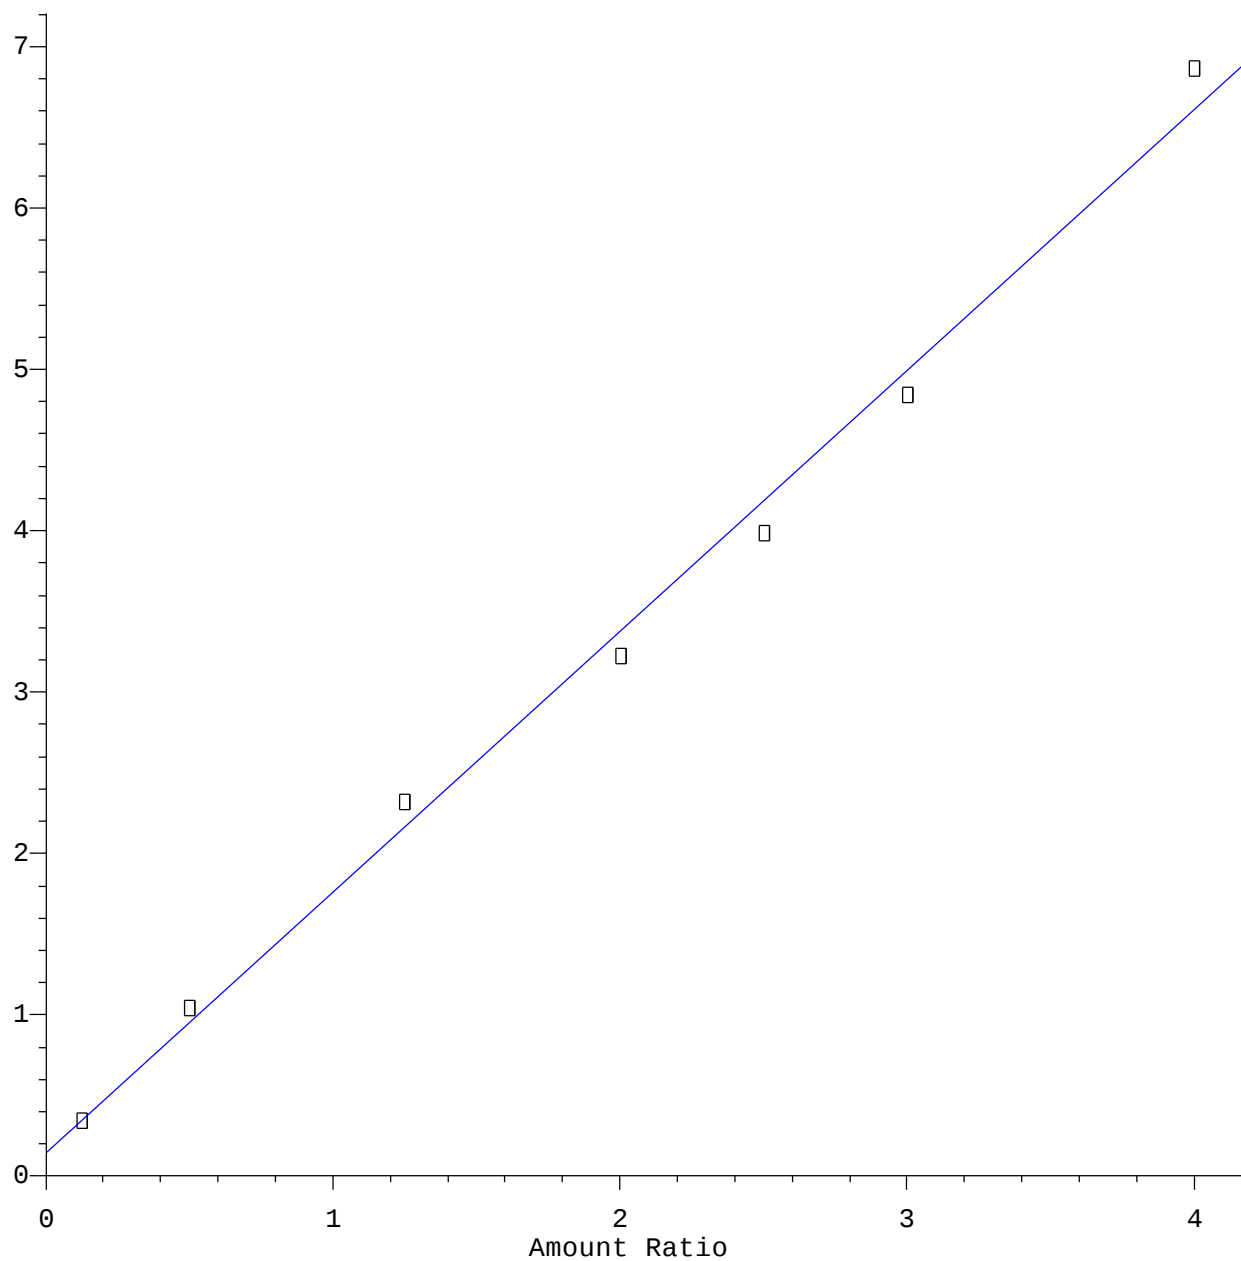


Resp Ratio = 1.62e+000 * Amt + 1.41e-001
Coef of Det (r^2) = 0.994 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF121815.M
Calibration Table Last Updated: Fri Dec 18 14:23:22 2015


2-Chloronaphthalene

Response Ratio

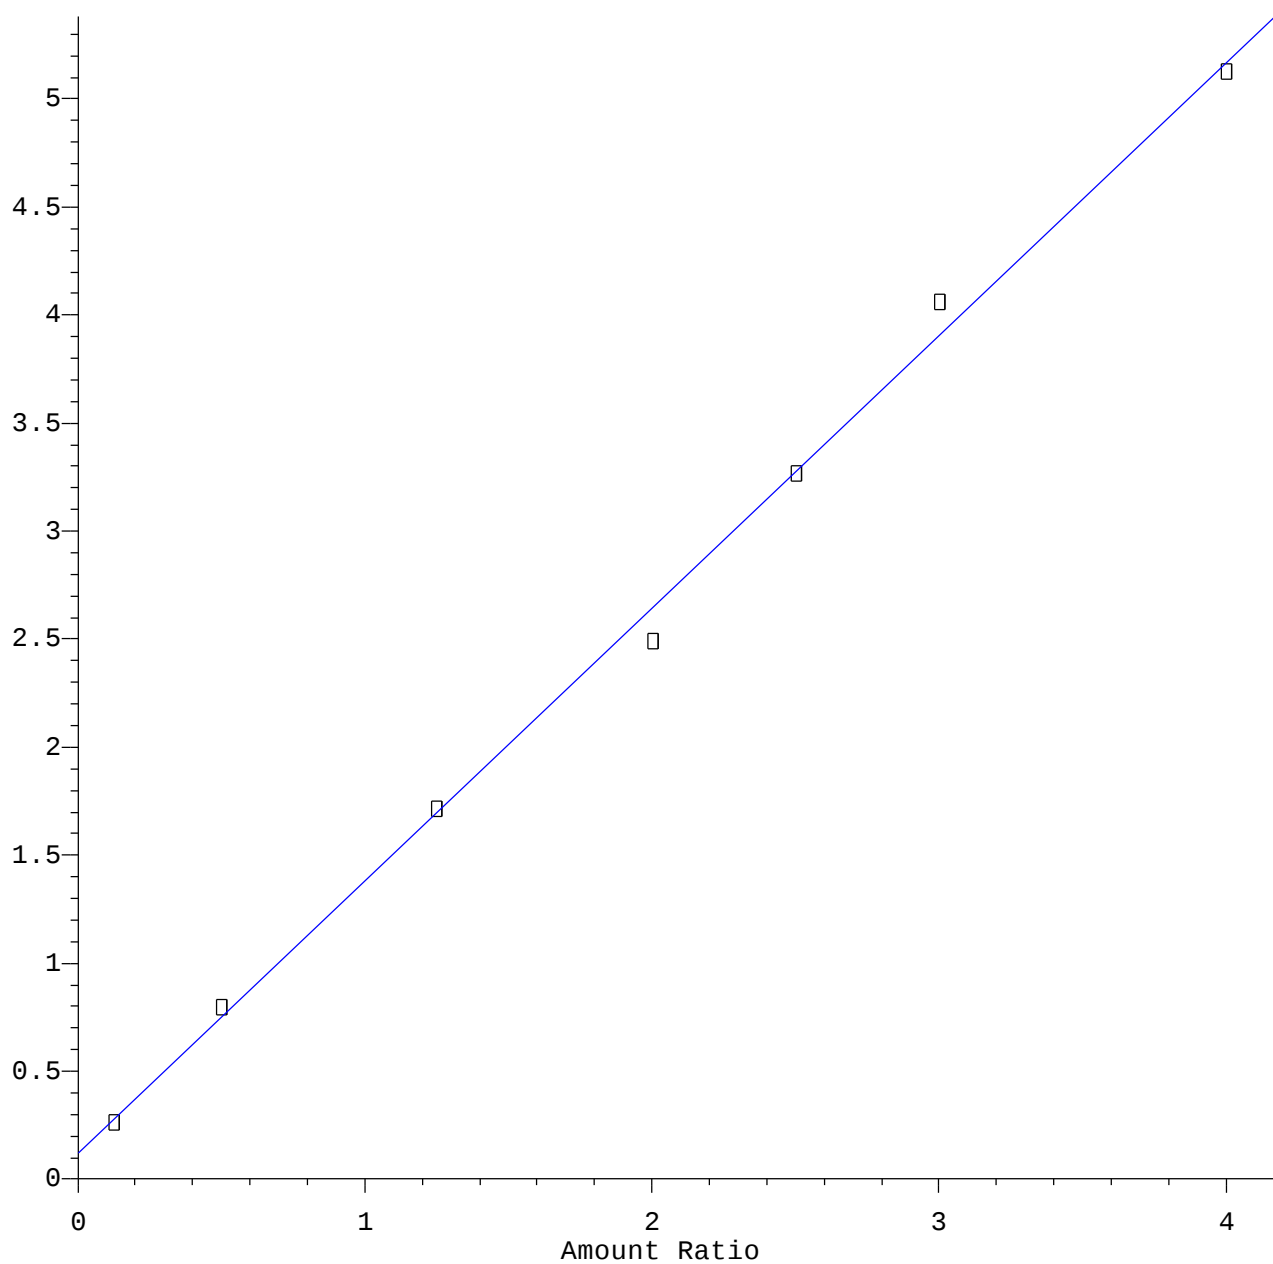


Resp Ratio = 1.26e+000 * Amt + 1.16e-001
Coef of Det (r^2) = 0.997 Curve Fit: Linear


Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF121815.M
Calibration Table Last Updated: Fri Dec 18 14:23:22 2015

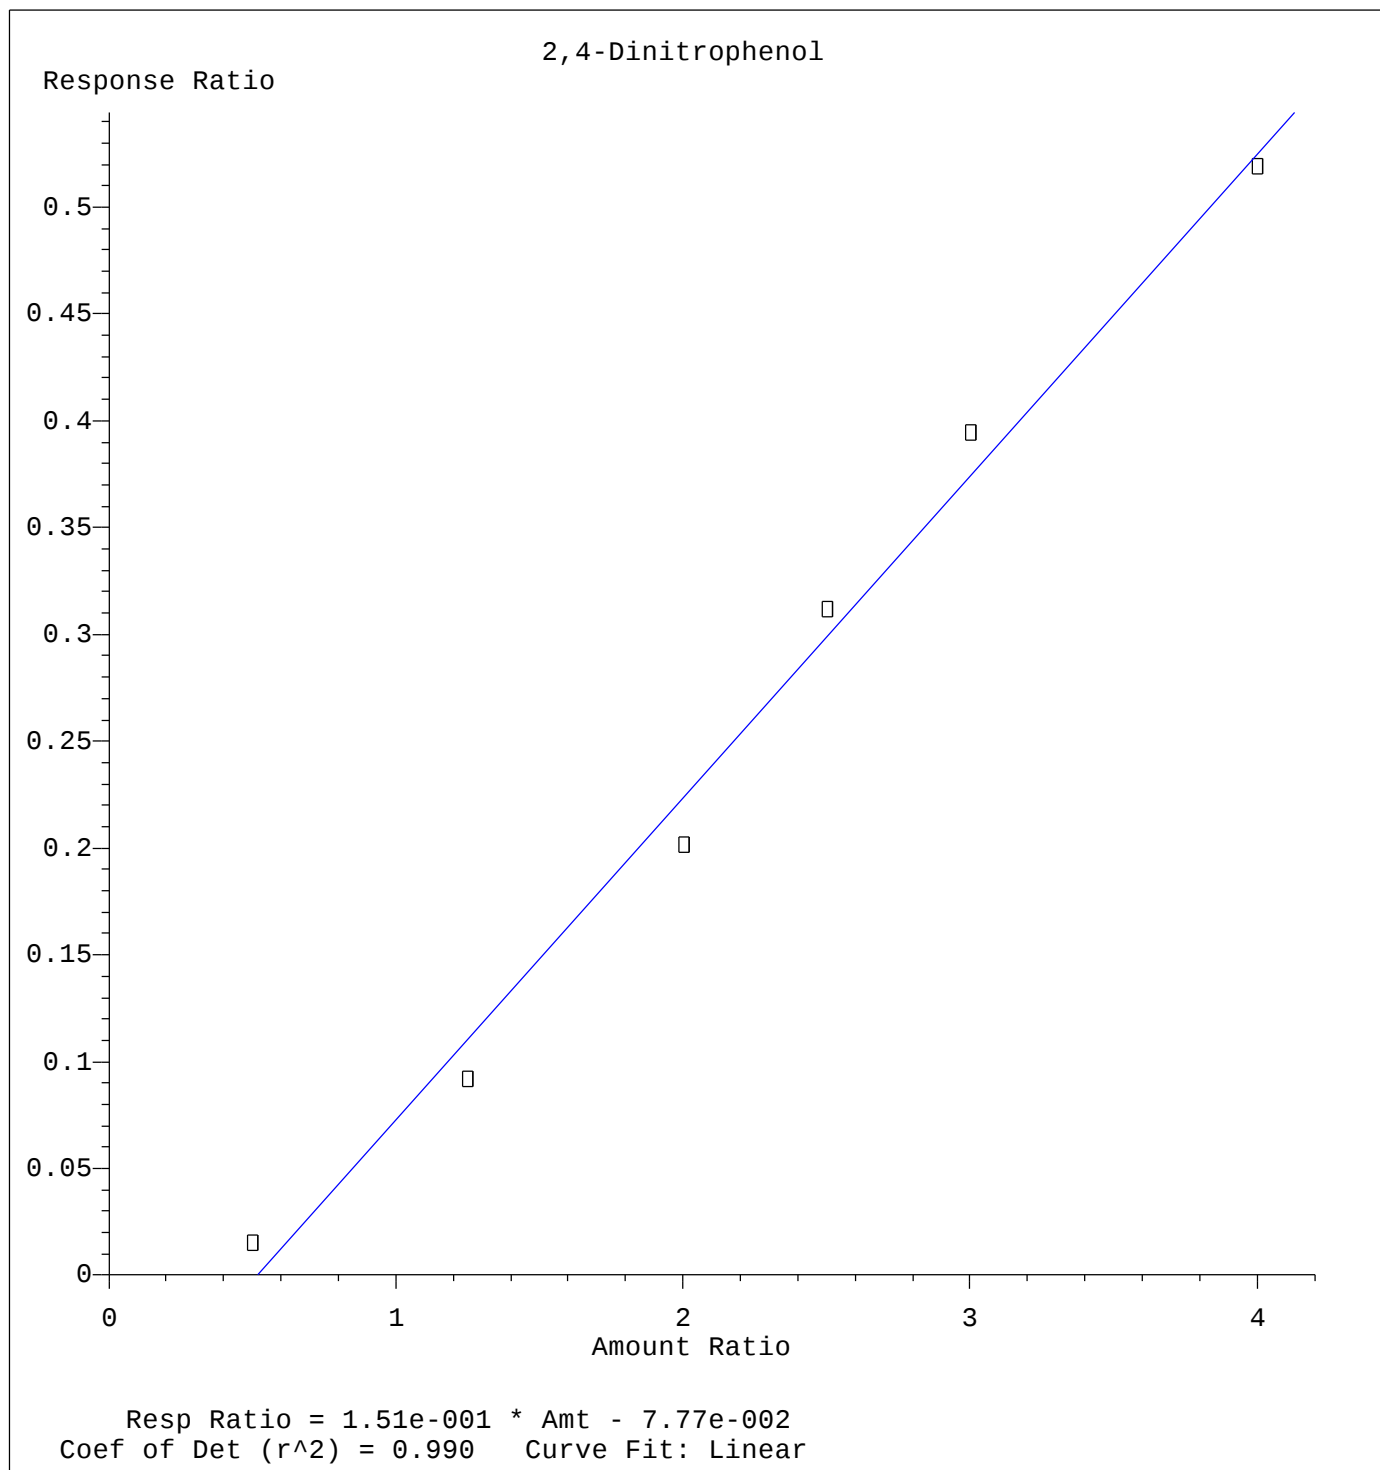


Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF121815.M
Calibration Table Last Updated: Fri Dec 18 14:23:22 2015

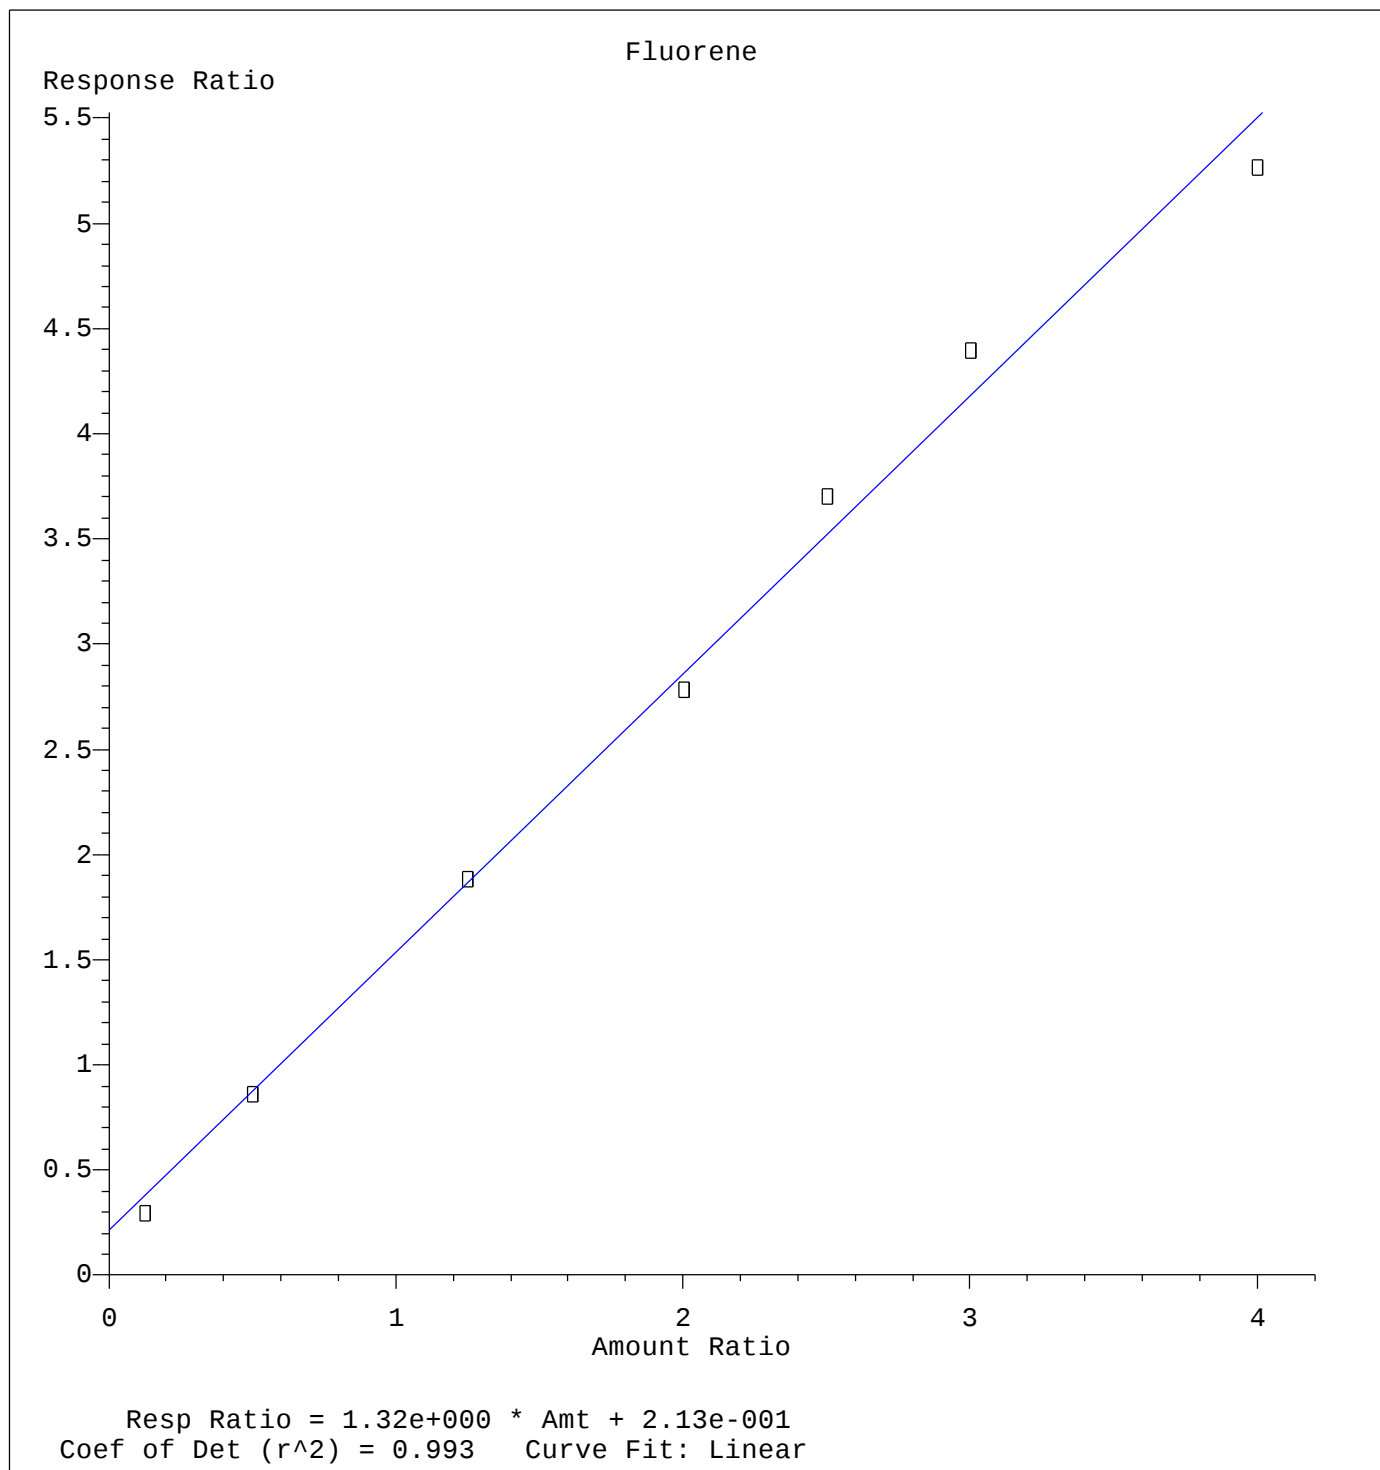


Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF121815.M
Calibration Table Last Updated: Fri Dec 18 14:23:22 2015

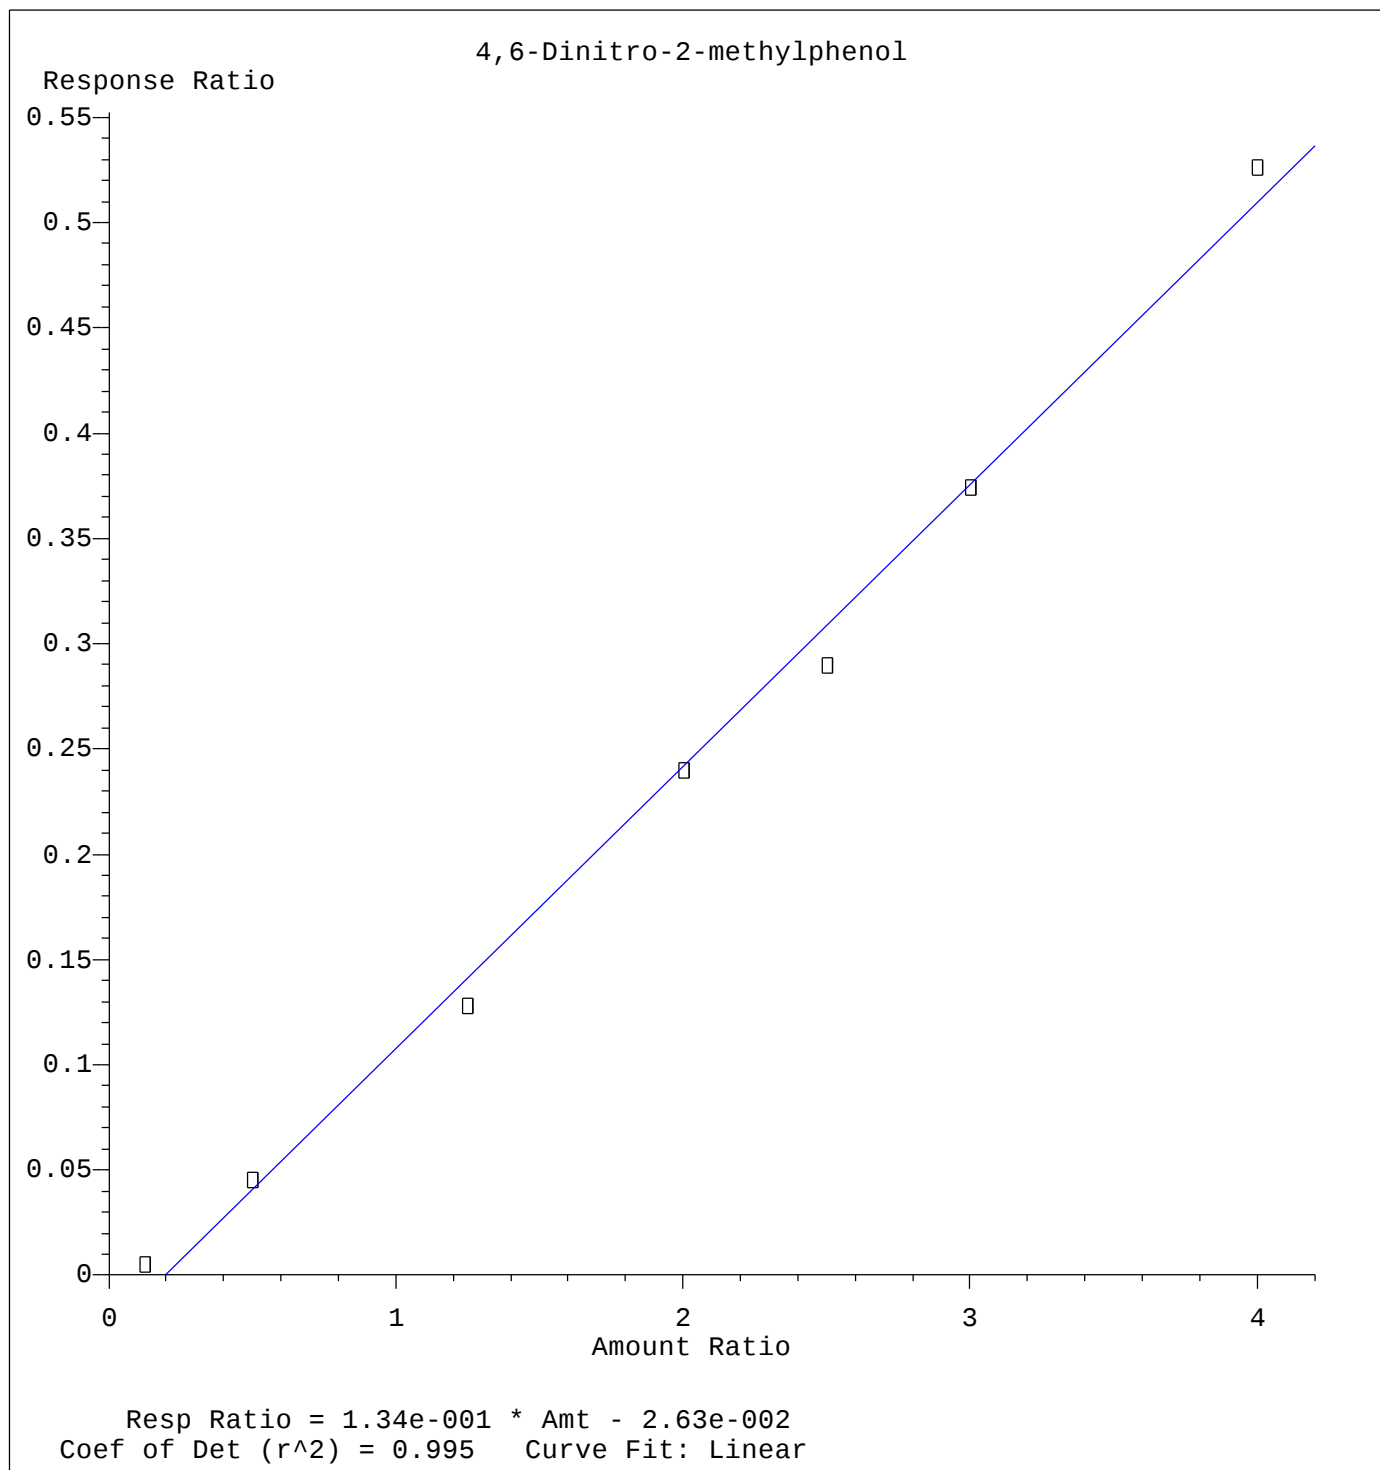


Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF121815.M
Calibration Table Last Updated: Fri Dec 18 14:23:22 2015

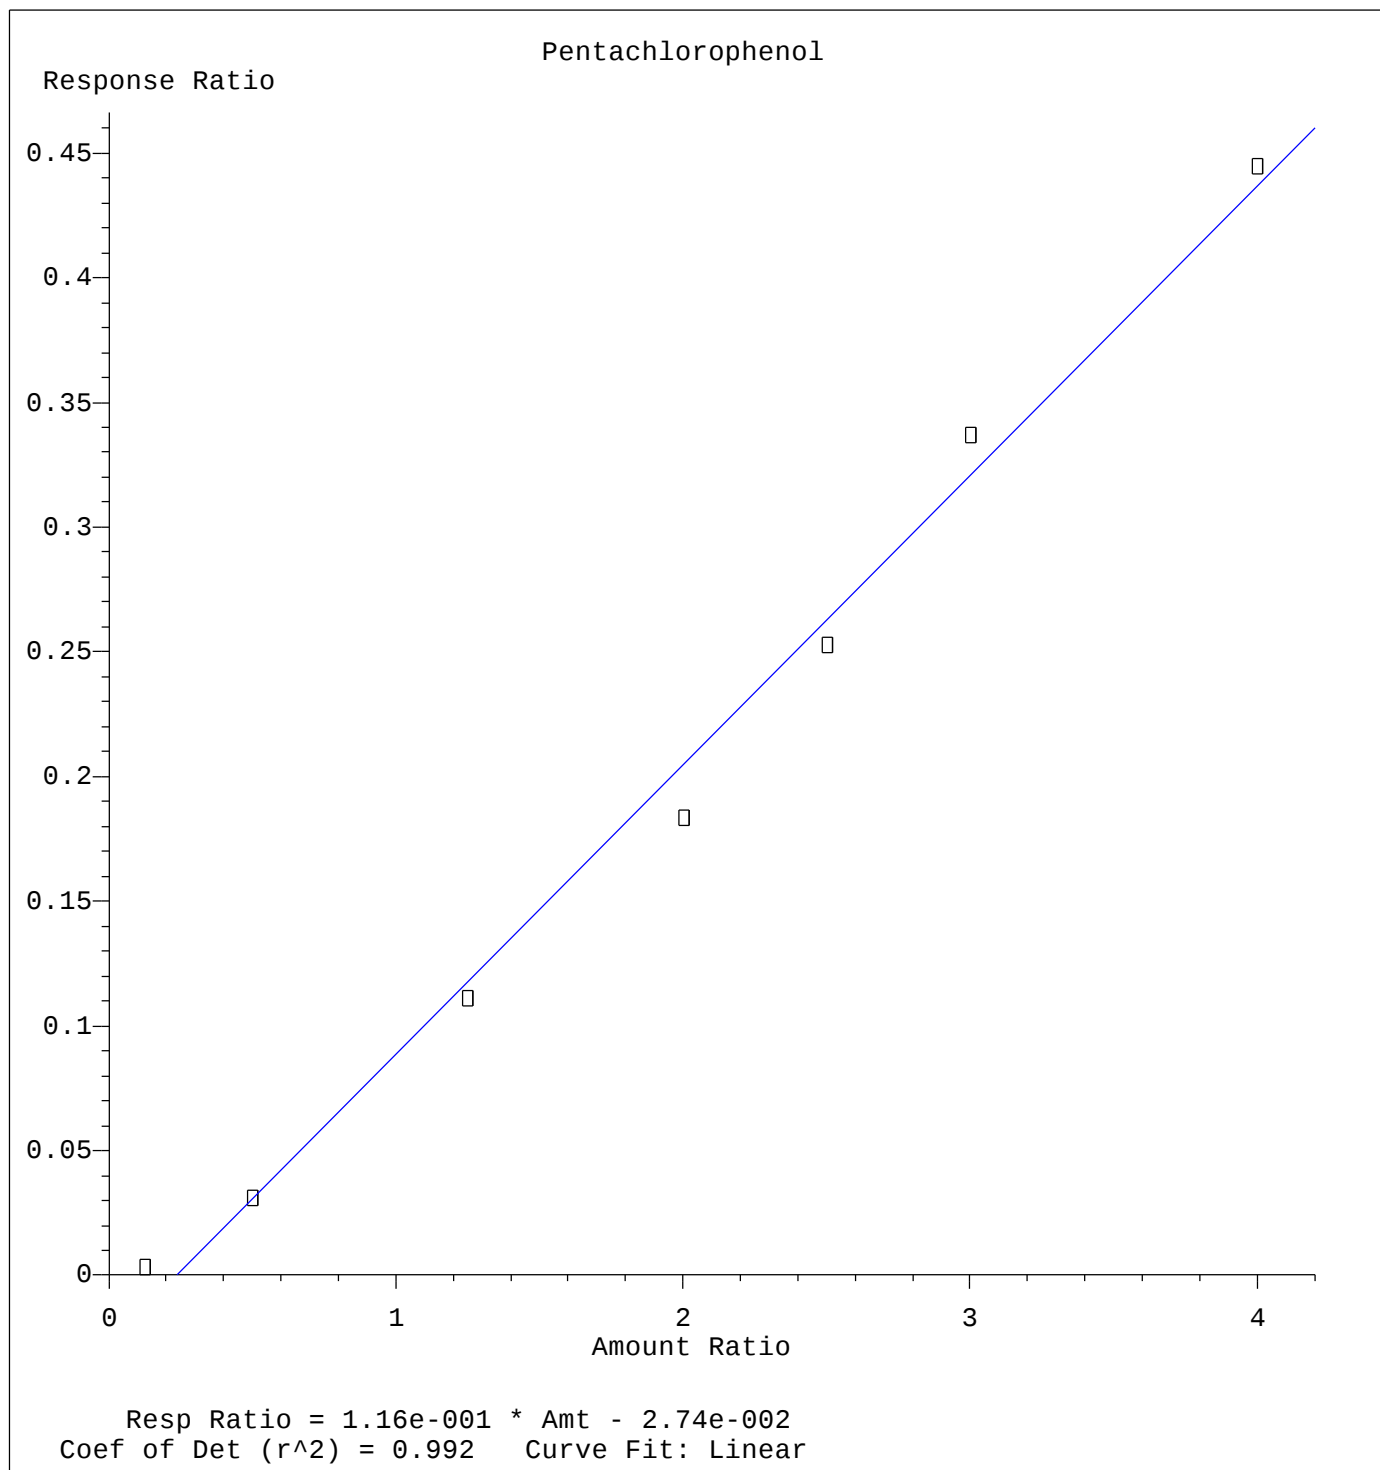

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF121815.M
Calibration Table Last Updated: Fri Dec 18 14:23:22 2015

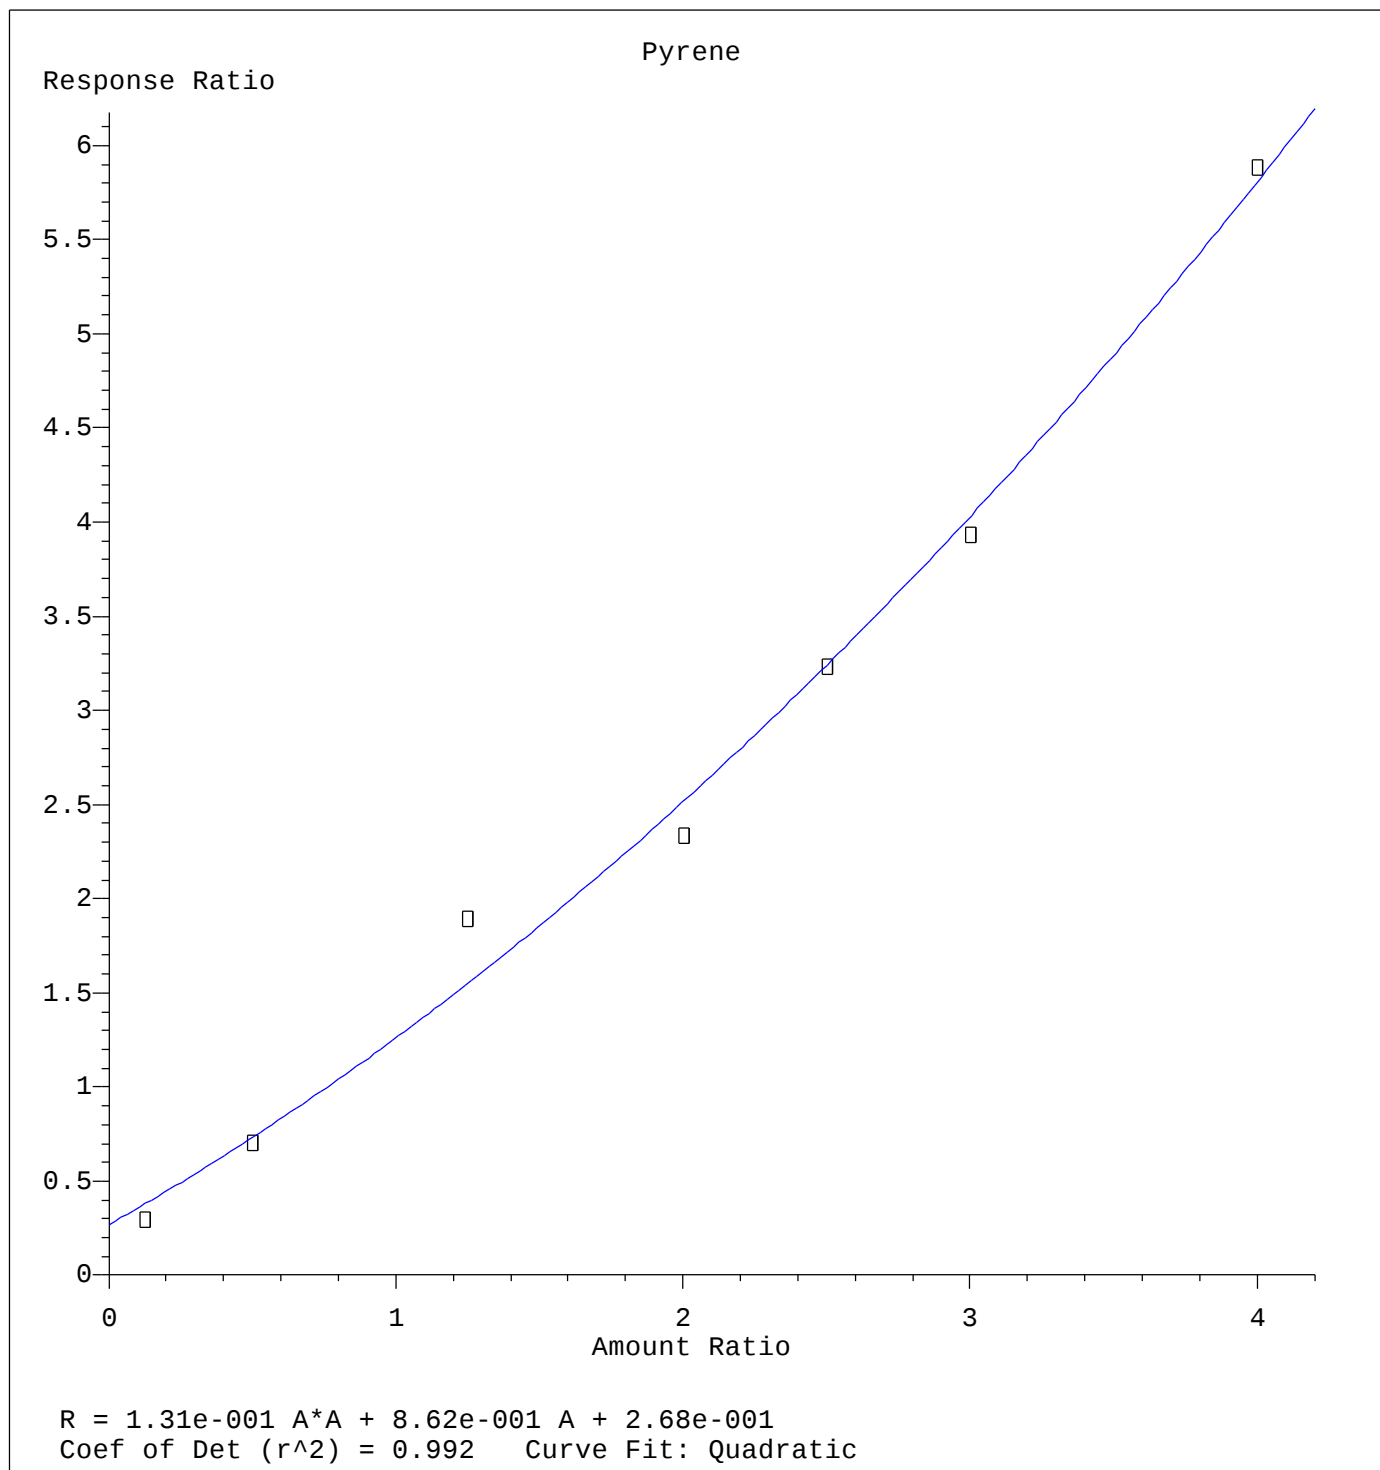

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF121815.M
Calibration Table Last Updated: Fri Dec 18 14:23:22 2015

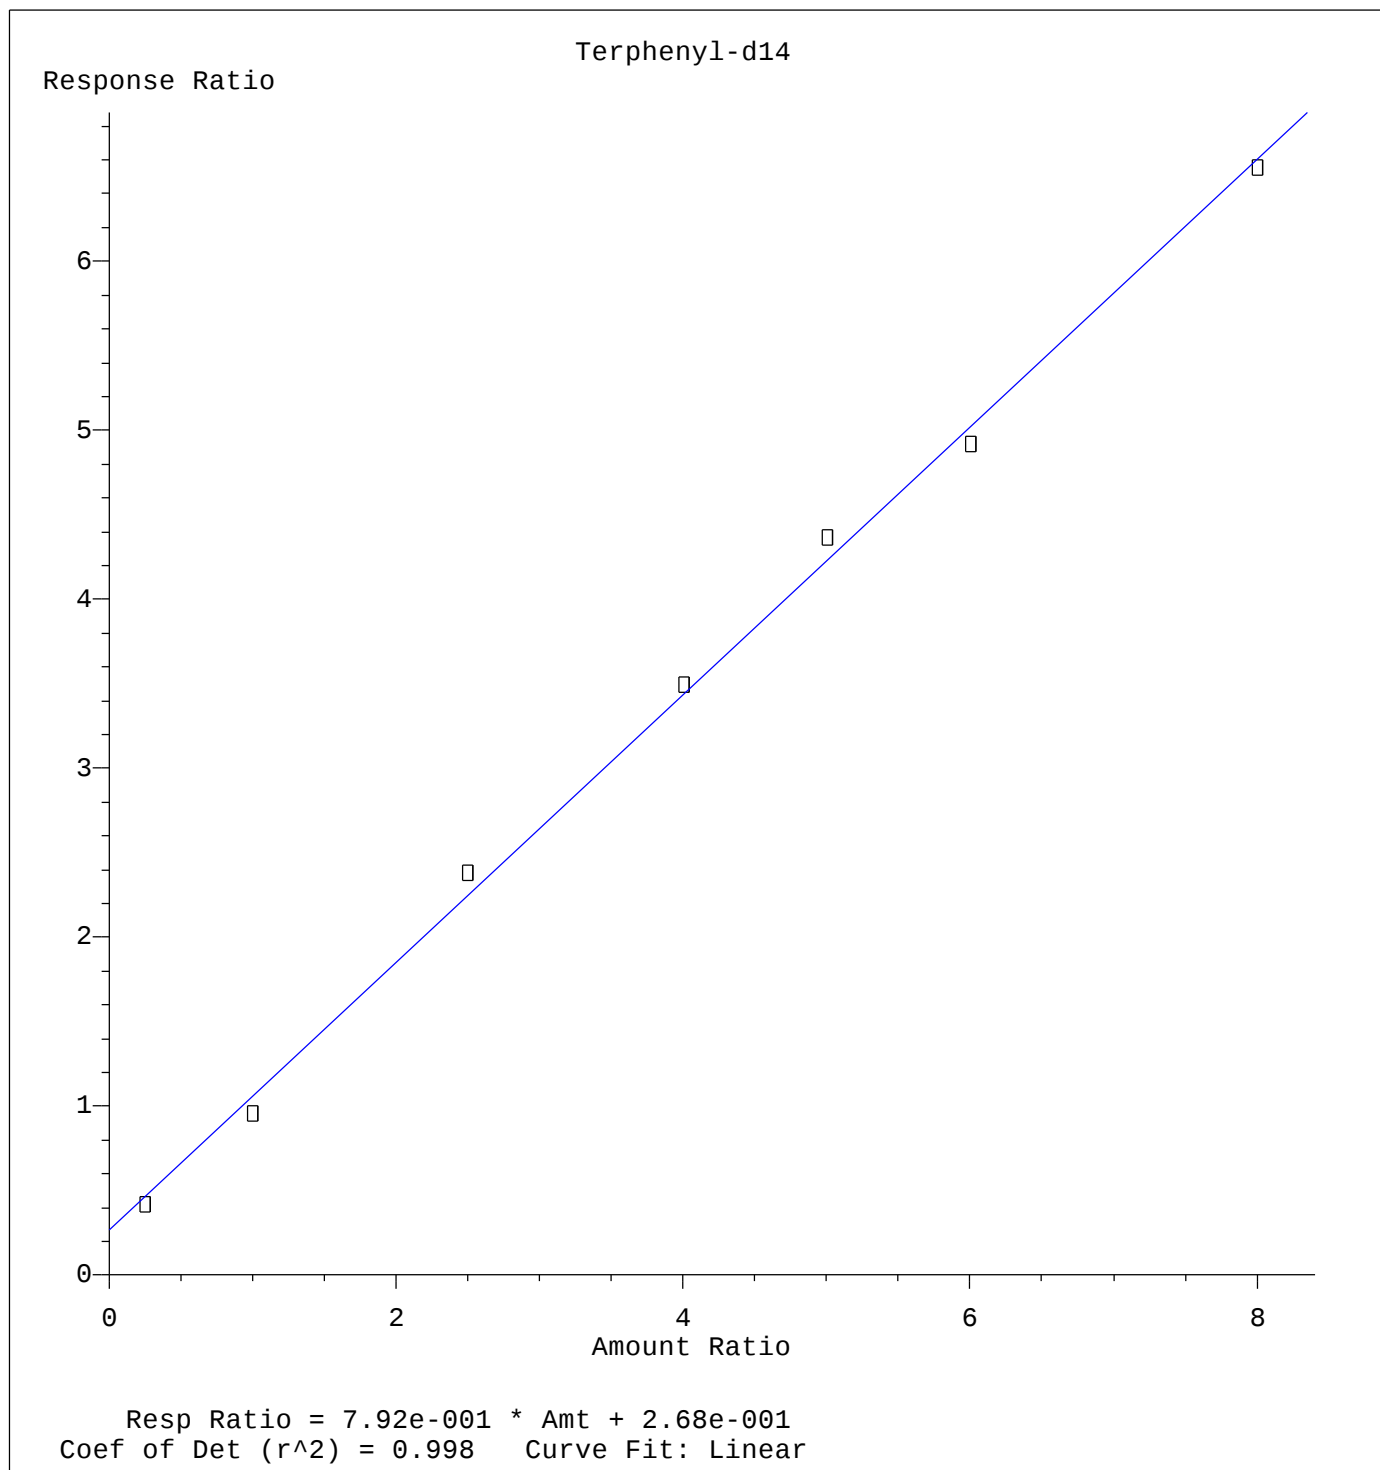

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF121815.M
Calibration Table Last Updated: Fri Dec 18 14:23:22 2015