


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF121815\
 Data File : BF083878.D
 Acq On : 17 Dec 2015 11:29
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121815.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 18 14:23:22 2015

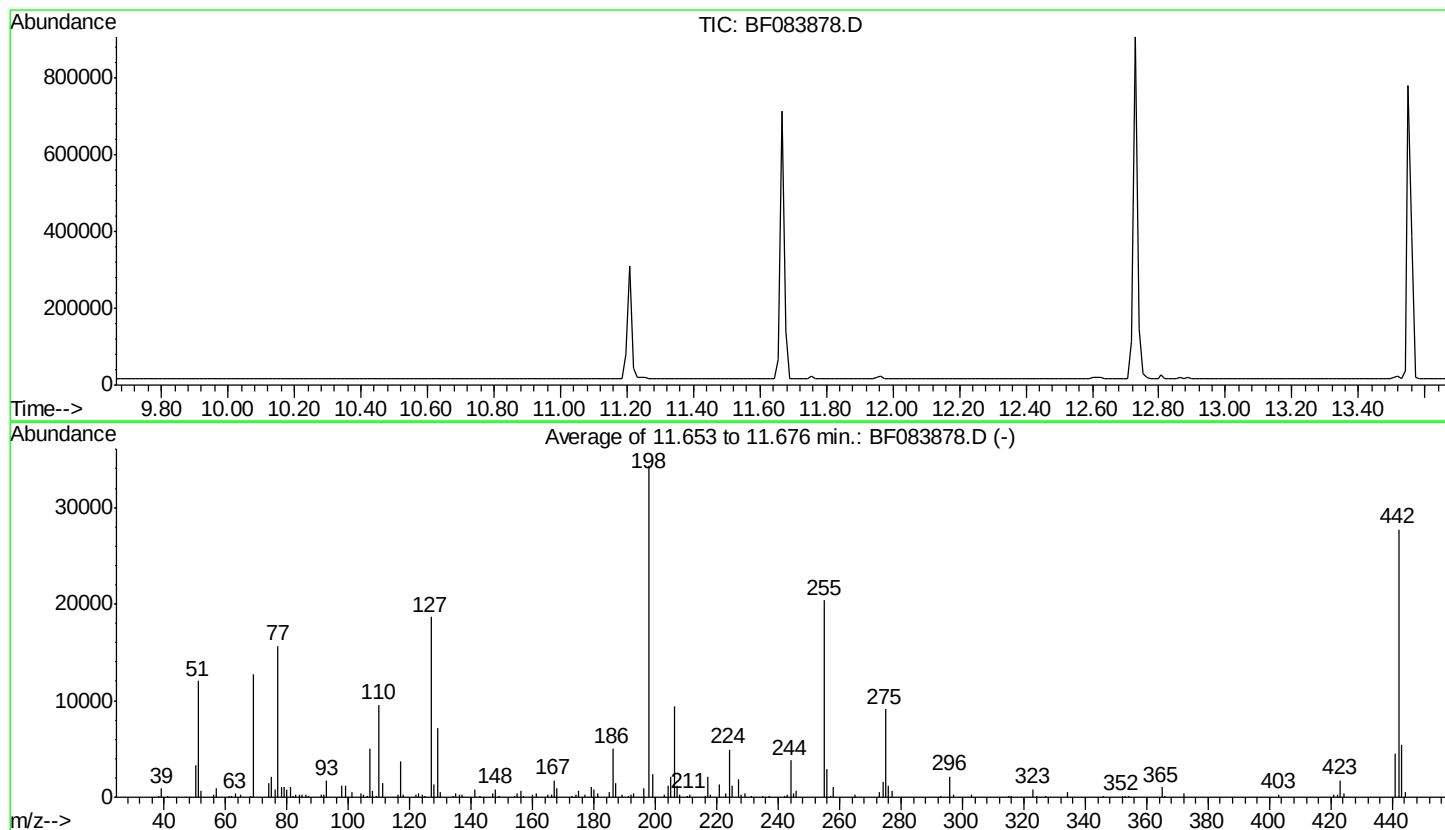

AutoFind: Scans 837, 838, 839; Background Corrected with Scan 834

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.0	12031	PASS
68	69	0.00	2	1.5	191	PASS
69	198	0.00	100	37.1	12734	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.3	18649	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	34331	PASS
199	198	5	9	6.9	2381	PASS
275	198	10	60	26.5	9096	PASS
365	198	1	100	3.0	1017	PASS
441	442	0.01	24	16.4	4537	PASS
442	198	50	100	80.8	27725	PASS
443	442	15	24	19.7	5468	PASS