


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF121815\
 Data File : BF083888.D
 Acq On : 18 Dec 2015 1:05
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121815.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 18 14:23:22 2015

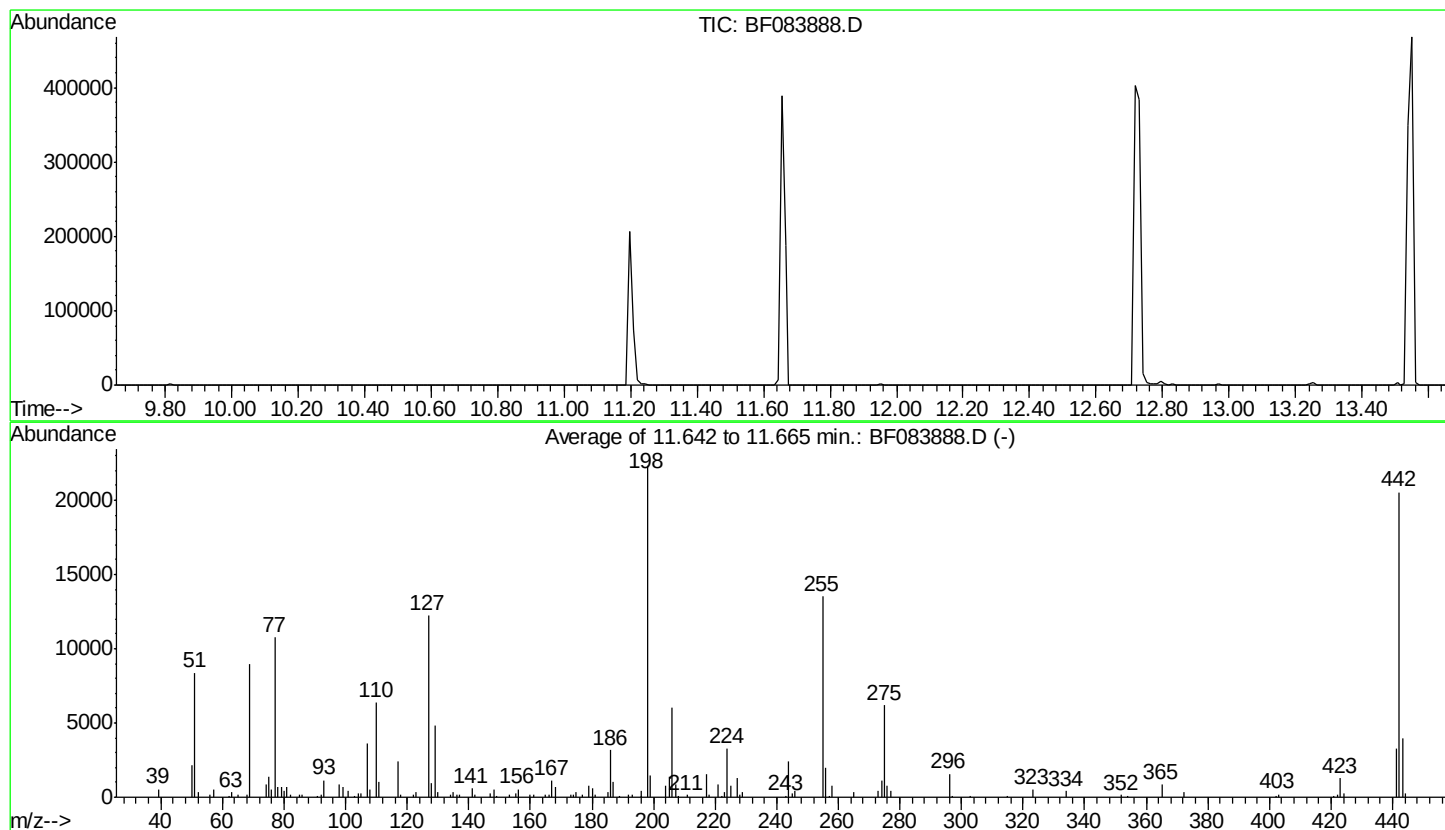

AutoFind: Scans 836, 837, 838; Background Corrected with Scan 833

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.6	8396	PASS
68	69	0.00	2	1.5	135	PASS
69	198	0.00	100	40.3	8992	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.8	12239	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	22328	PASS
199	198	5	9	6.5	1443	PASS
275	198	10	60	27.6	6169	PASS
365	198	1	100	3.8	858	PASS
441	442	0.01	24	16.0	3294	PASS
442	198	50	100	92.0	20531	PASS
443	442	15	24	19.5	4007	PASS