
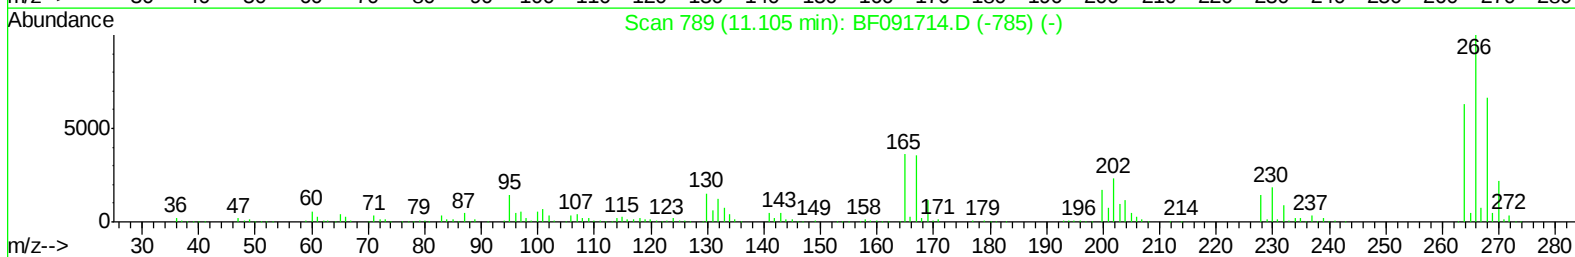
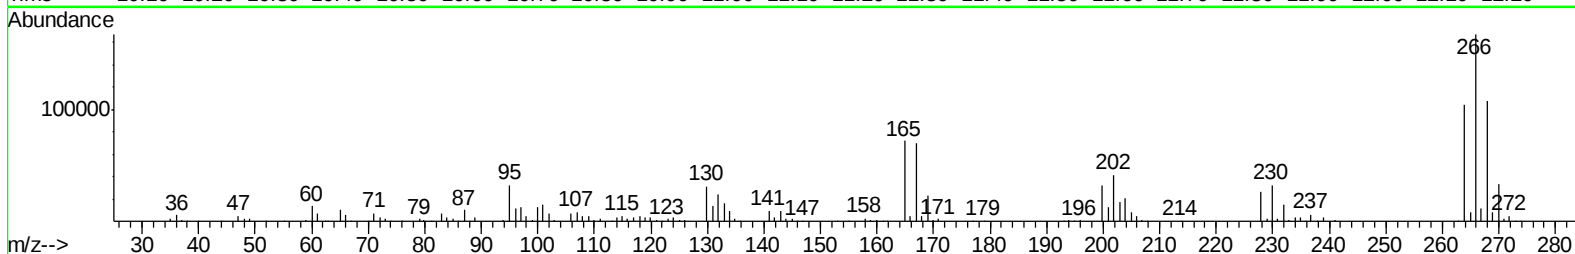


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF121816\
Data File : BF091732.D
Acq On : 18 Dec 2016 12:55
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 19 07:54:56 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 17 22:53:54 2016
Response via : Initial Calibration

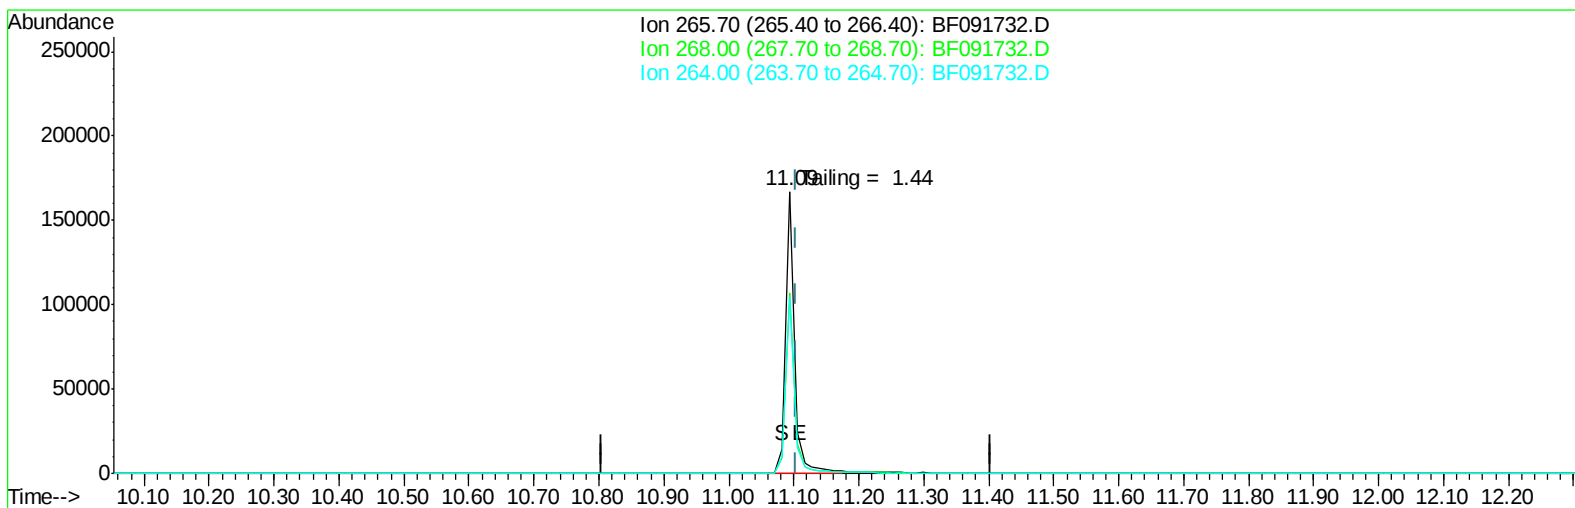

TIC: BF091732.D

(69) Pentachlorophenol (C)




11.093min (-0.011) 37582.96ng

response 157327

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	64.32
264.00	62.90	62.54
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF121816\
Data File : BF091732.D
Acq On : 18 Dec 2016 12:55
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 19 07:54:56 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 17 22:53:54 2016
Response via : Initial Calibration

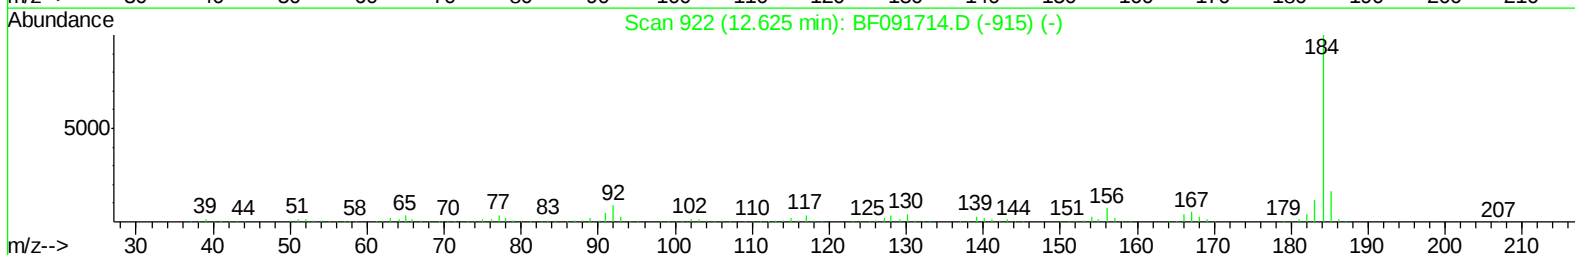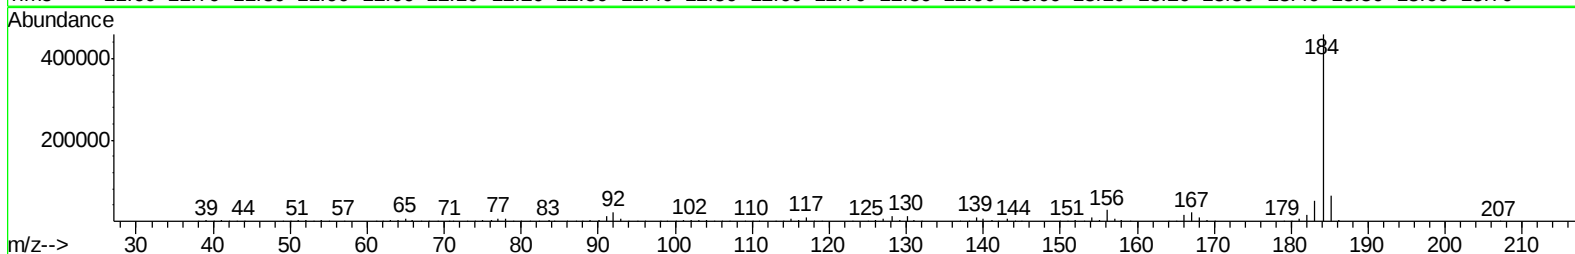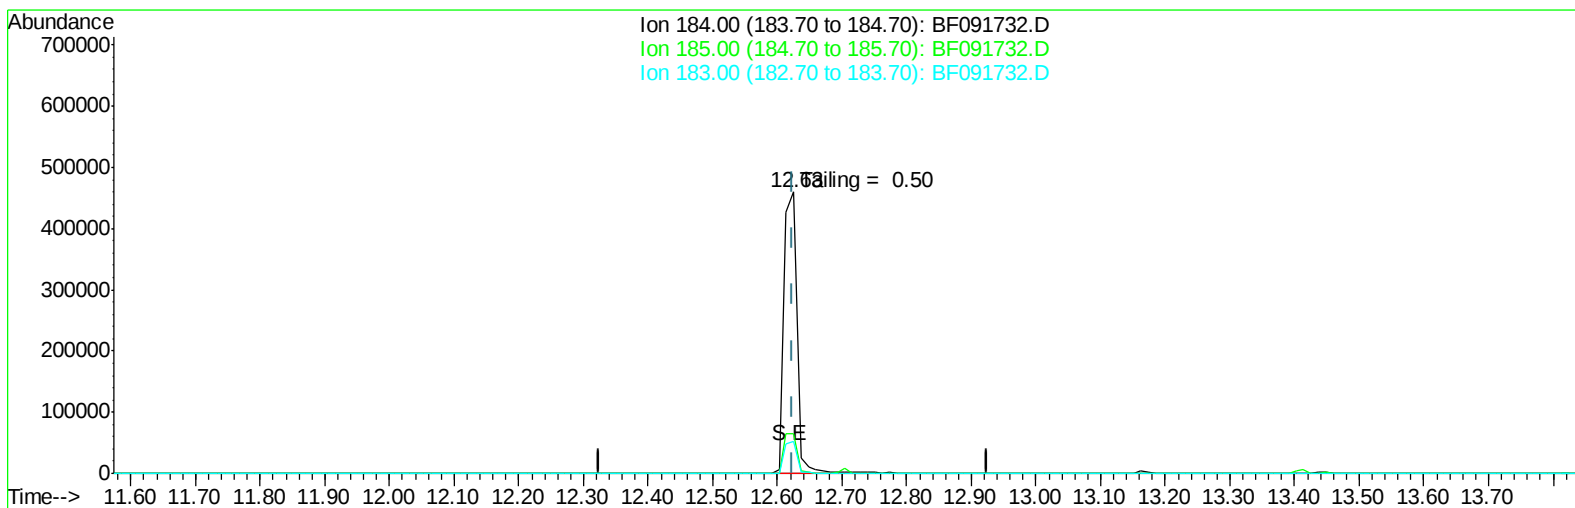

TIC: BF091732.D

(76) Benzidine

12.625min (+0.000) 11574.41ng

response 658682

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.04
183.00	11.50	11.16
0.00	0.00	0.00