
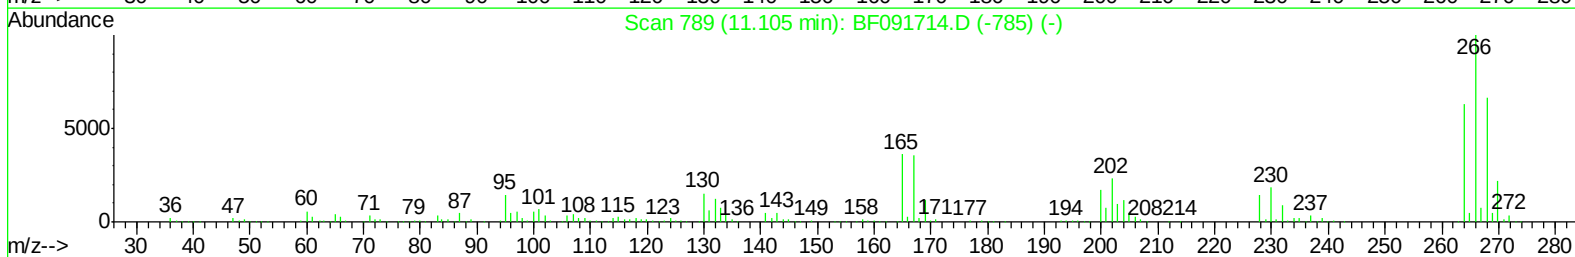
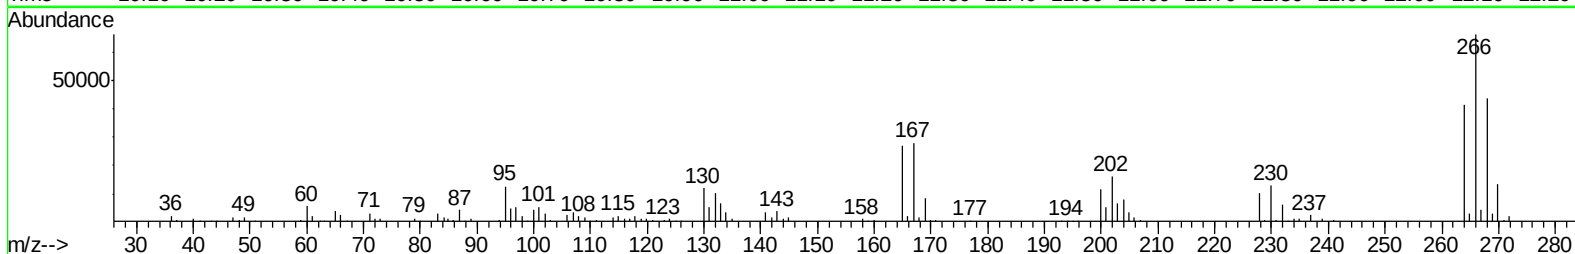


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF121816\
Data File : BF091758.D
Acq On : 19 Dec 2016 1:15
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 19 07:57:48 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 17 22:53:54 2016
Response via : Initial Calibration

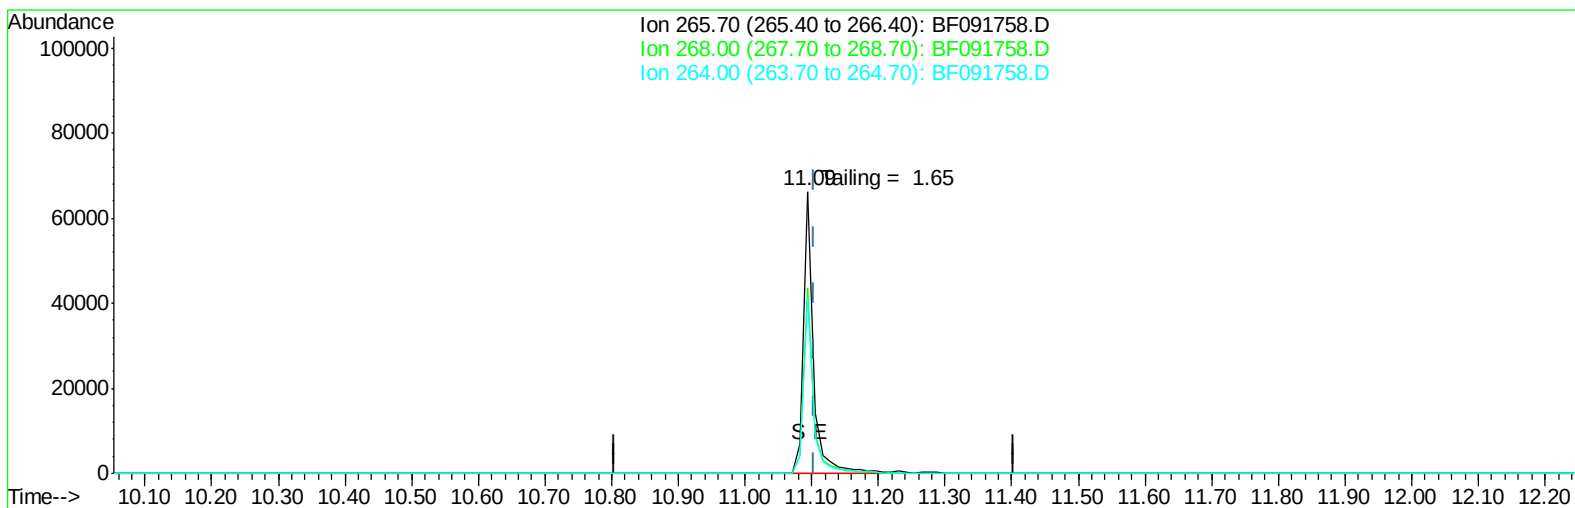

TIC: BF091758.D

(69) Pentachlorophenol (C)




11.093min (-0.011) 17643.61ng

response 69883

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	65.78
264.00	62.90	62.37
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF121816\
Data File : BF091758.D
Acq On : 19 Dec 2016 1:15
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 19 07:57:48 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 17 22:53:54 2016
Response via : Initial Calibration

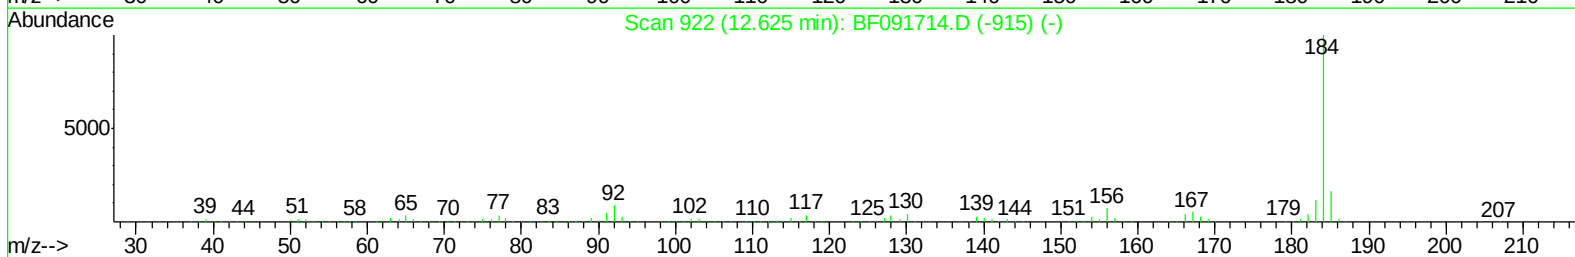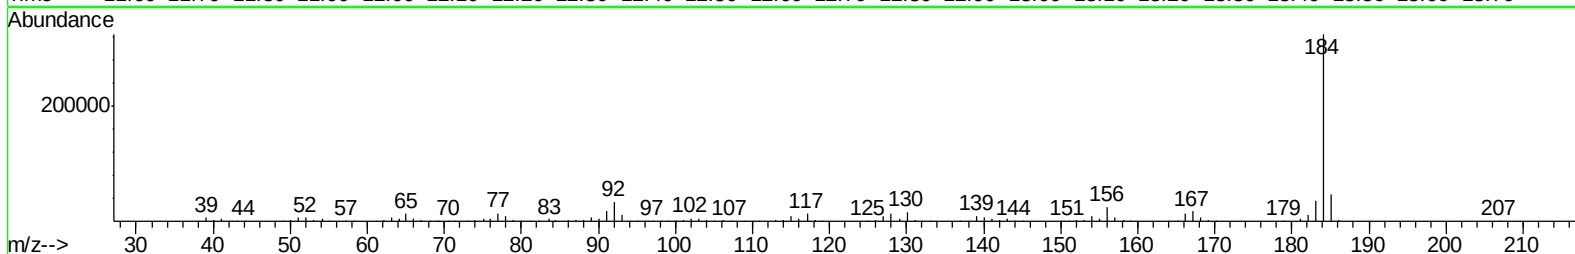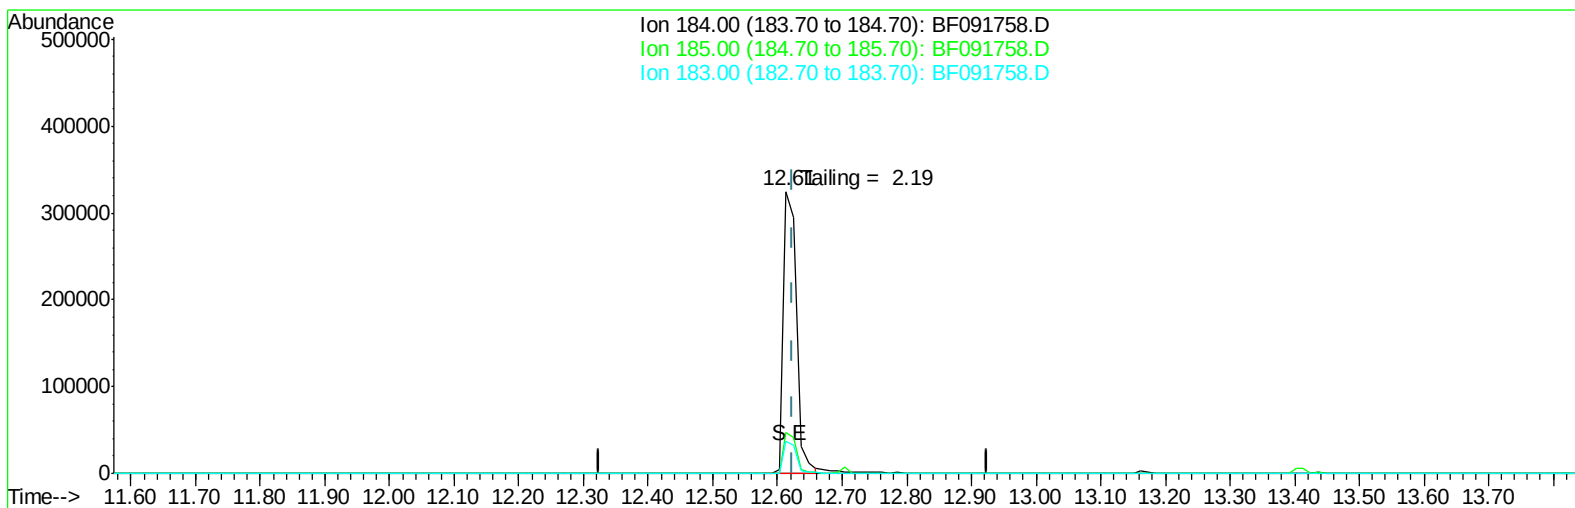

TIC: BF091758.D

(76) Benzidine

12.614min (-0.011) 8145.50ng

response 479492

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.70
183.00	11.50	11.25
0.00	0.00	0.00